

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 15:41
 Operator : AR\AJ
 Sample : P3529-02MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COAA0MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:58:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.930	18422255	112.3E6	21.974	21.342
27)	SA Decachlor...	9.117	8.143	44833033	99569990	25.776	26.496
Target Compounds							
2)	A alpha-BHC	4.034	3.444	89532466	412.7E6	59.154	50.633
3)	MA gamma-BHC...	4.364	3.780	92367516	392.4E6	59.304	50.911
4)	MA Heptachlor	4.964	4.138	99134136	362.7E6	56.799	48.120
5)	MB Aldrin	5.307	4.425	99775923	356.0E6	56.536	48.581
6)	B beta-BHC	4.546	4.073	36411517	170.7E6	50.396	47.455
7)	B delta-BHC	4.795	4.312	96888650	405.1E6	56.105	48.299
8)	B Heptachlo...	5.727	4.930	94831632	324.6E6	55.794	48.650
9)	A Endosulfan I	6.111	5.305	93573180	298.2E6	58.742	50.265m
10)	B trans-Chl...	5.981	5.184	95162140	324.3E6	57.634	50.892
11)	B cis-Chlor...	6.063	5.249	96827369	316.5E6	56.271	50.282
12)	B 4,4'-DDE	6.231	5.434	196.8E6	601.5E6	112.525	98.629
13)	MA Dieldrin	6.384	5.573	213.7E6	617.0E6	118.958	100.291
14)	MA Endrin	6.611	5.851	179.1E6	554.2E6	119.571	100.388
15)	B Endosulfa...	6.822	6.142	184.3E6	518.6E6	111.795	99.883
16)	A 4,4'-DDD	6.740	5.990	149.9E6	498.5E6	116.574	101.603
17)	MA 4,4'-DDT	7.056	6.246	151.9E6	503.4E6	112.025	101.616
18)	B Endrin al...	6.950	6.321	130.3E6	384.2E6	114.638	102.680
19)	B Endosulfa...	7.185	6.545	173.9E6	466.5E6	114.538	99.921
20)	A Methoxychlor	7.527	6.819	446.1E6	1028.9E6	559.376	477.789
21)	B Endrin ke...	7.667	7.056	186.2E6	534.5E6	112.418	102.646

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 15:41
Operator : AR\AJ
Sample : P3529-02MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:58:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

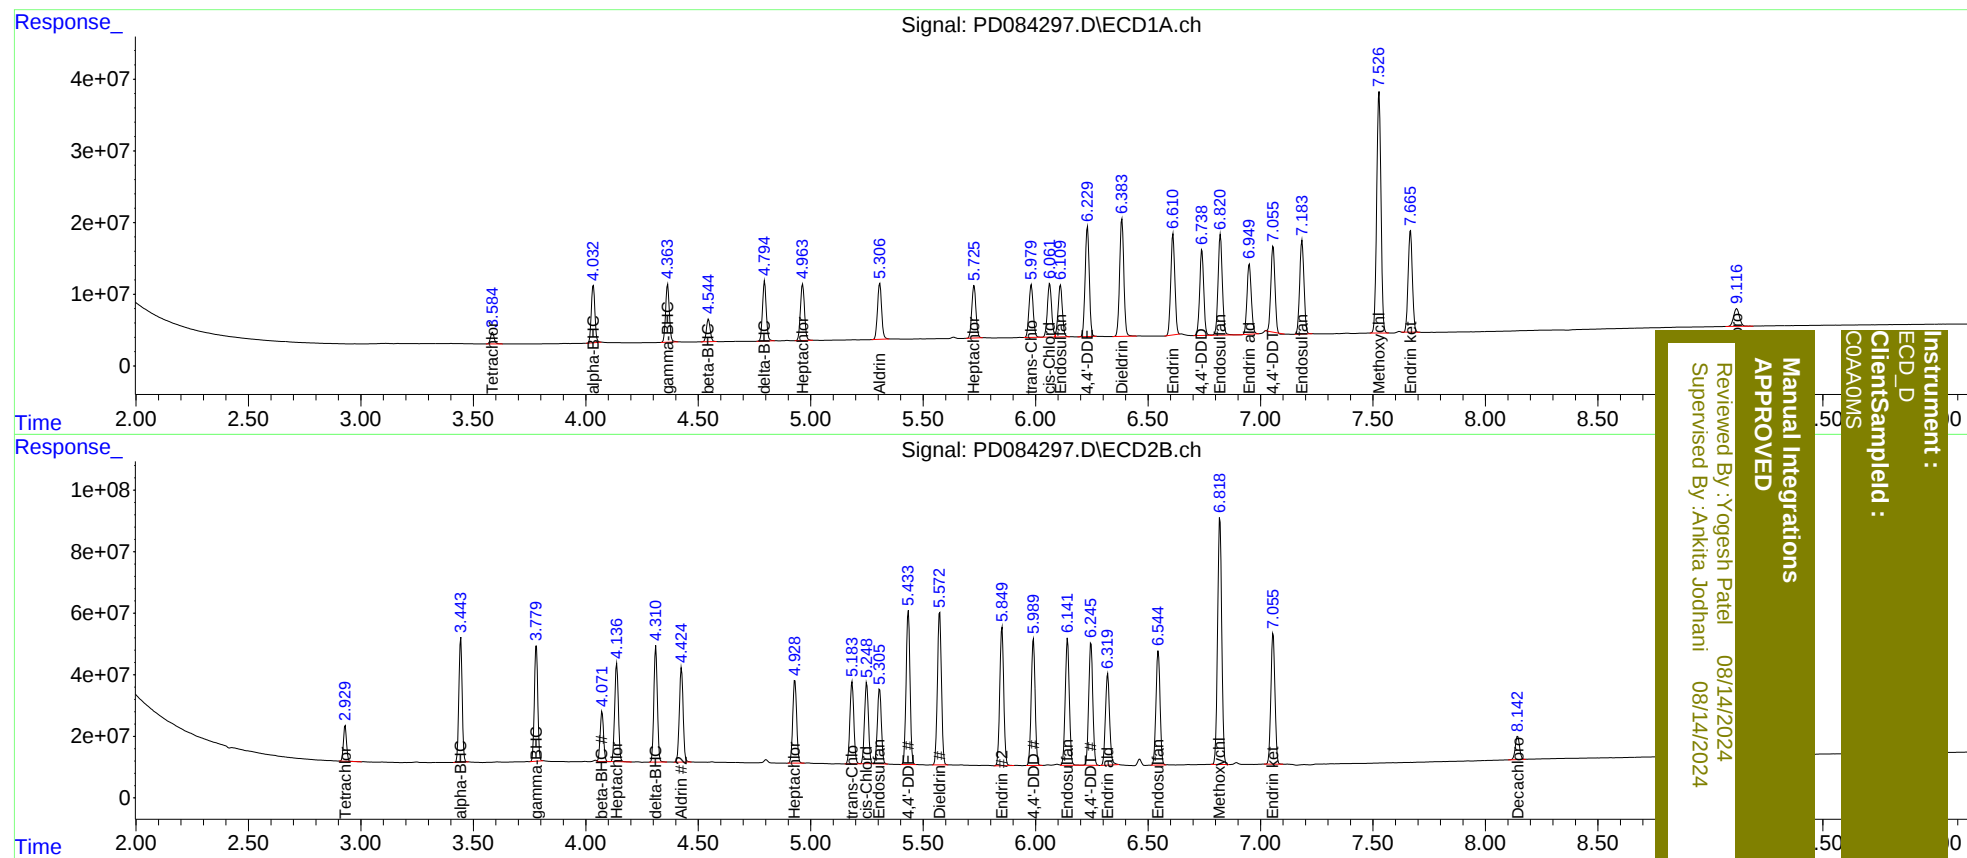

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 08/14/2024
Supervised By : Ankita Jodhani 08/14/2024

Instrument :
ECD_D
Client Sampled :
COAAOMS