

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 15:54
 Operator : AR\AJ
 Sample : P3529-03MSD
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA0MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:58:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.930	18562462	113.2E6	22.141	21.504
27)	SA Decachlor...	9.117	8.142	45260535	101.1E6	26.022	26.912
Target Compounds							
2)	A alpha-BHC	4.033	3.444	91341001	420.2E6	60.349	51.552
3)	MA gamma-BHC...	4.364	3.780	94231278	398.6E6	60.500	51.718
4)	MA Heptachlor	4.964	4.138	101.1E6	369.0E6	57.931	48.956
5)	MB Aldrin	5.307	4.425	102.0E6	363.5E6	57.810	49.601
6)	B beta-BHC	4.545	4.072	37128652	172.9E6	51.388	48.071
7)	B delta-BHC	4.795	4.311	98511393	411.0E6	57.045	49.001
8)	B Heptachlo...	5.726	4.930	96176150	330.9E6	56.586	49.597
9)	A Endosulfan I	6.110	5.305	94966269	302.7E6	59.616	51.013m
10)	B trans-Chl...	5.981	5.184	96916061	330.8E6	58.696	51.919
11)	B cis-Chlor...	6.063	5.249	98222748	322.4E6	57.082	51.222
12)	B 4,4'-DDE	6.230	5.434	200.0E6	611.1E6	114.352	100.204
13)	MA Dieldrin	6.383	5.573	216.8E6	623.5E6	120.655	101.359
14)	MA Endrin	6.611	5.850	181.8E6	564.0E6	121.373	102.167
15)	B Endosulfa...	6.822	6.142	186.4E6	524.6E6	113.041	101.035
16)	A 4,4'-DDD	6.739	5.988	151.6E6	509.5E6	117.902	103.855m
17)	MA 4,4'-DDT	7.054	6.245	156.0E6	512.2E6	115.081m	103.397m
18)	B Endrin al...	6.950	6.321	132.2E6	390.2E6	116.299	104.287
19)	B Endosulfa...	7.185	6.545	176.1E6	471.5E6	115.999	100.995
20)	A Methoxychlor	7.527	6.819	451.8E6	1045.4E6	566.503	485.443
21)	B Endrin ke...	7.667	7.056	188.7E6	541.6E6	113.963	104.004

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 15:54
Operator : AR\AJ
Sample : P3529-03MSD
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:58:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

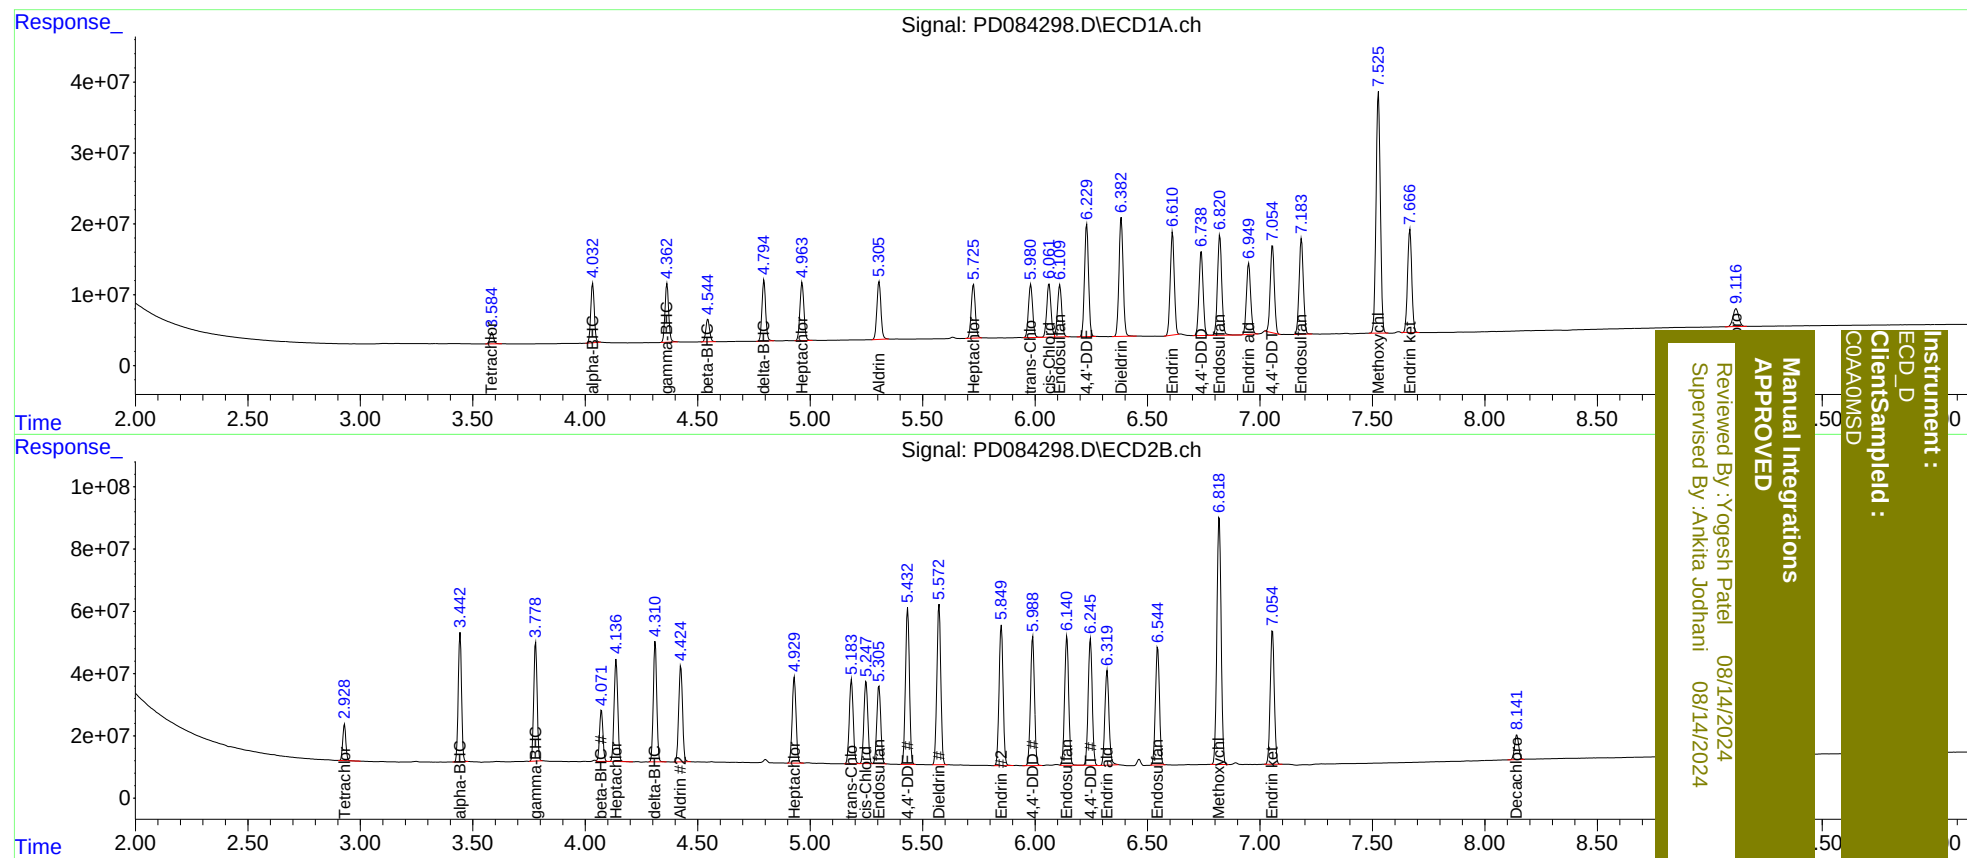

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 08/14/2024
Supervised By : Ankita Jodhani 08/14/2024

Instrument :
ECD_D
Client Sampled :
COAA0MSD