

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 18:21
 Operator : AR\AJ
 Sample : P3439-03MSDRX
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVW9MSDRX

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/22/2024
 Supervised By :Ankita Jodhani 08/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:01:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.567	2.925	69889871	19002248	83.364m	3.610m#
2) SA Decachlor...	9.102	8.159	10587005	83787266	6.087m	22.296m#
Target Compounds						
2) A alpha-BHC	4.034	3.444	200.5E6	535.5E6	132.468	65.698 #
3) MA gamma-BHC...	4.307f	3.779	104077.4E6	716.7E6	66821.835m	92.998m#
4) MA Heptachlor	4.964	4.137	84158725	104.6E6	48.219m	13.878m#
5) MB Aldrin	5.308	4.426	137.9E6	340.5E6	78.143	46.455 #
6) B beta-BHC	4.555	4.072	27645040	29054094	38.263m	8.079m#
7) B delta-BHC	4.794	4.311	229.0E6	642.6E6	132.624m	76.610 #
8) B Heptachlo...	5.729	4.929	102.2E6	311.2E6	60.130	46.635
9) A Endosulfan I	6.105	5.305	138.8E6	320.7E6	87.149m	54.049m#
10) B trans-Chl...	5.980	5.179	298.5E6	264.5E6	180.753m	41.514m#
11) B cis-Chlor...	6.066	5.254	14945901	224.1E6	8.686m	35.614 #
12) B 4,4'-DDE	6.228	5.435	248.8E6	588.3E6	142.230m	96.470m#
13) MA Dieldrin	6.384	5.573	334.8E6	511.0E6	186.375m	83.068m#
14) MA Endrin	6.610	5.848	88335548	681.9E6	58.968m	123.520 #
15) B Endosulfa...	6.819	6.145	340.8E6	422.6E6	206.722m	81.391m#
16) A 4,4'-DDD	6.738	5.986	349.5E6	66913902	271.738m	13.639m#
17) MA 4,4'-DDT	7.053	6.229	450.9E6	2470.0E6	332.606m	498.612m#
18) B Endrin al...	6.955	6.319	330.2E6	376.6E6	290.531m	100.665m#
19) B Endosulfa...	7.183	6.544	137.1E6	275.9E6	90.299m	59.090m#
20) A Methoxychlor	7.526	6.819	395.4E6	557.2E6	495.839	258.739 #
21) B Endrin ke...	7.666	7.055	206.4E6	301.2E6	124.603	57.845 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084309.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 18:21
Operator : AR\AJ
Sample : P3439-03MSDRX
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:01:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

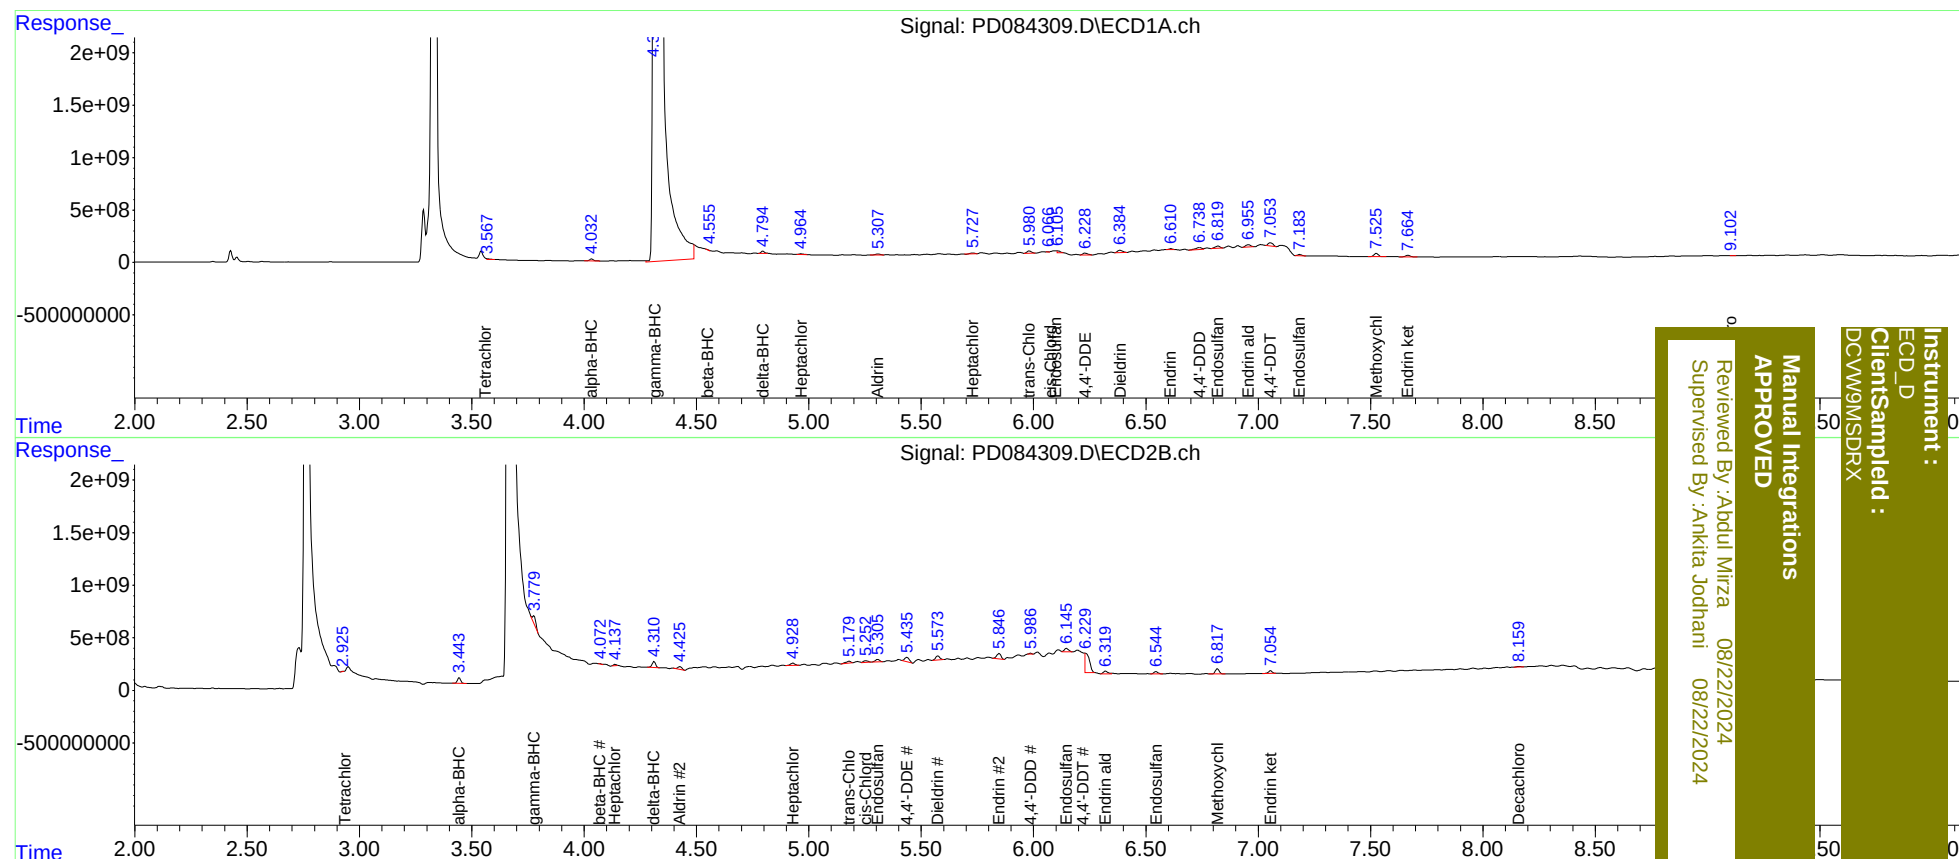

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/22/2024
Supervised By: Ankita Jodhani 08/22/2024

Instrument :
ECD_D
Client Sampled :
DCW/MSDRX