

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081323\
 Data File : PD077131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 00:56
 Operator : AR\AJ
 Sample : 03971-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DUP-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:34:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	27741486	16473356	11.723	12.094
28)	SA Decachlor...	9.084	7.902	37934276	17586562	13.844	12.289
Target Compounds							
7)	B delta-BHC	4.769	0.000	2139363	0	0.613	N.D. #
8)	B Heptachlo...	5.690	0.000	1046218	0	0.316	N.D. #
9)	A Endosulfan I	6.113f	0.000	314573	0	0.104	N.D. #
11)	B alpha-Chl...	6.033	0.000	265702	0	0.081	N.D. #
14)	MA Endrin	0.000	5.643f	0	312212	N.D.	0.213 #
15)	B Endosulfa...	6.784f	0.000	190729	0	0.060	N.D. #
21)	B Endrin ke...	7.631f	0.000	263481	0	0.087	N.D. #
26)	Chlordane-4	6.033	0.000	265702	0	0.459	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081323\
Data File : PD077131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 00:56
Operator : AR\AJ
Sample : 03971-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
DUP-05

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:34:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

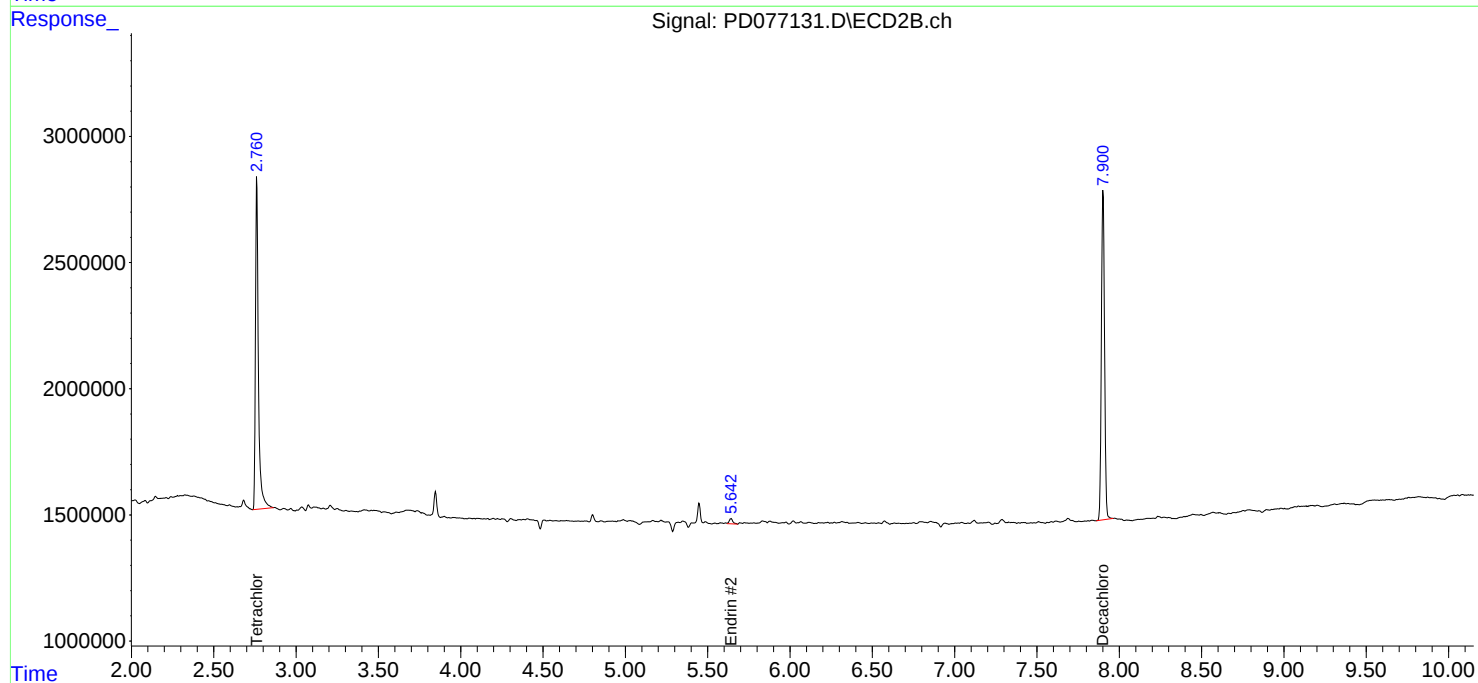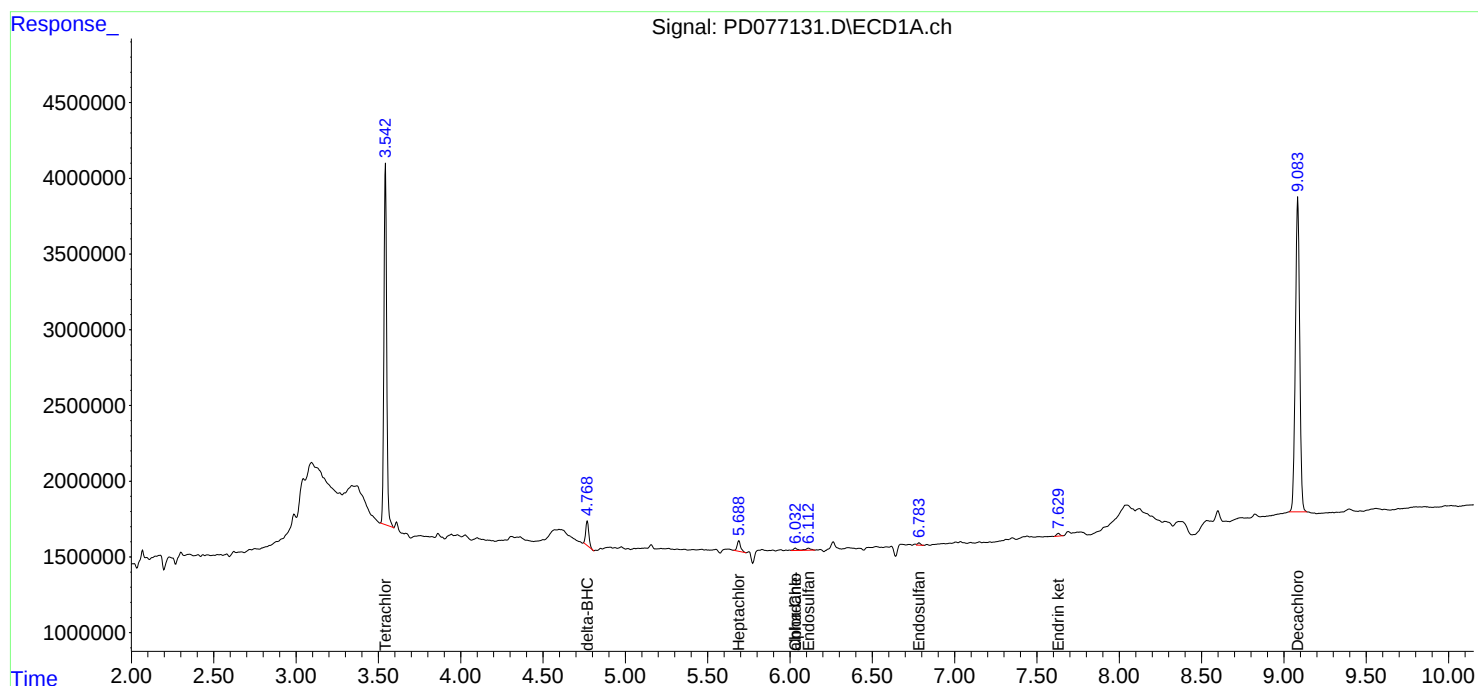


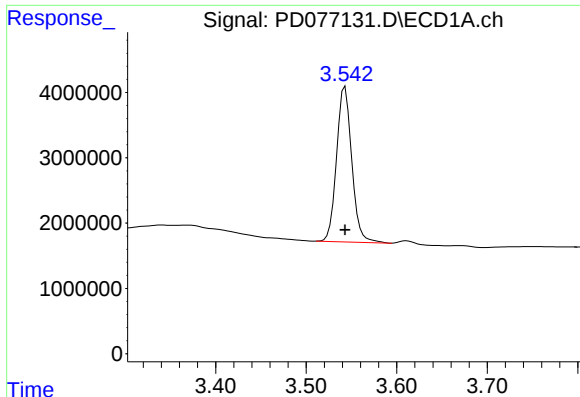

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 27741486
Conc: 11.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-05

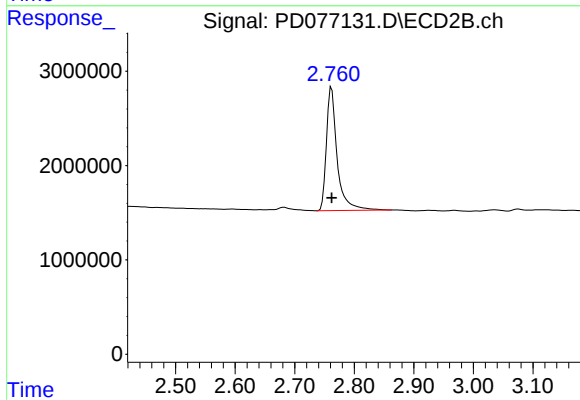


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 16473356
Conc: 12.09 ng/ml

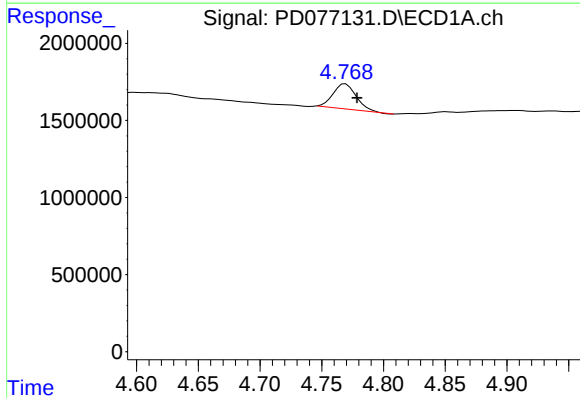


#7 delta-BHC

R.T.: 4.769 min
Delta R.T.: -0.009 min
Response: 2139363
Conc: 0.61 ng/ml

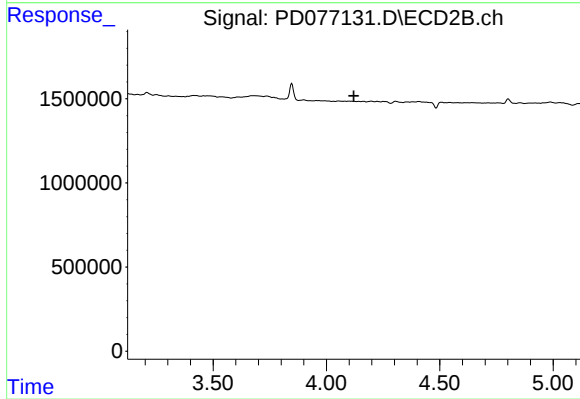

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.120 min
Response: 0
Conc: N.D.

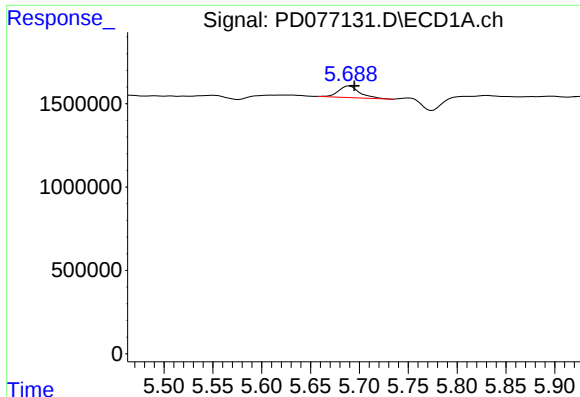

#8 Heptachlor epoxide


R.T.: 5.690 min
Delta R.T.: -0.005 min
Response: 1046218
Conc: 0.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-05

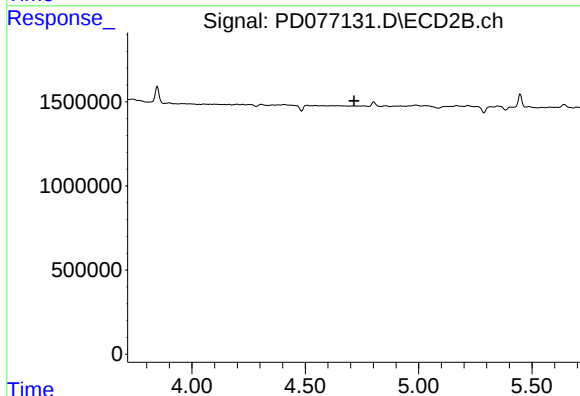


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

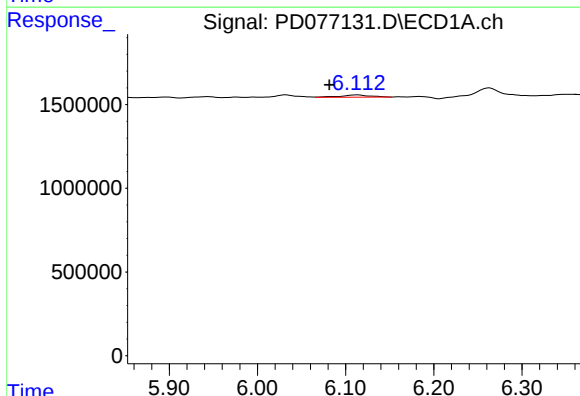


#9 Endosulfan I

R.T.: 6.113 min
Delta R.T.: 0.031 min
Response: 314573
Conc: 0.10 ng/ml

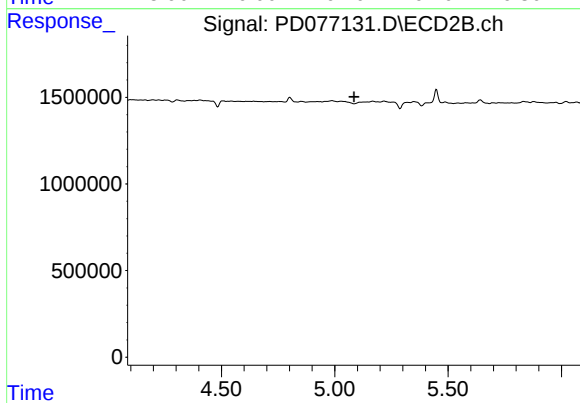

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.086 min
Response: 0
Conc: N.D.

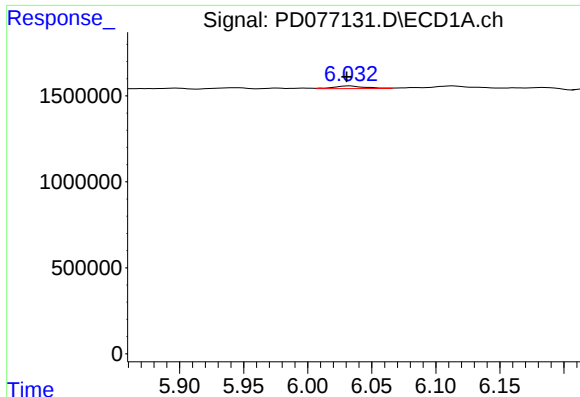

#11 alpha-Chlordane


R.T.: 6.033 min
Delta R.T.: 0.002 min
Response: 265702
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-05

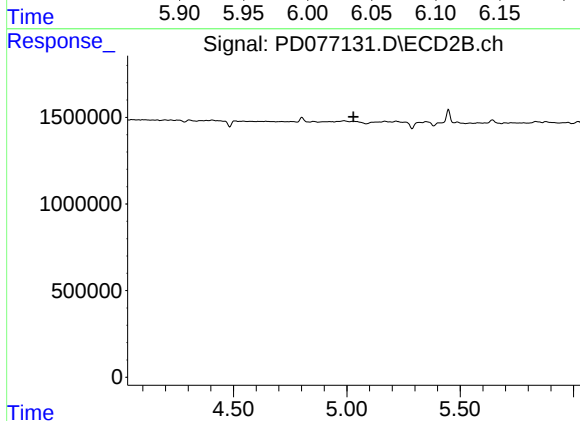


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.030 min
Response: 0
Conc: N.D.

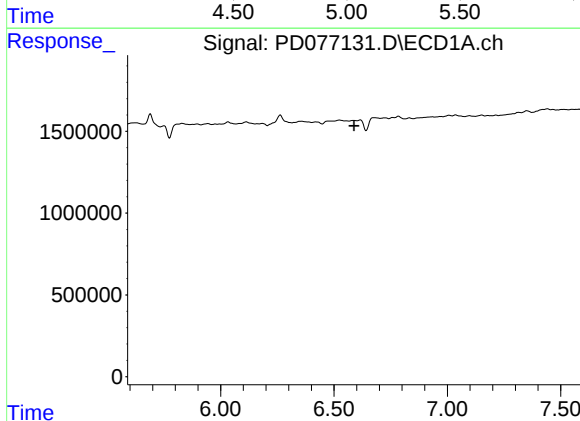


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.588 min
Response: 0
Conc: N.D.

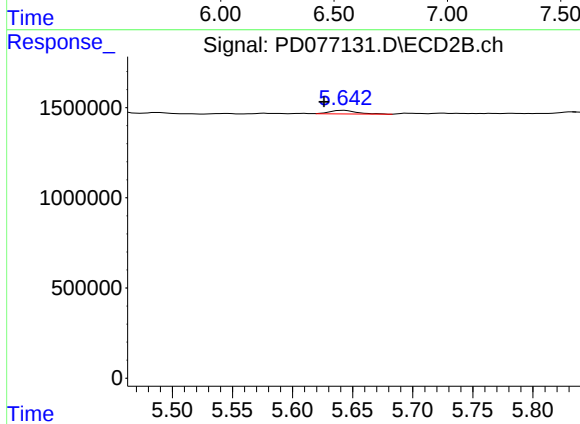

#14 Endrin


R.T.: 5.643 min
Delta R.T.: 0.017 min
Response: 312212
Conc: 0.21 ng/ml

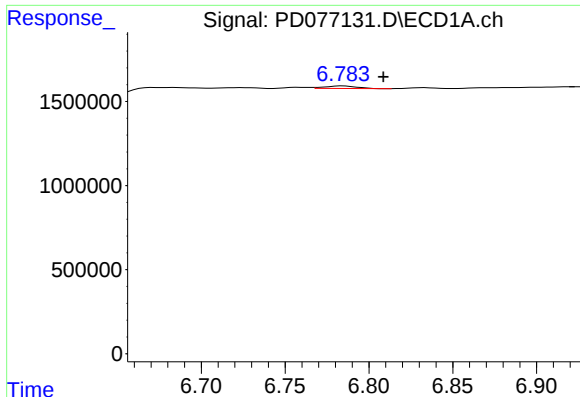

#15 Endosulfan II


R.T.: 6.784 min
Delta R.T.: -0.024 min
Response: 190729
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-05

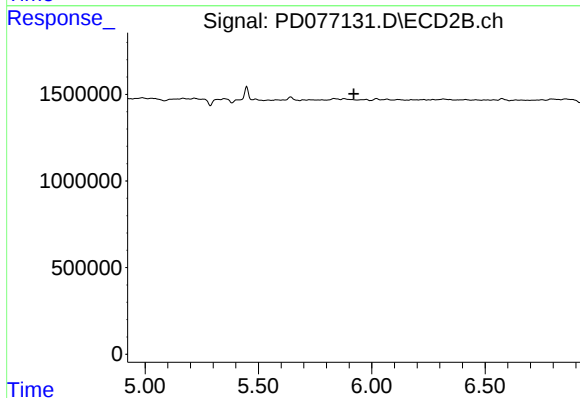


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

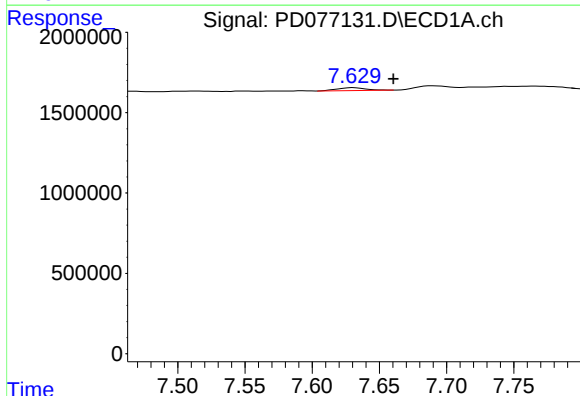


#21 Endrin ketone

R.T.: 7.631 min
Delta R.T.: -0.030 min
Response: 263481
Conc: 0.09 ng/ml

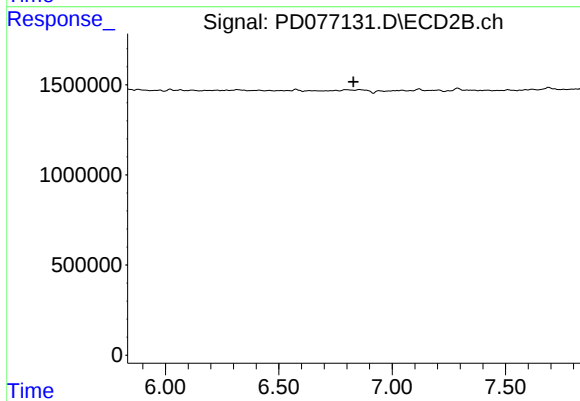

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

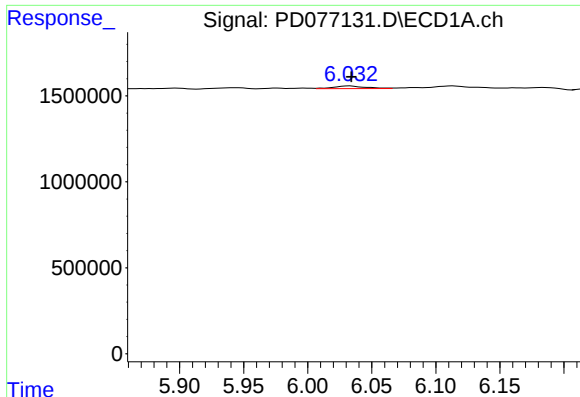

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: -0.001 min
Response: 265702
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-05

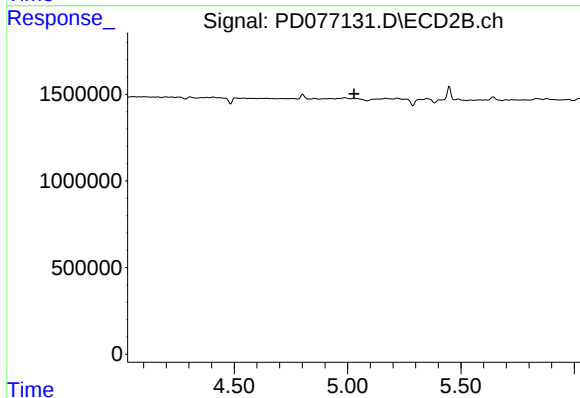


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.029 min
Response: 0
Conc: N.D.

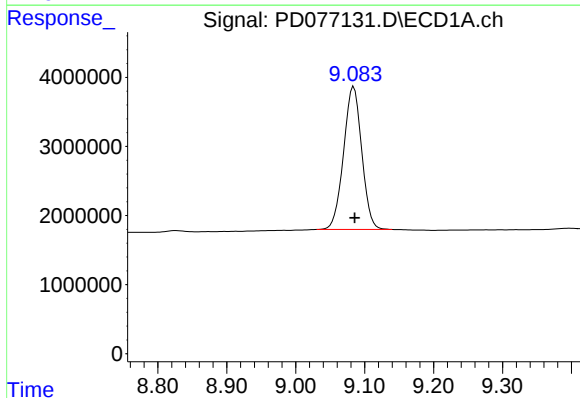

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.002 min
Response: 37934276
Conc: 13.84 ng/ml

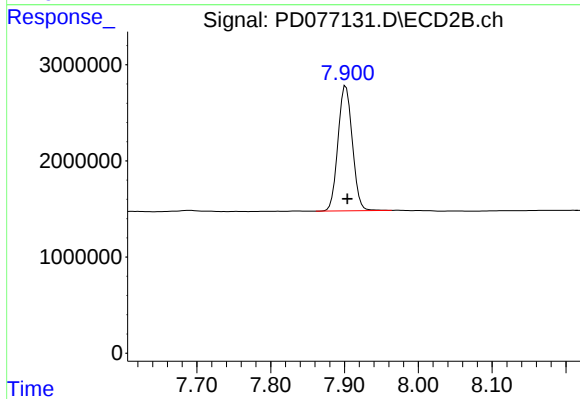

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.002 min
Response: 17586562
Conc: 12.29 ng/ml