

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081323\
 Data File : PD077122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2023 22:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/14/2023
 Supervised By : Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:13:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.778	58159568	32171894	24.576	23.619m
28)	SA Decachlor...	9.088	7.919	70595456	33500040	25.763	23.409m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081323\
Data File : PD077122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2023 22:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/14/2023
Supervised By : Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:13:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

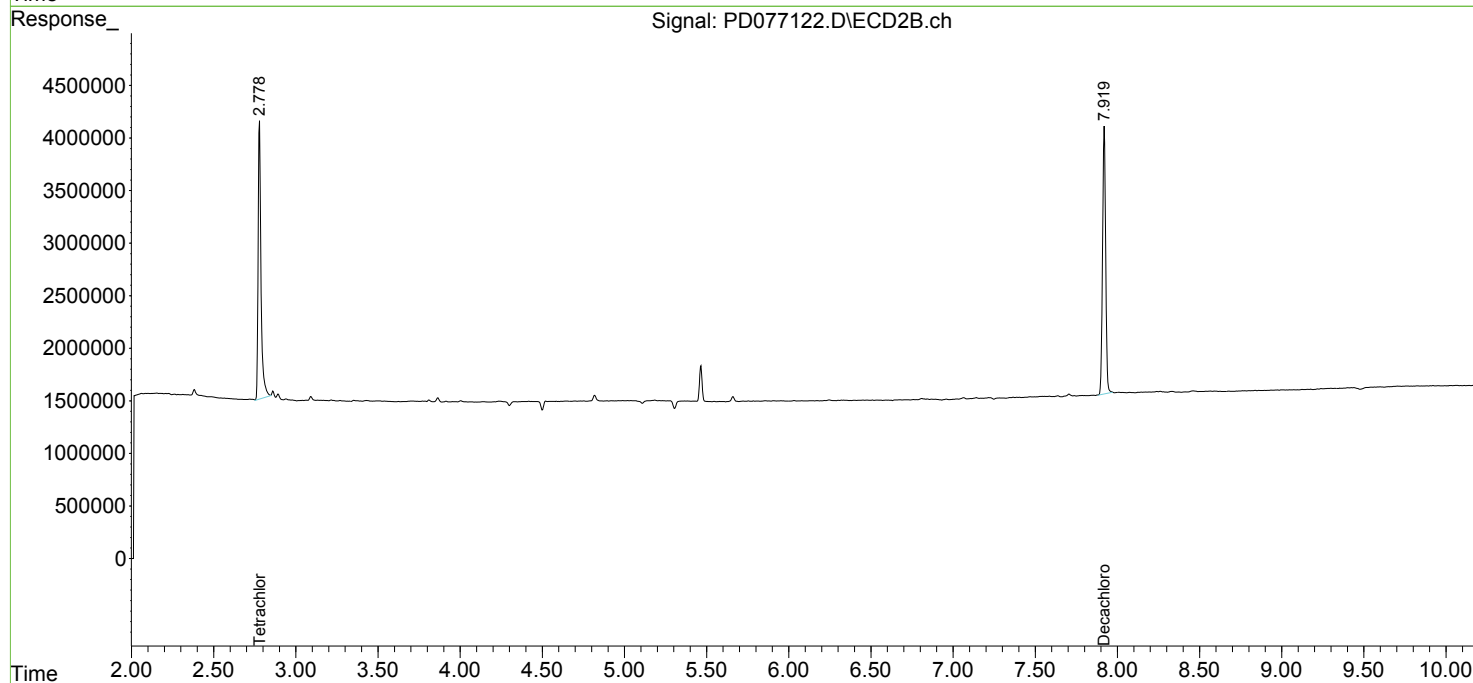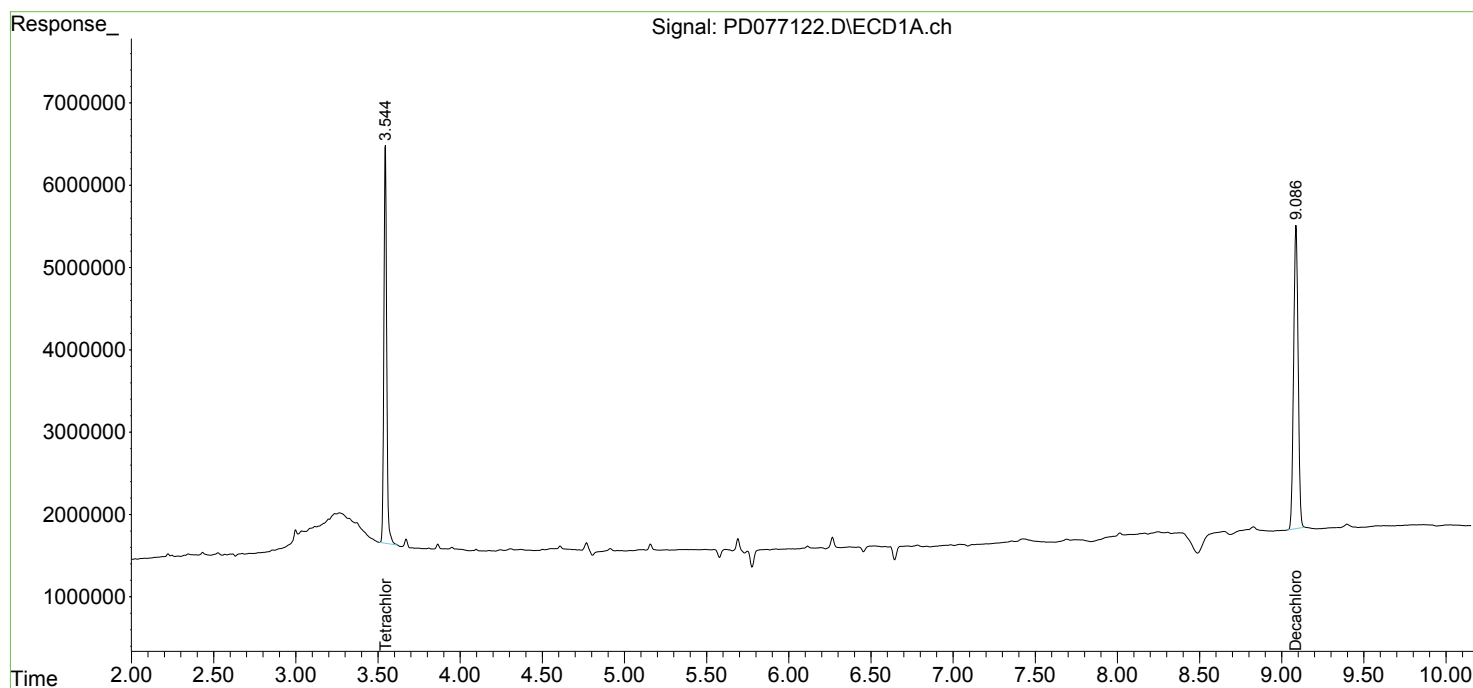

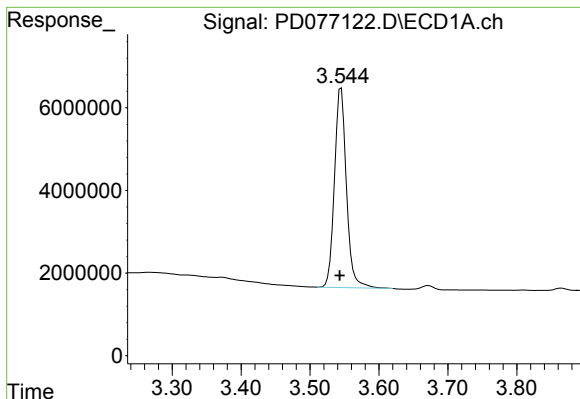


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.002 min
Response: 58159568
Conc: 24.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/14/2023
Supervised By :Ankita Jodhani 08/14/2023

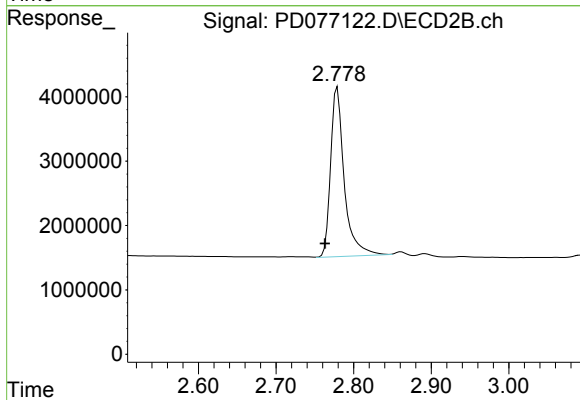


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.015 min
Response: 32171894
Conc: 23.62 ng/ml m

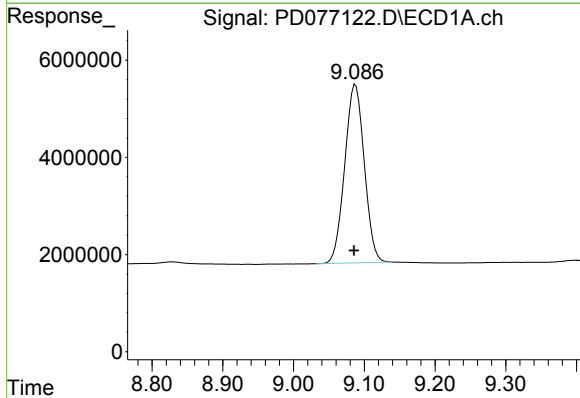

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.002 min
Response: 70595456
Conc: 25.76 ng/ml

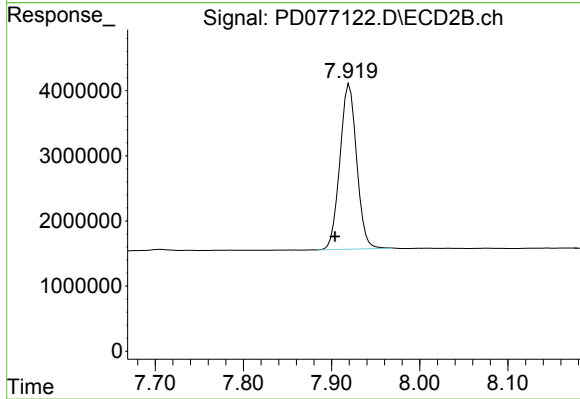

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: 0.015 min
Response: 33500040
Conc: 23.41 ng/ml m