

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081323\
 Data File : PD077132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 01:10
 Operator : AR\AJ
 Sample : 03971-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B-PP03A

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/14/2023
 Supervised By : Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:35:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	24452483	14613975	10.333	10.729
28)	SA Decachlor...	9.084	7.903	32302629	15905743	11.789	11.114
Target Compounds							
12)	B 4,4'-DDE	6.202	5.217	1769232	887184	0.596	0.612m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081323\
Data File : PD077132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 01:10
Operator : AR\AJ
Sample : 03971-08
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
B-PP03A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/14/2023
Supervised By : Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:35:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

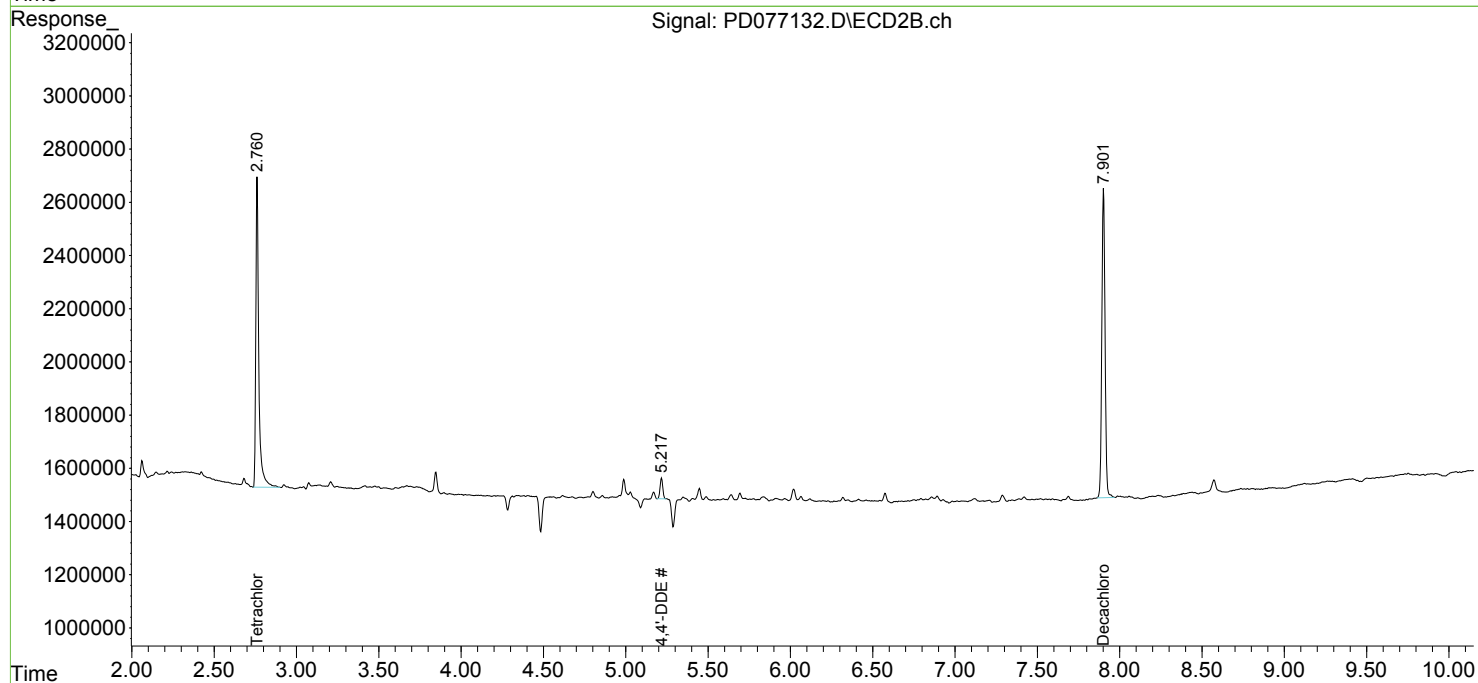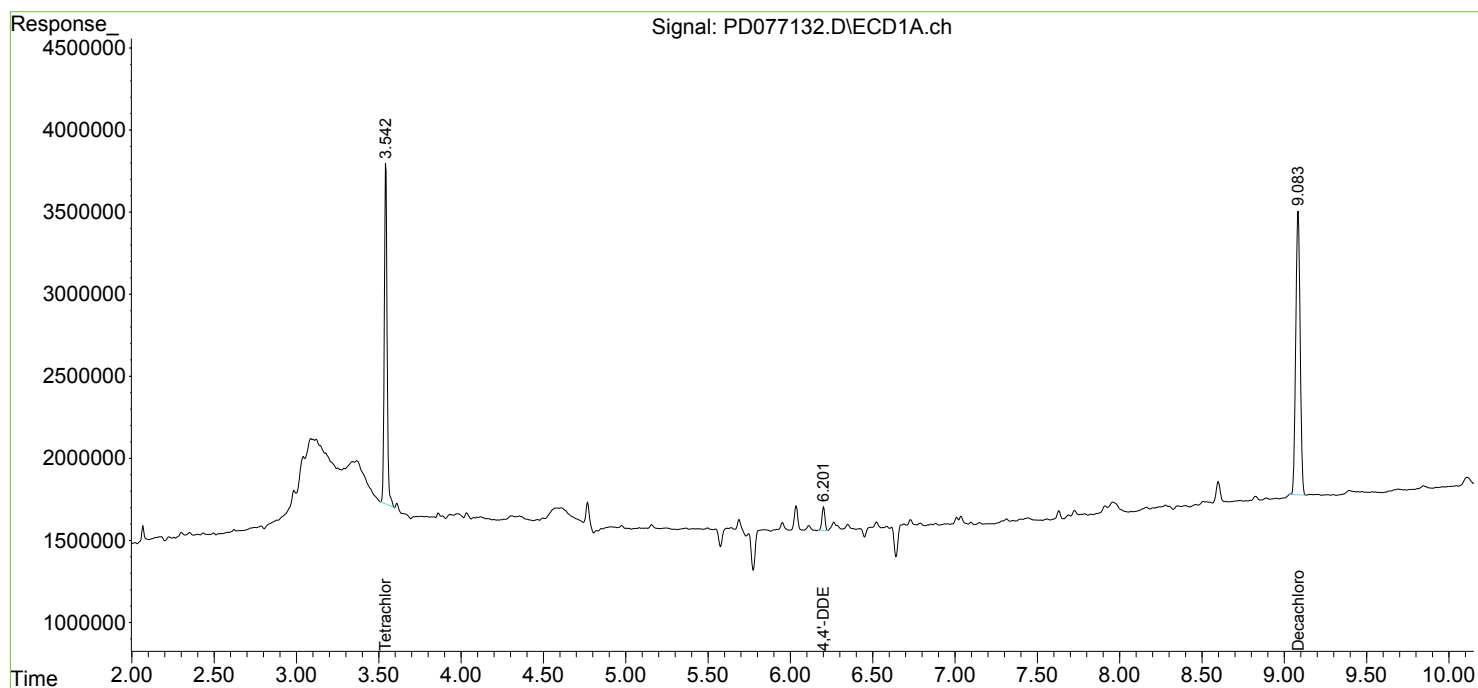

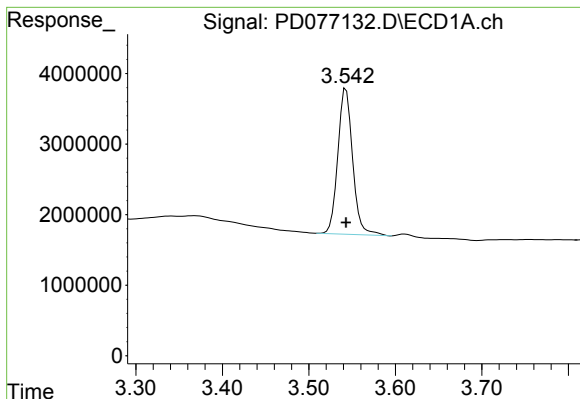


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 24452483
Conc: 10.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
B-PP03A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/14/2023
Supervised By :Ankita Jodhani 08/14/2023

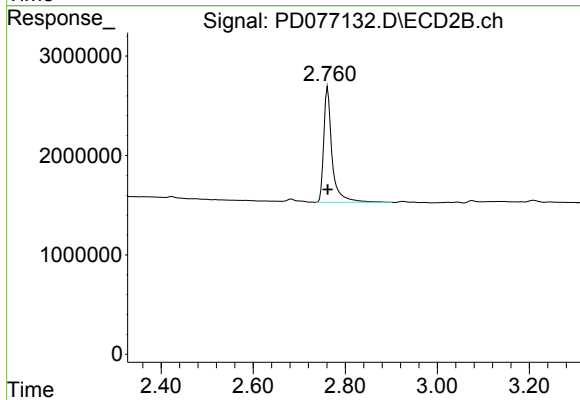


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 14613975
Conc: 10.73 ng/ml

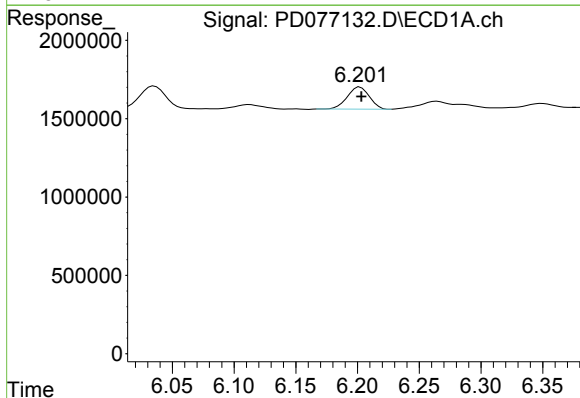


#12 4,4'-DDE

R.T.: 6.202 min
Delta R.T.: -0.001 min
Response: 1769232
Conc: 0.60 ng/ml

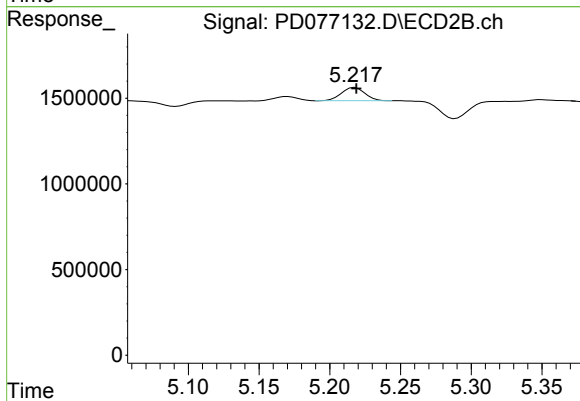

#12 4,4'-DDE

R.T.: 5.217 min
Delta R.T.: -0.002 min
Response: 887184
Conc: 0.61 ng/ml m

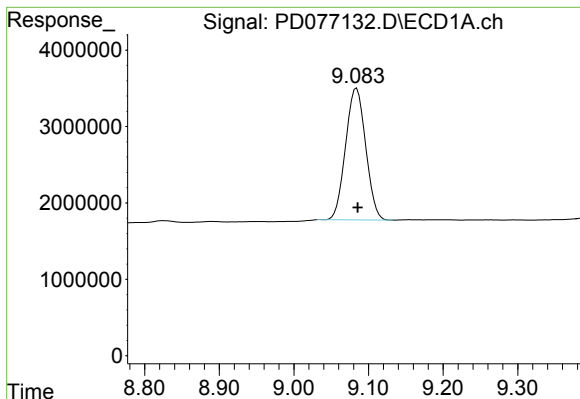

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.002 min
Response: 32302629
Conc: 11.79 ng/ml

Instrument :

ECD_D

ClientSampleId :


B-PP03A

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 08/14/2023

Supervised By :Ankita Jodhani 08/14/2023

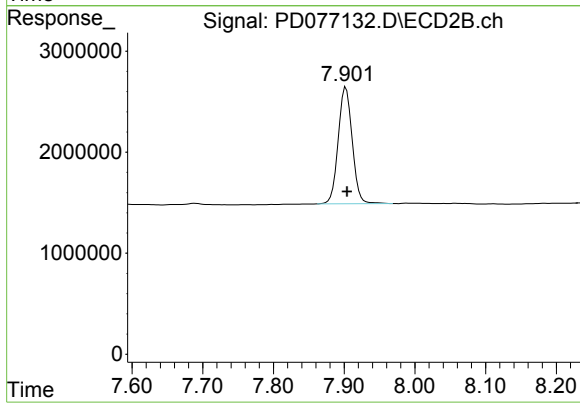

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: -0.001 min
Response: 15905743
Conc: 11.11 ng/ml