

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081323\
 Data File : PD077143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 03:48
 Operator : AR\AJ
 Sample : 03958-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 NEVINS-SB02-Z37-39

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/14/2023
 Supervised By : Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 04:35:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.774	38459719	20843662	16.252m	15.302m
2)	SA Decachlor...	9.083	7.916	39394670	19593337	14.377	13.691

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081323\
Data File : PD077143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 03:48
Operator : AR\AJ
Sample : 03958-05
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
NEVINS-SB02-Z37-39


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/14/2023
Supervised By : Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 04:35:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

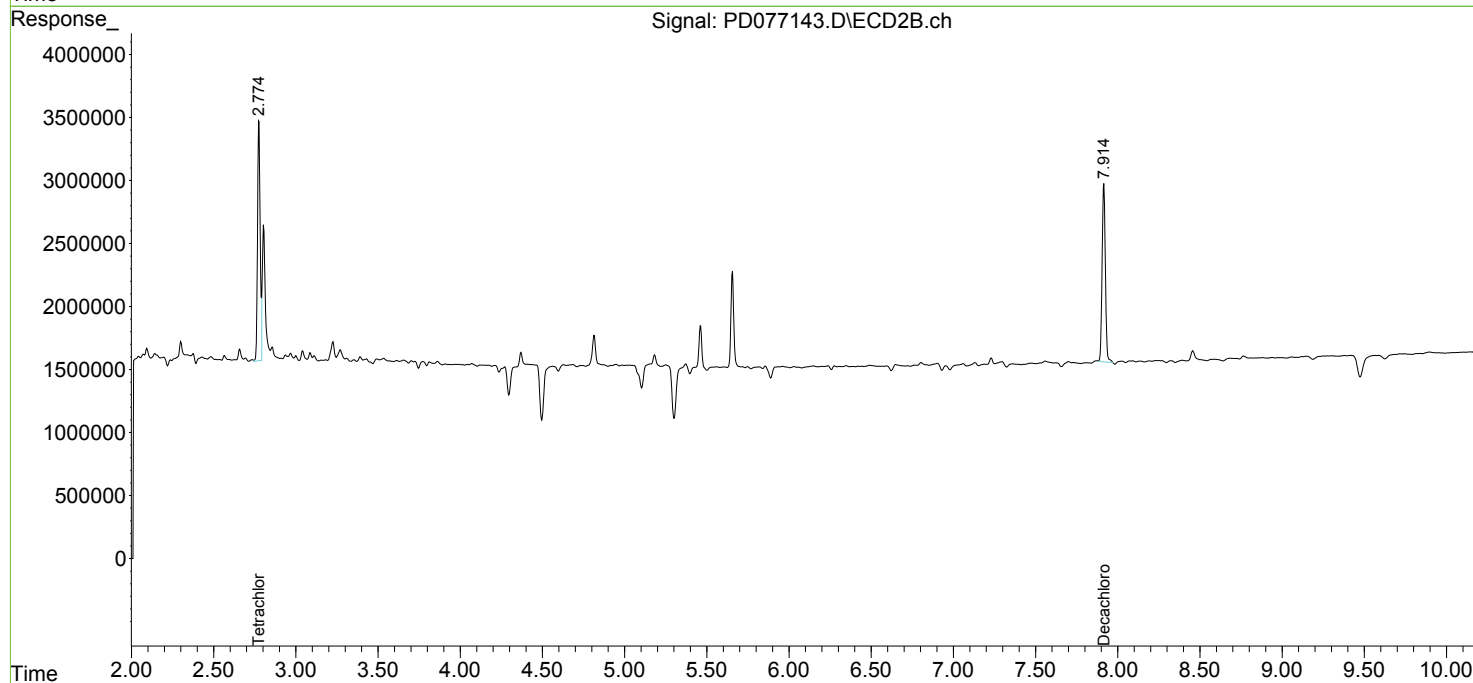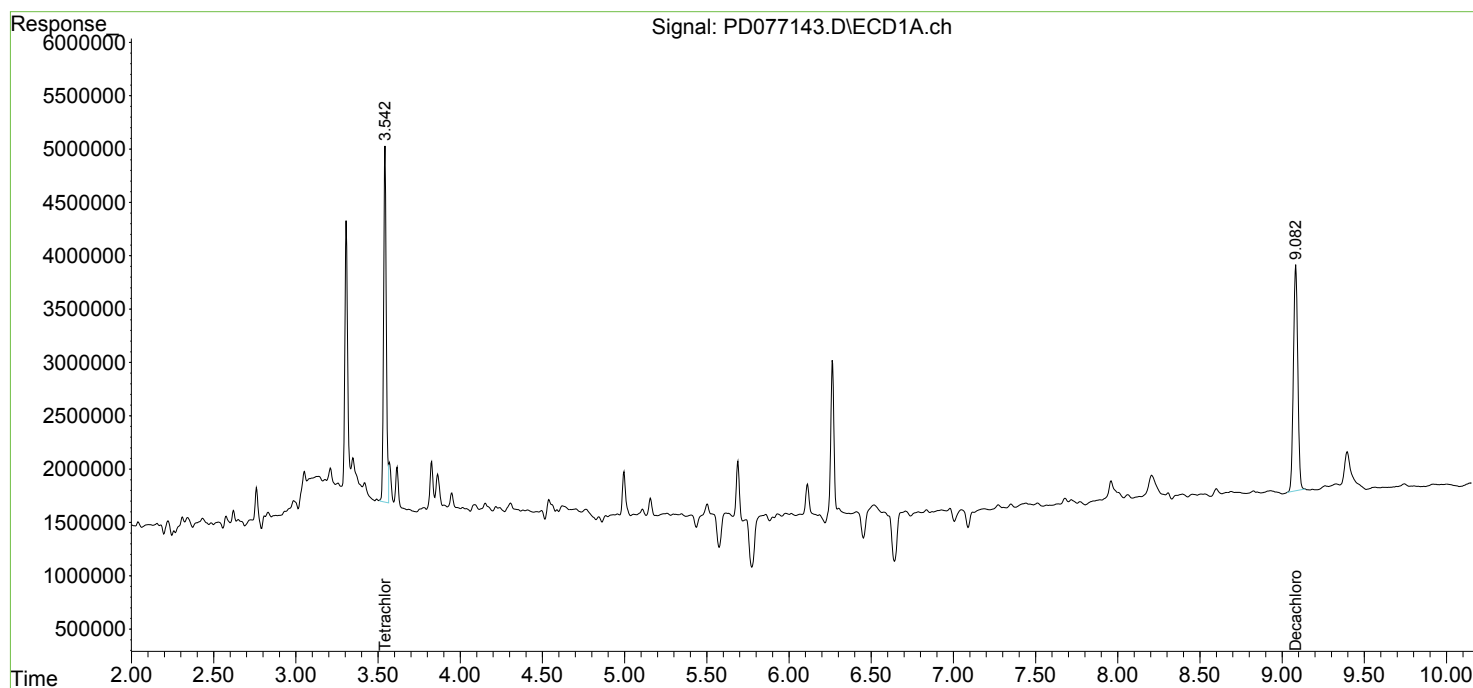

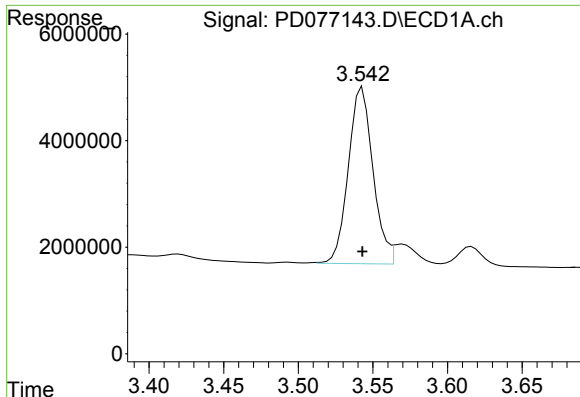

#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.001 min
Response: 38459719
Conc: 16.25 ng/ml

Instrument :

ECD_D


ClientSampleId :

NEVINS-SB02-Z37-39

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 08/14/2023
Supervised By :Ankita Jodhani 08/14/2023

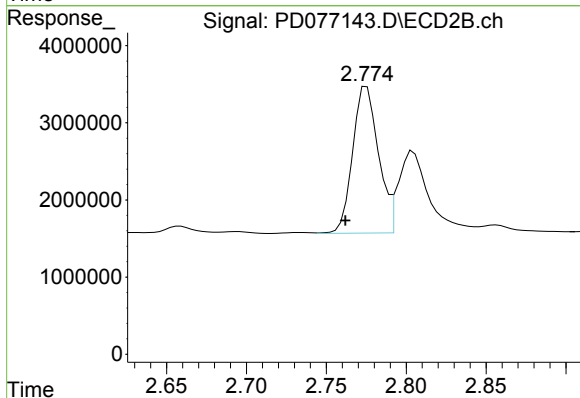


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.012 min
Response: 20843662
Conc: 15.30 ng/ml m

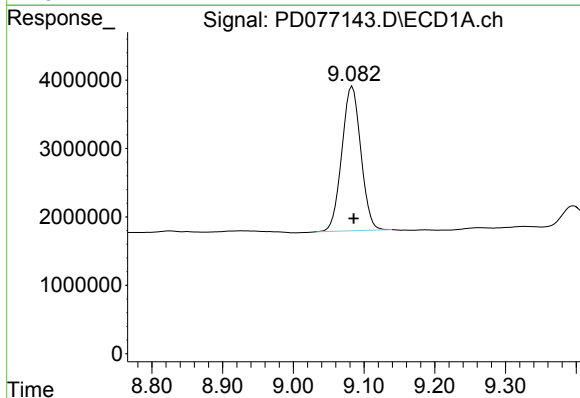

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.002 min
Response: 39394670
Conc: 14.38 ng/ml

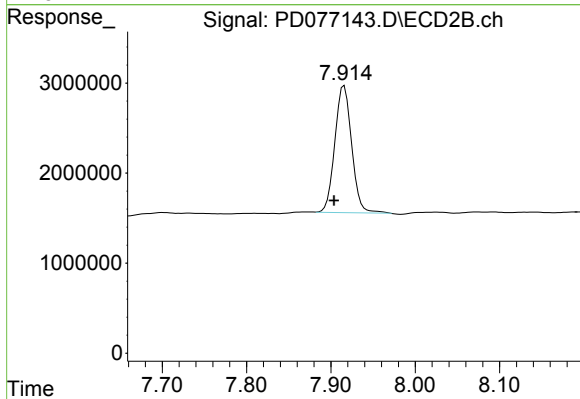

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.012 min
Response: 19593337
Conc: 13.69 ng/ml