

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
 Data File : PD077572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 15:08
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 16:11:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 01 16:06:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.760	116.4E6	86385384	50.000	50.000
28)	SA Decachlor...	9.083	7.901	139.9E6	79741682	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.707	3.757	56283356	27972787	500.000	500.000
24)	Chlordane-2	5.239	4.333	60876109	31020008	500.000	500.000
25)	Chlordane-3	5.952	4.963	247.0E6	97433453	500.000	500.000
26)	Chlordane-4	6.033	5.026	301.8E6	93139505	500.000	500.000
27)	Chlordane-5	6.886	5.923	49935424	32384461	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
Data File : PD077572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 15:08
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 16:11:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
Quant Title : GC Extractables
QLast Update : Fri Sep 01 16:06:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

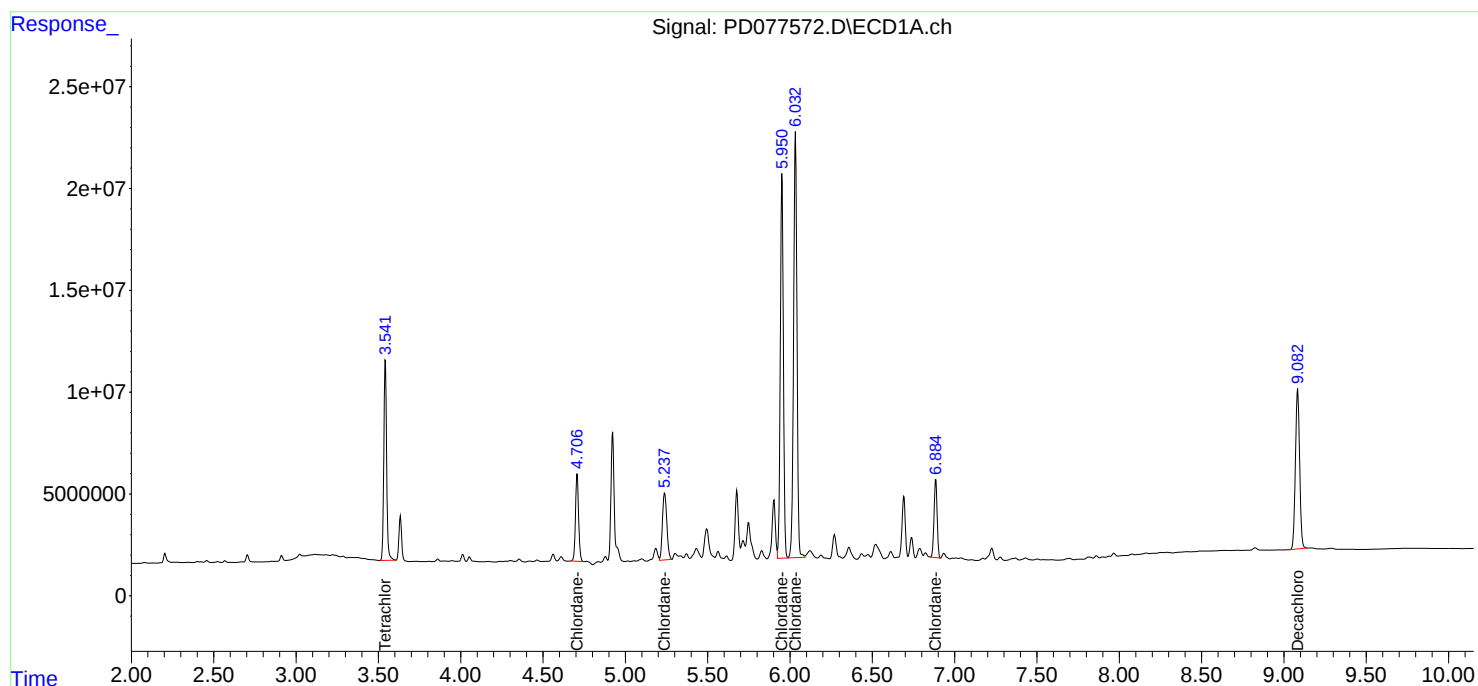


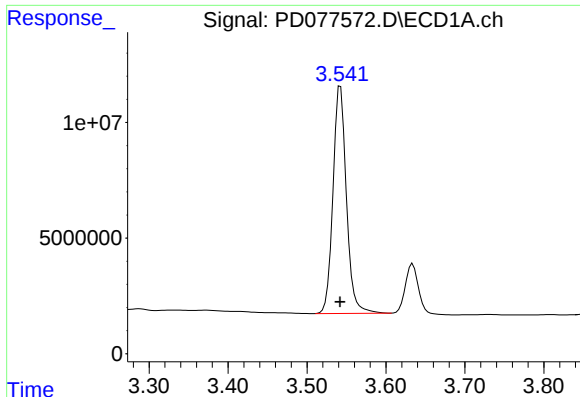

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 116440931
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

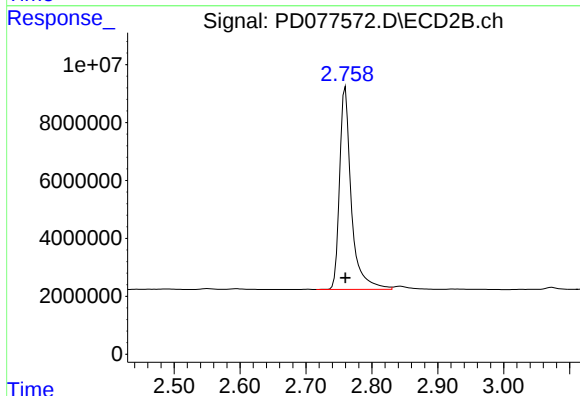


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 86385384
Conc: 50.00 ng/ml

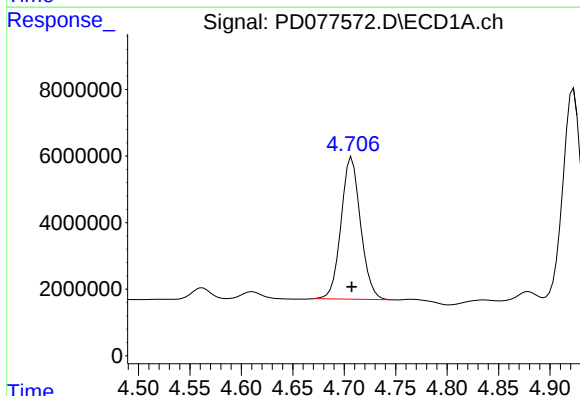


#23 Chlordane-1

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 56283356
Conc: 500.00 ng/ml

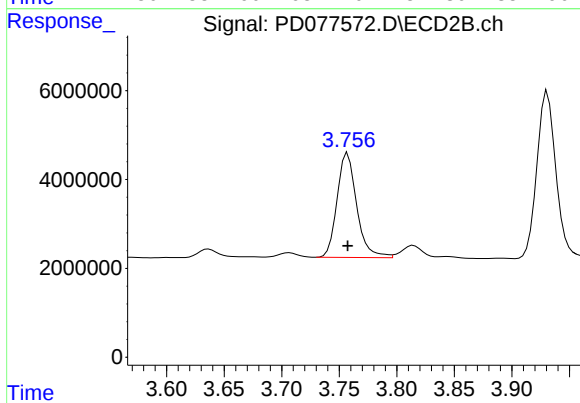

#23 Chlordane-1


R.T.: 3.757 min
Delta R.T.: 0.000 min
Response: 27972787
Conc: 500.00 ng/ml

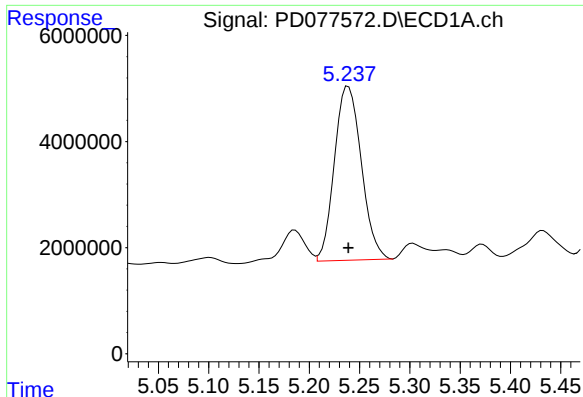

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 60876109
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

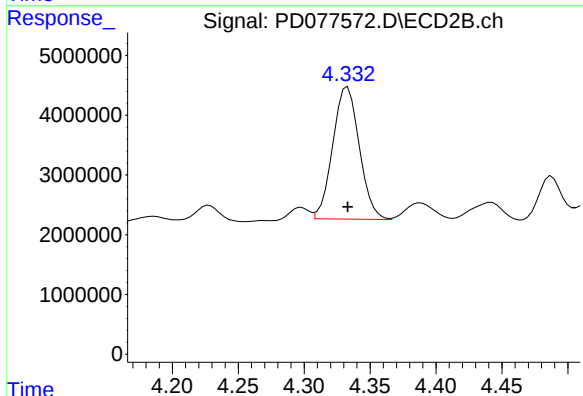


#24 Chlordane-2

R.T.: 4.333 min
Delta R.T.: 0.000 min
Response: 31020008
Conc: 500.00 ng/ml

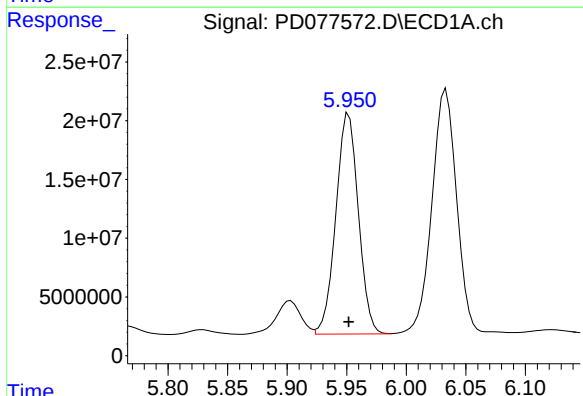


#25 Chlordane-3

R.T.: 5.952 min
Delta R.T.: 0.000 min
Response: 246996101
Conc: 500.00 ng/ml

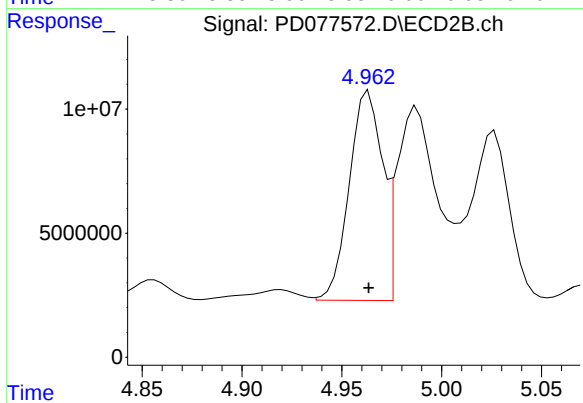

#25 Chlordane-3


R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 97433453
Conc: 500.00 ng/ml

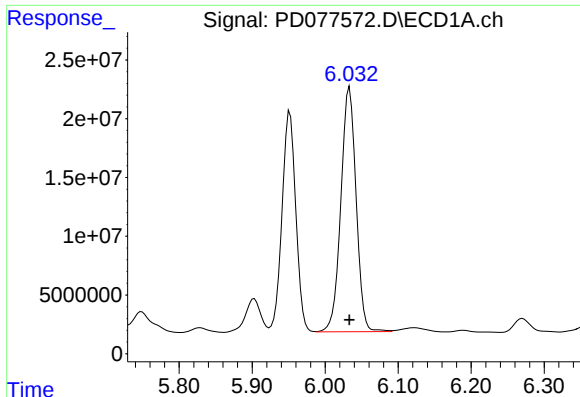

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 301750139
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

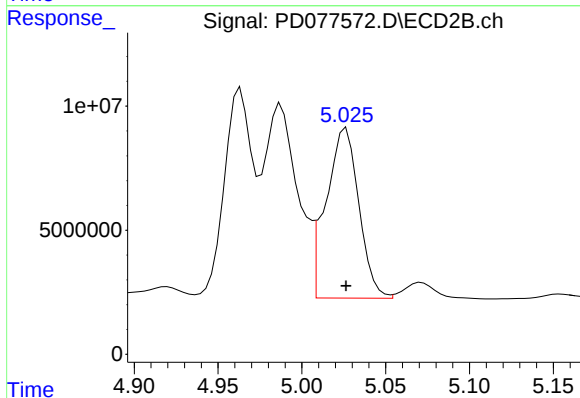


#26 Chlordane-4

R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 93139505
Conc: 500.00 ng/ml

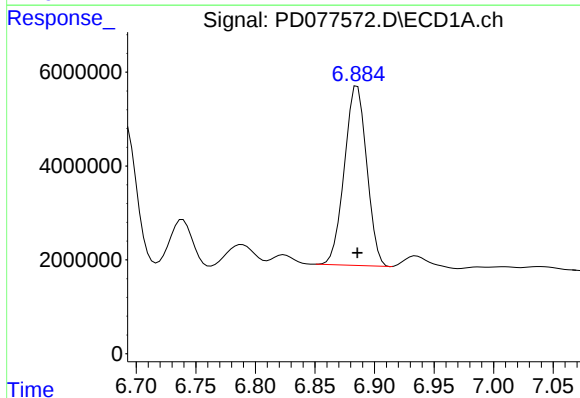


#27 Chlordane-5

R.T.: 6.886 min
Delta R.T.: 0.000 min
Response: 49935424
Conc: 500.00 ng/ml

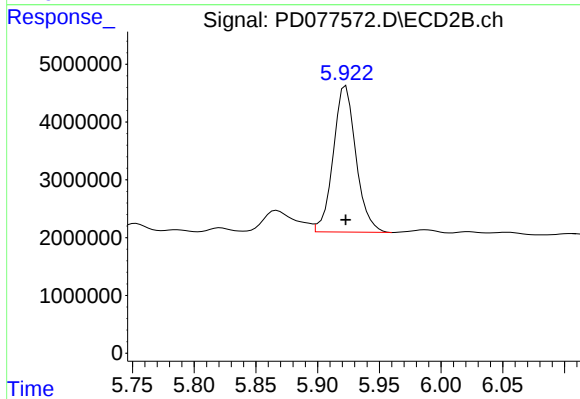

#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 32384461
Conc: 500.00 ng/ml

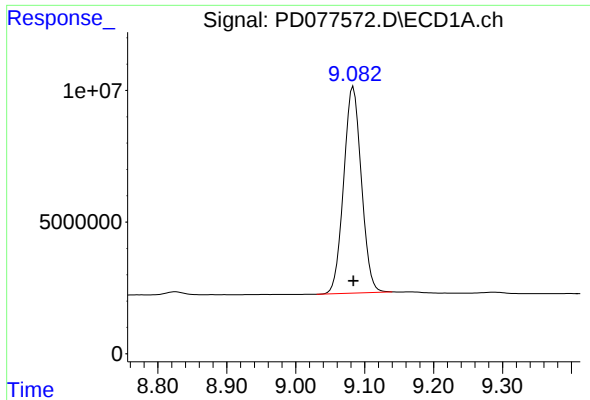

#28 Decachlorobiphenyl


R.T.: 9.083 min

Delta R.T.: 0.000 min

Response: 139908265

Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

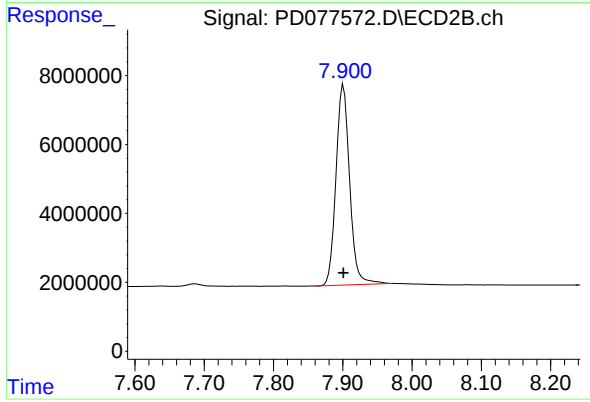

#28 Decachlorobiphenyl

R.T.: 7.901 min

Delta R.T.: 0.000 min

Response: 79741682

Conc: 50.00 ng/ml