

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
 Data File : PD077573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 15:21
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 16:11:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 01 16:06:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.760	58421627	42359285	25.086	24.518
28)	SA Decachlor...	9.082	7.900	72651979	40475748	25.964	25.379
Target Compounds							
23)	Chlordane-1	4.707	3.757	27927349	13827586	248.096	247.161
24)	Chlordane-2	5.237	4.333	31605759	15524107	259.591	250.227
25)	Chlordane-3	5.950	4.963	119.0E6	46723767	240.889	239.773
26)	Chlordane-4	6.033	5.026	147.4E6	45178109	244.205	242.529
27)	Chlordane-5	6.884	5.922	24461897	15289592	244.935	236.064



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
Data File : PD077573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 15:21
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 16:11:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
Quant Title : GC Extractables
QLast Update : Fri Sep 01 16:06:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

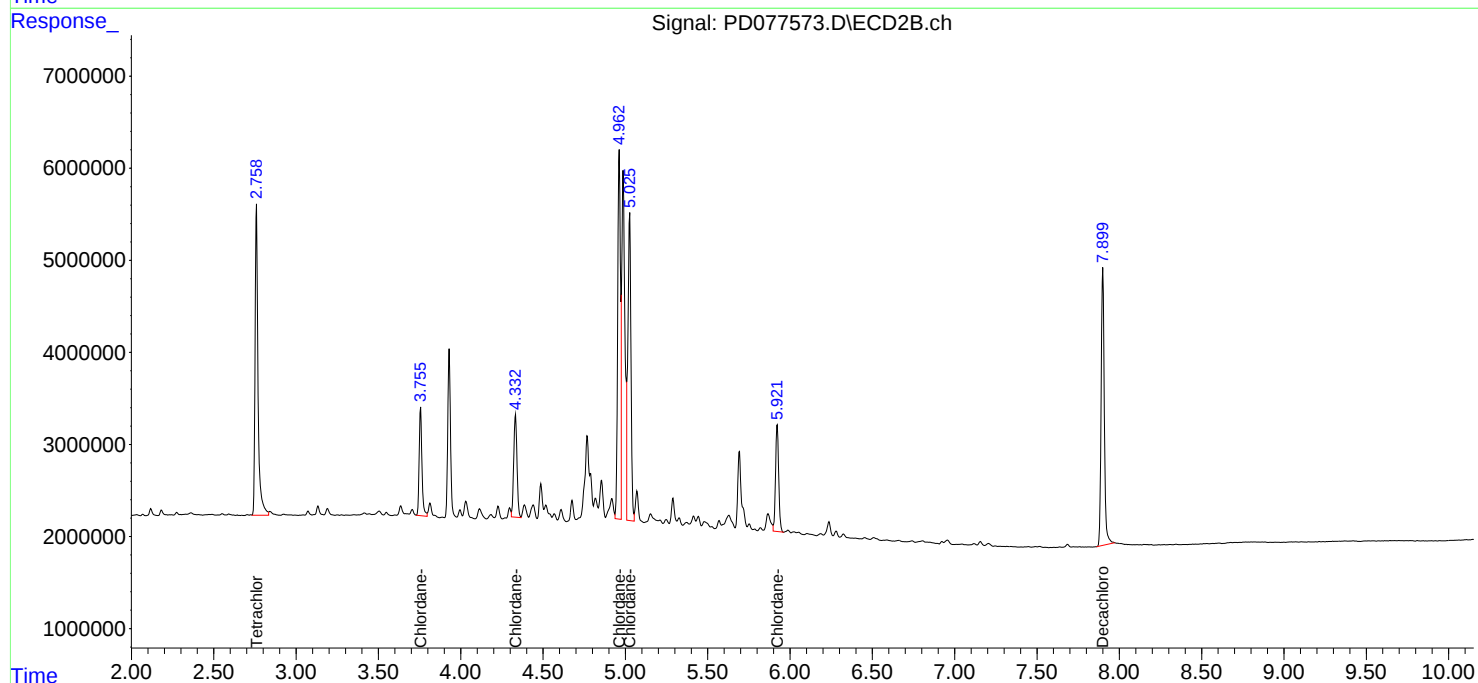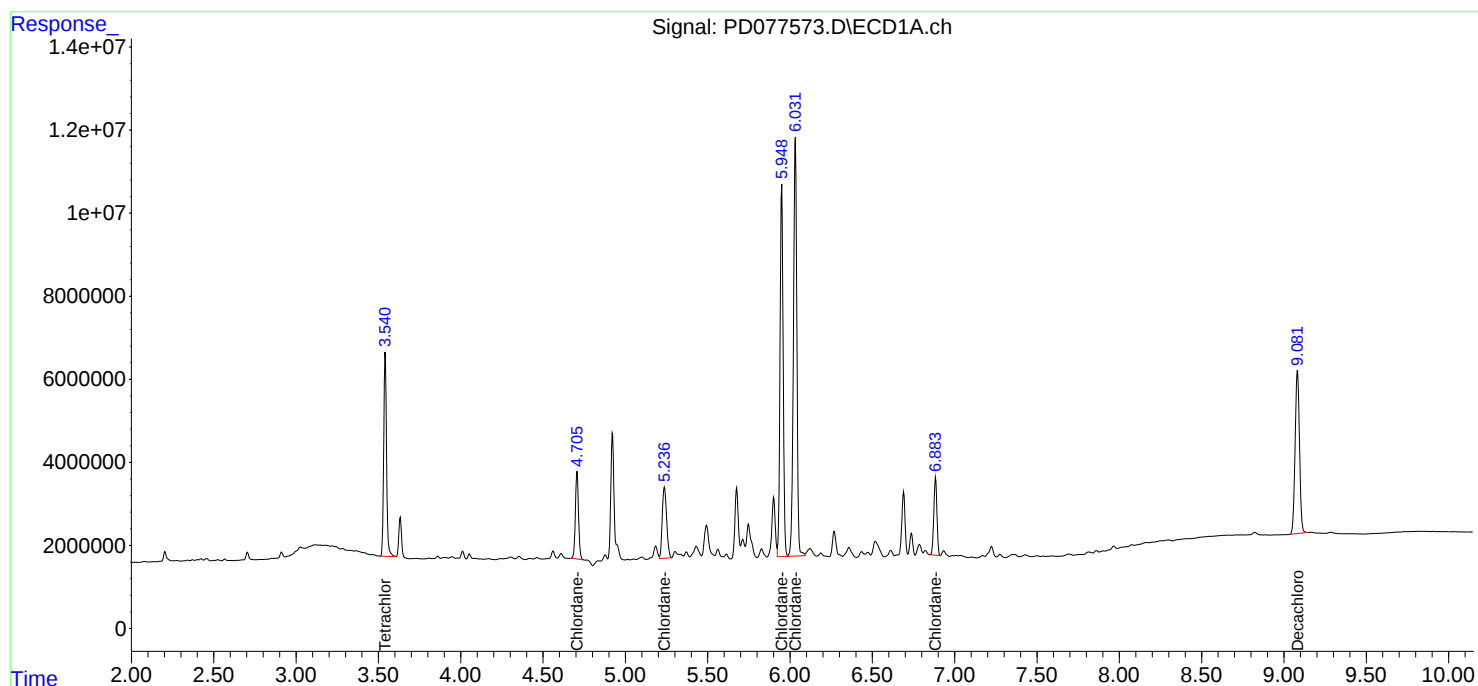


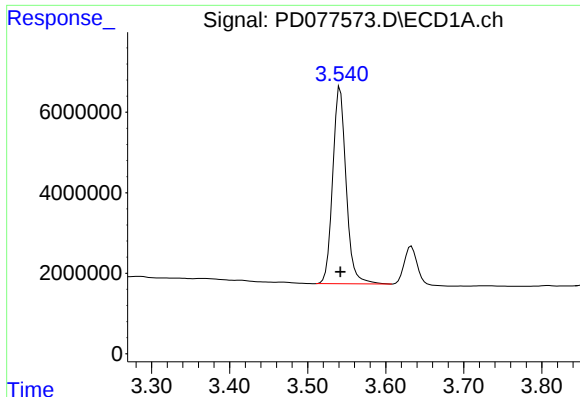

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 58421627
Conc: 25.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

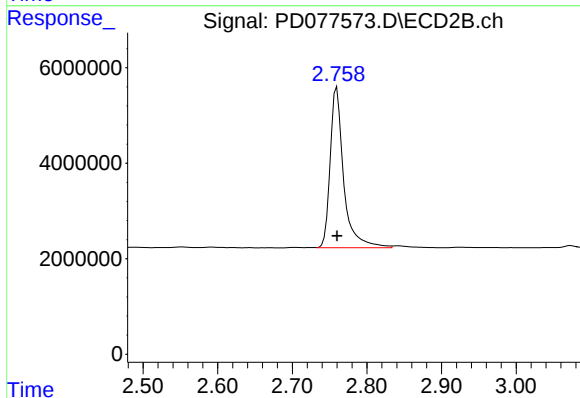


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 42359285
Conc: 24.52 ng/ml

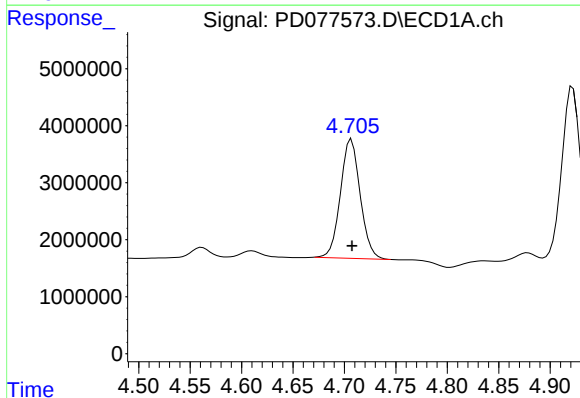


#23 Chlordane-1

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 27927349
Conc: 248.10 ng/ml

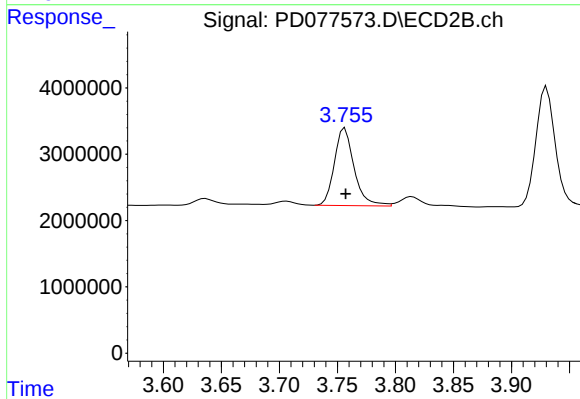

#23 Chlordane-1


R.T.: 3.757 min
Delta R.T.: 0.000 min
Response: 13827586
Conc: 247.16 ng/ml

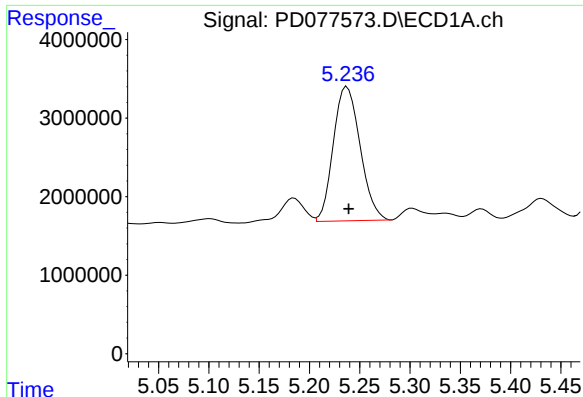

#24 Chlordane-2


R.T.: 5.237 min
Delta R.T.: -0.002 min
Response: 31605759
Conc: 259.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

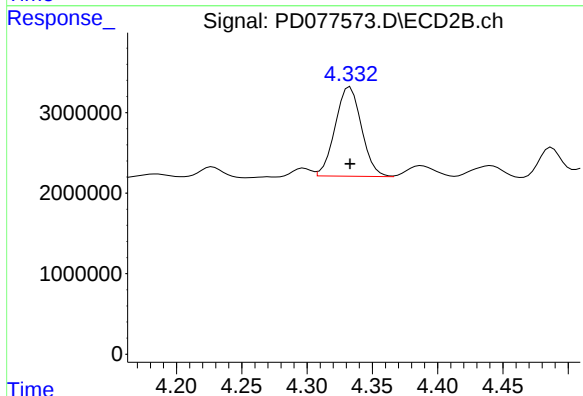


#24 Chlordane-2

R.T.: 4.333 min
Delta R.T.: 0.000 min
Response: 15524107
Conc: 250.23 ng/ml

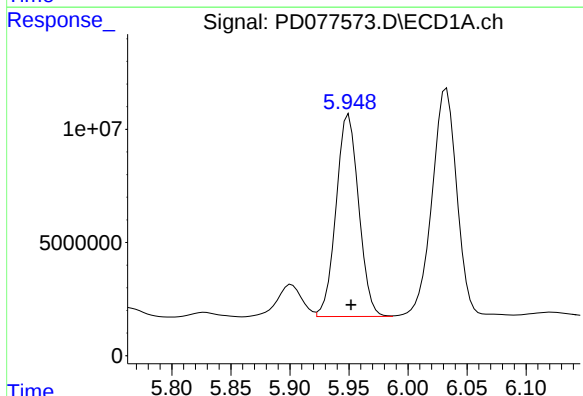


#25 Chlordane-3

R.T.: 5.950 min
Delta R.T.: -0.002 min
Response: 118997435
Conc: 240.89 ng/ml

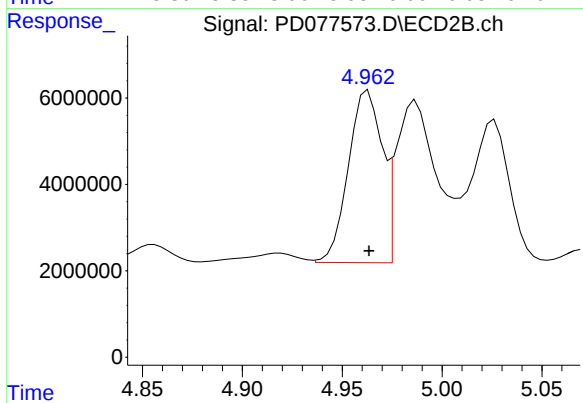

#25 Chlordane-3


R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 46723767
Conc: 239.77 ng/ml

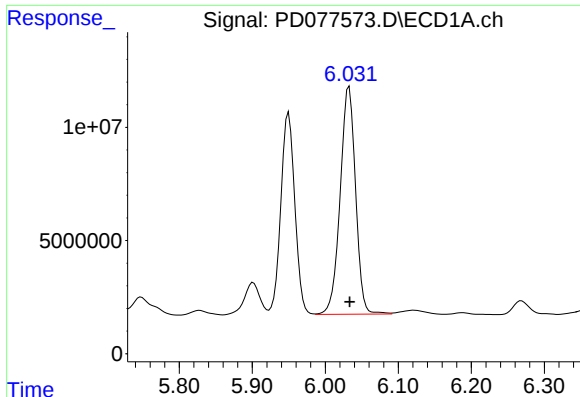

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 147377734
Conc: 244.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

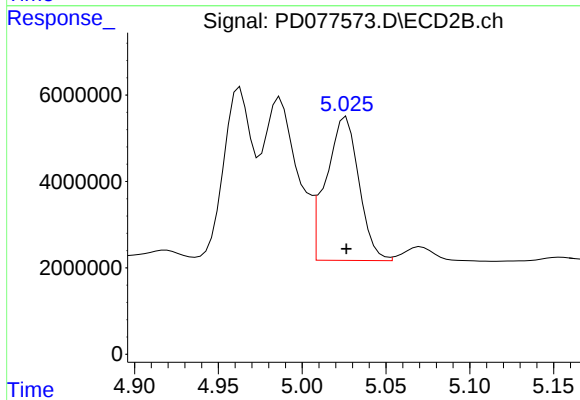


#26 Chlordane-4

R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 45178109
Conc: 242.53 ng/ml

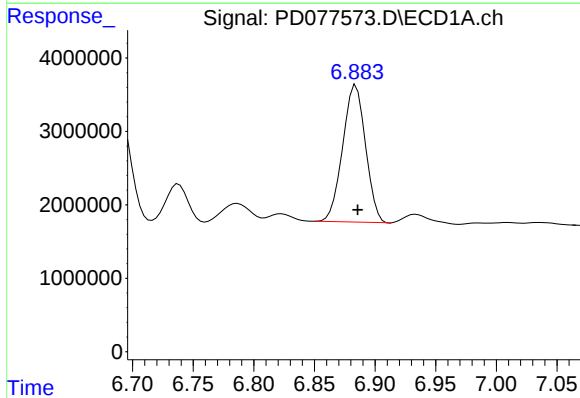


#27 Chlordane-5

R.T.: 6.884 min
Delta R.T.: -0.001 min
Response: 24461897
Conc: 244.94 ng/ml

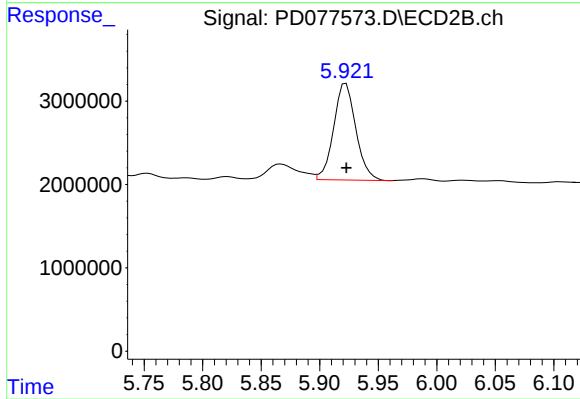

#27 Chlordane-5


R.T.: 5.922 min
Delta R.T.: 0.000 min
Response: 15289592
Conc: 236.06 ng/ml

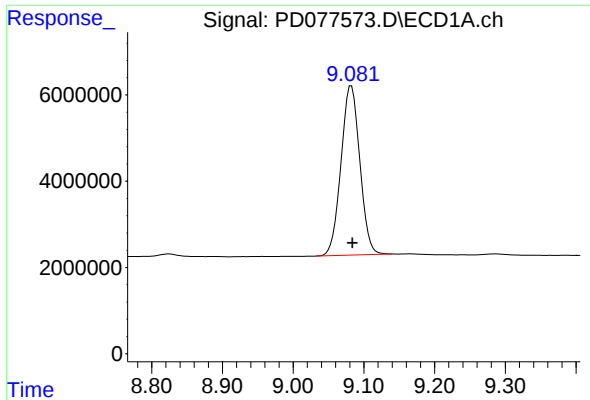

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.001 min
Response: 72651979
Conc: 25.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

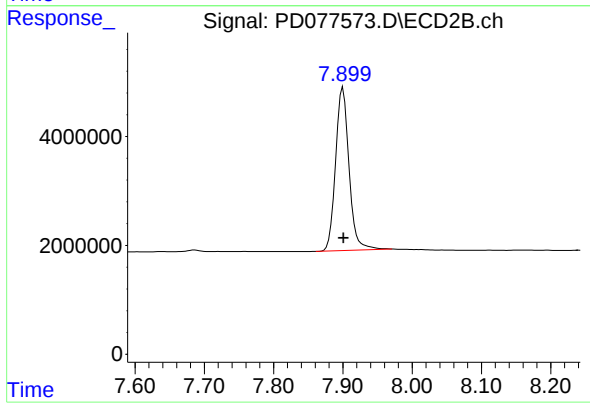

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 40475748
Conc: 25.38 ng/ml