

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
 Data File : PD077564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 13:21
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 18:18:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 01 16:18:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.760	46867303	29366545	18.459	18.567
28)	SA Decachlor...	9.083	7.901	58155722	31907497	19.091	18.490
Target Compounds							
9)	A Endosulfan I	6.080	5.083	30166389	16613500	9.172	8.869
10)	B gamma-Chl...	5.950	4.963	32696369	18737388	9.288	9.321
12)	B 4,4'-DDE	6.202	5.216	58816073	33296860	18.268	18.242
13)	MA Dieldrin	6.356	5.348	63213118	36624337	17.767	17.937
19)	B Endosulfa...	7.172	6.320	52655834	29439209	18.554	18.385
20)	A Methoxychlor	7.512	6.598	141.5E6	72646255	91.506	93.829
21)	B Endrin ke...	7.658	6.827	59831664	34130633	18.409	18.051



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
Data File : PD077564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 13:21
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 18:18:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
Quant Title : GC Extractables
QLast Update : Fri Sep 01 16:18:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

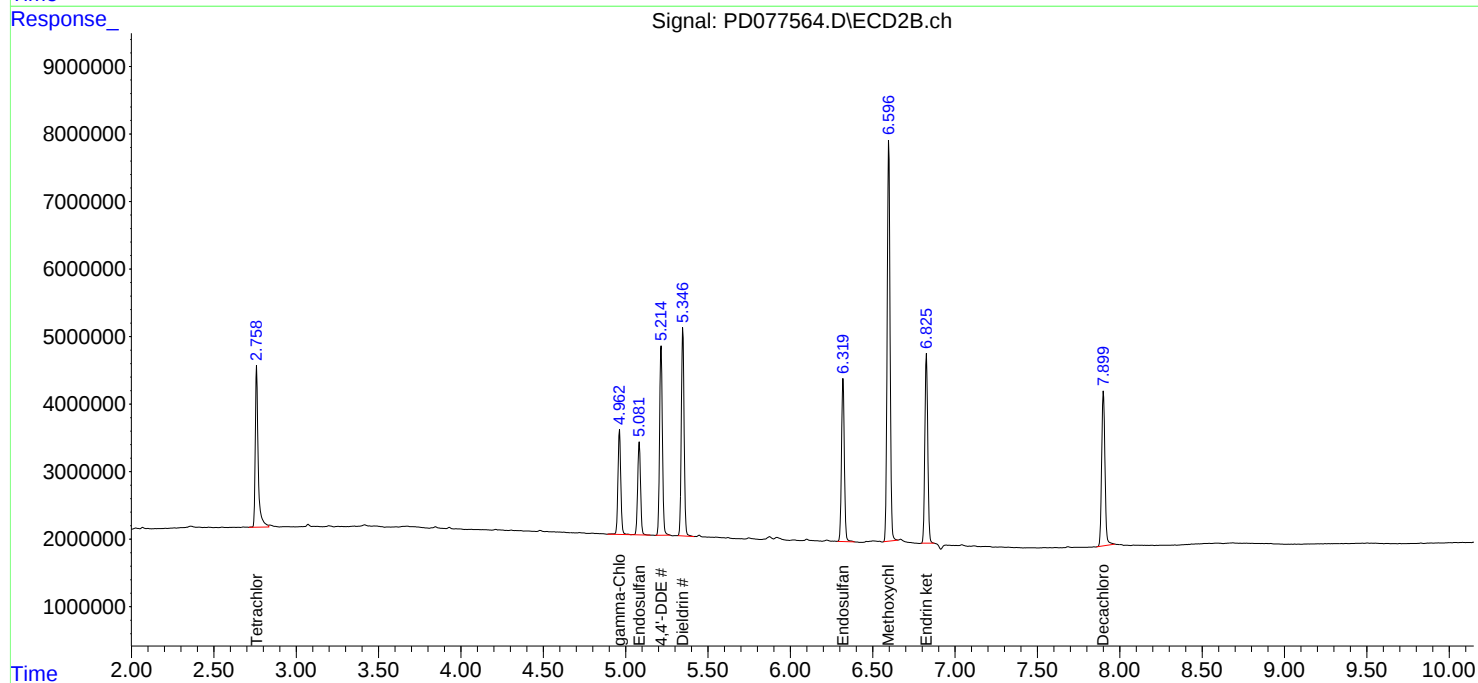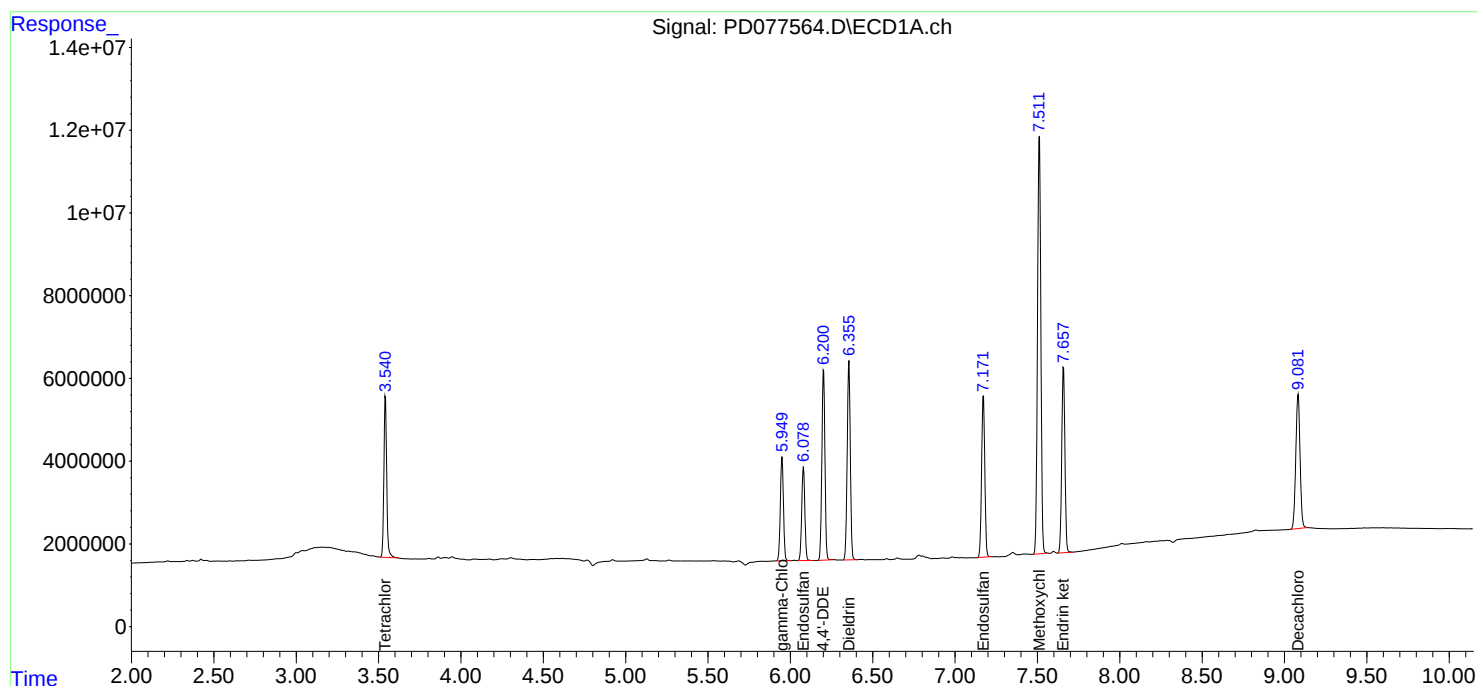


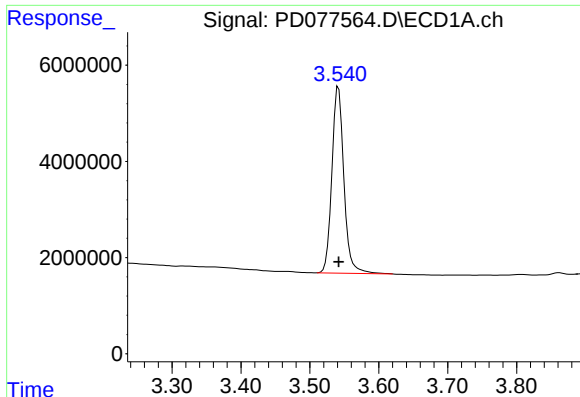

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 46867303
Conc: 18.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

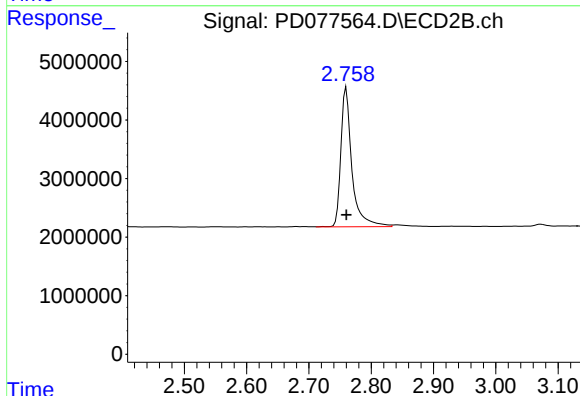


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 29366545
Conc: 18.57 ng/ml

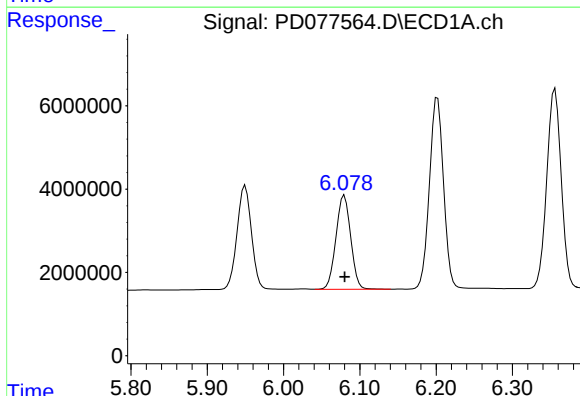


#9 Endosulfan I

R.T.: 6.080 min
Delta R.T.: 0.000 min
Response: 30166389
Conc: 9.17 ng/ml

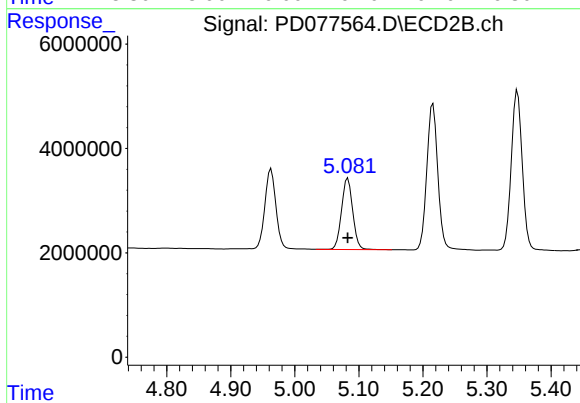

#9 Endosulfan I


R.T.: 5.083 min
Delta R.T.: 0.000 min
Response: 16613500
Conc: 8.87 ng/ml

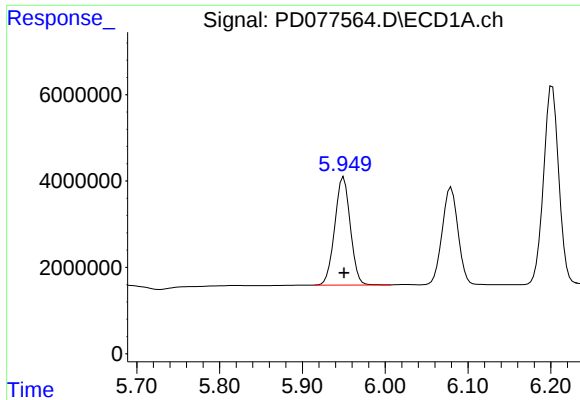

#10 gamma-Chlordane


R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 32696369
Conc: 9.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

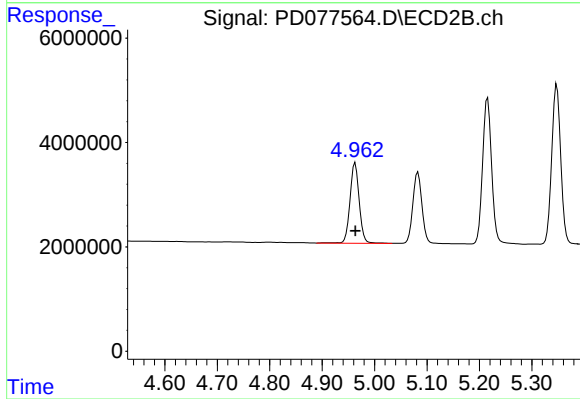


#10 gamma-Chlordane

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 18737388
Conc: 9.32 ng/ml

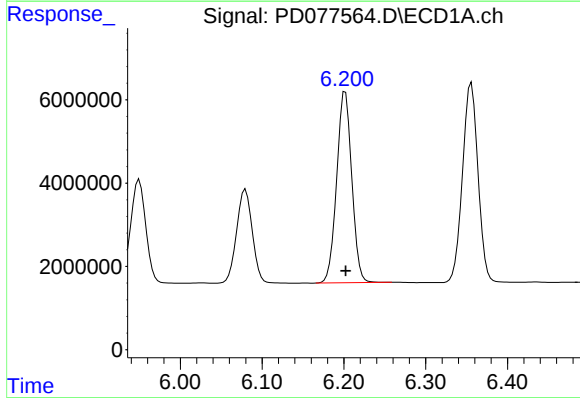


#12 4,4'-DDE

R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 58816073
Conc: 18.27 ng/ml

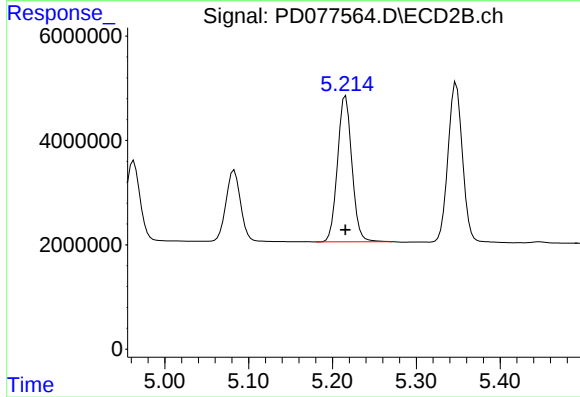

#12 4,4'-DDE


R.T.: 5.216 min
Delta R.T.: 0.000 min
Response: 33296860
Conc: 18.24 ng/ml

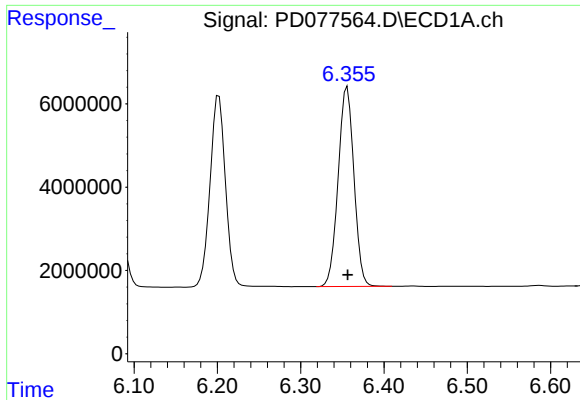

#13 Dieldrin


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 63213118
Conc: 17.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

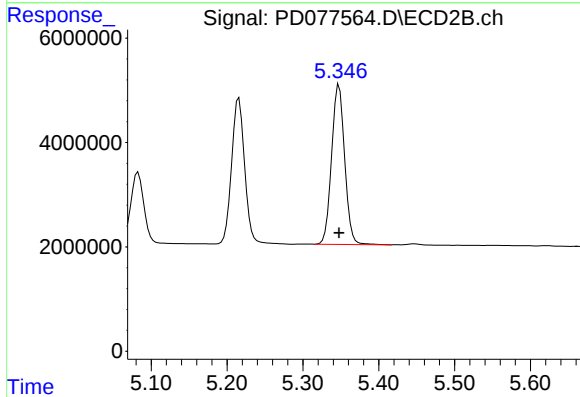


#13 Dieldrin

R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 36624337
Conc: 17.94 ng/ml

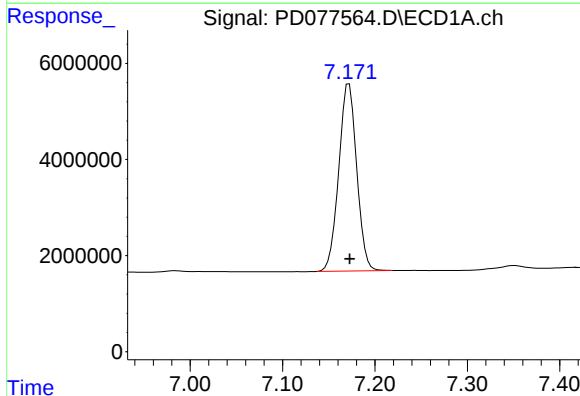


#19 Endosulfan Sulfate

R.T.: 7.172 min
Delta R.T.: 0.000 min
Response: 52655834
Conc: 18.55 ng/ml

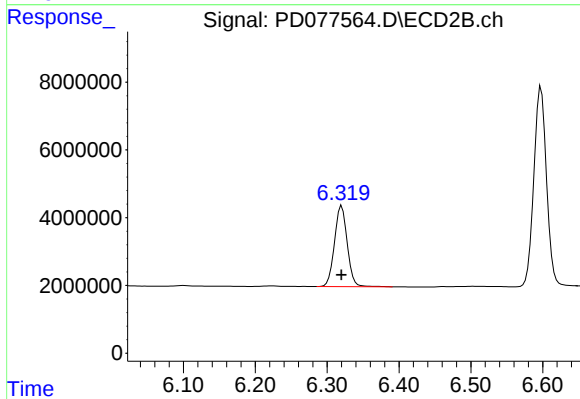

#19 Endosulfan Sulfate


R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 29439209
Conc: 18.39 ng/ml

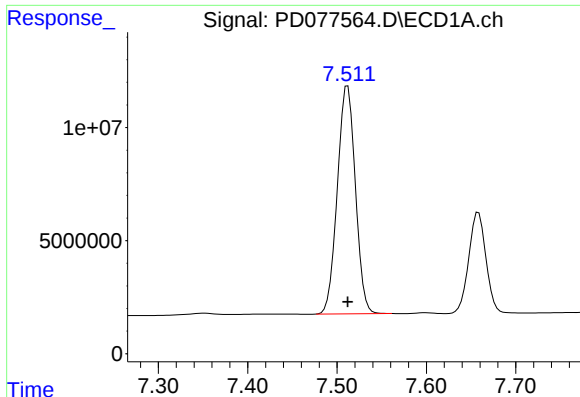

#20 Methoxychlor


R.T.: 7.512 min
Delta R.T.: 0.000 min
Response: 141537187
Conc: 91.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

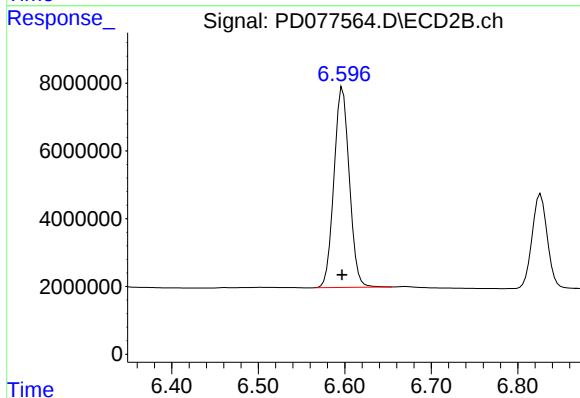


#20 Methoxychlor

R.T.: 6.598 min
Delta R.T.: 0.000 min
Response: 72646255
Conc: 93.83 ng/ml

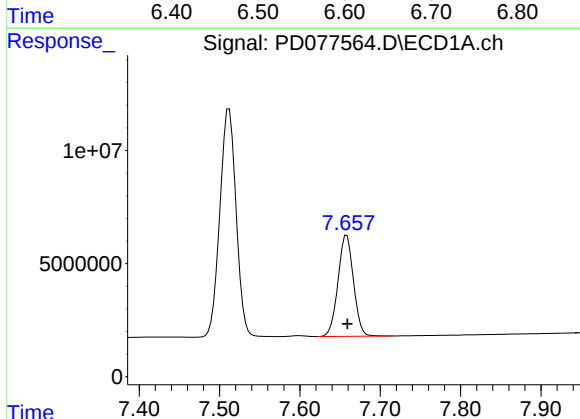


#21 Endrin ketone

R.T.: 7.658 min
Delta R.T.: 0.000 min
Response: 59831664
Conc: 18.41 ng/ml

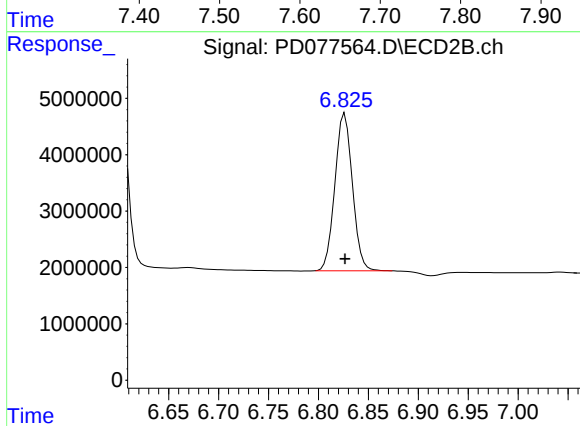

#21 Endrin ketone


R.T.: 6.827 min
Delta R.T.: 0.000 min
Response: 34130633
Conc: 18.05 ng/ml

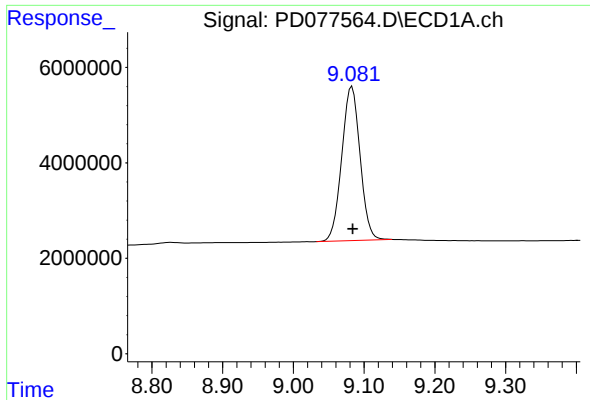

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.001 min
Response: 58155722
Conc: 19.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

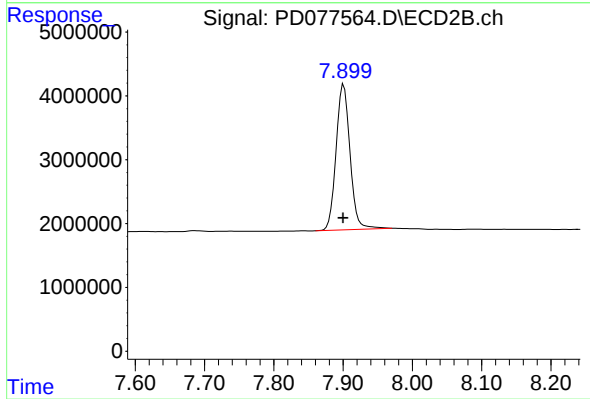

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 31907497
Conc: 18.49 ng/ml