

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
 Data File : PD077570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 14:41
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 16:10:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 01 16:06:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.759	242.1E6	182.8E6	103.965	105.792
28)	SA Decachlor...	9.084	7.900	277.7E6	161.7E6	99.256	101.394
Target Compounds							
23)	Chlordane-1	4.707	3.757	118.1E6	58728506	1049.111	1049.744
24)	Chlordane-2	5.239	4.333	120.1E6	61521288	986.820	991.639
25)	Chlordane-3	5.951	4.964	528.4E6	207.6E6	1069.717	1065.525
26)	Chlordane-4	6.033	5.027	634.6E6	202.6E6	1051.610	1087.808
27)	Chlordane-5	6.885	5.923	103.5E6	69113473	1036.534	1067.078



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
Data File : PD077570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 14:41
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 16:10:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
Quant Title : GC Extractables
QLast Update : Fri Sep 01 16:06:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

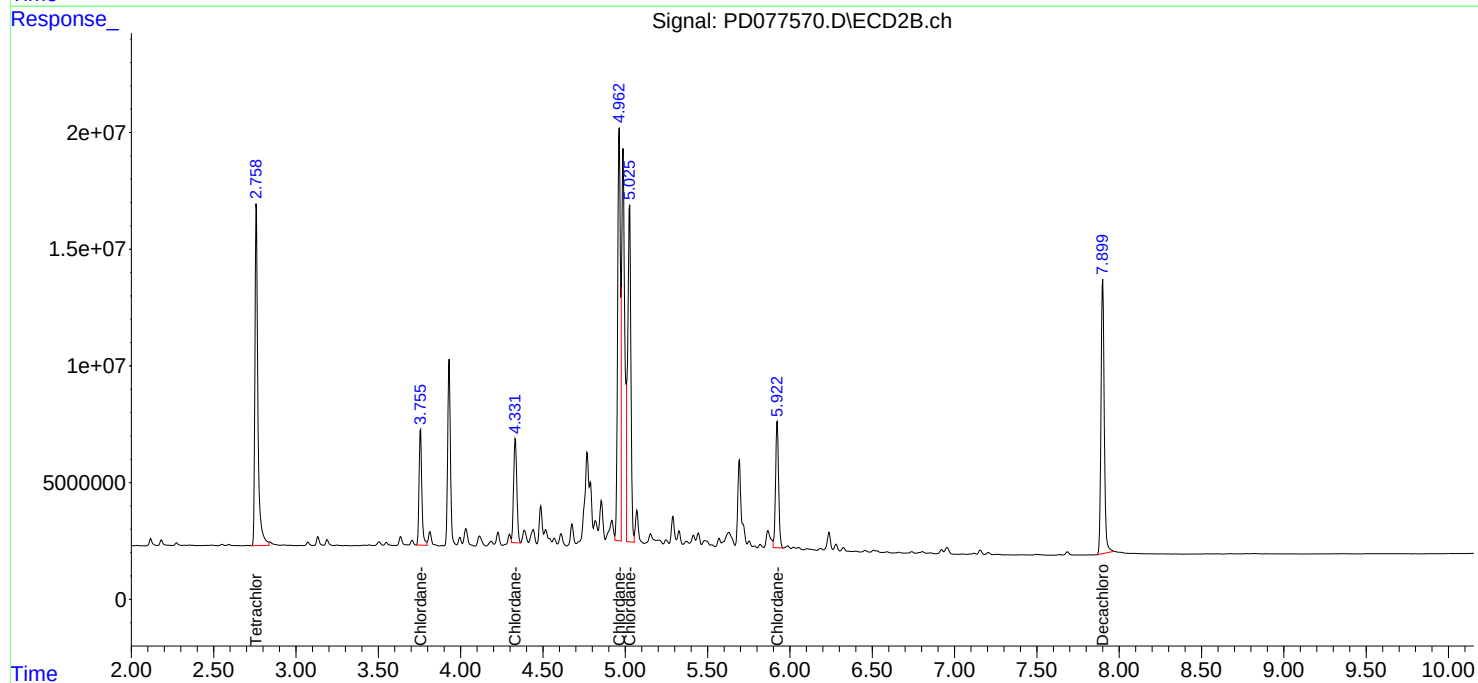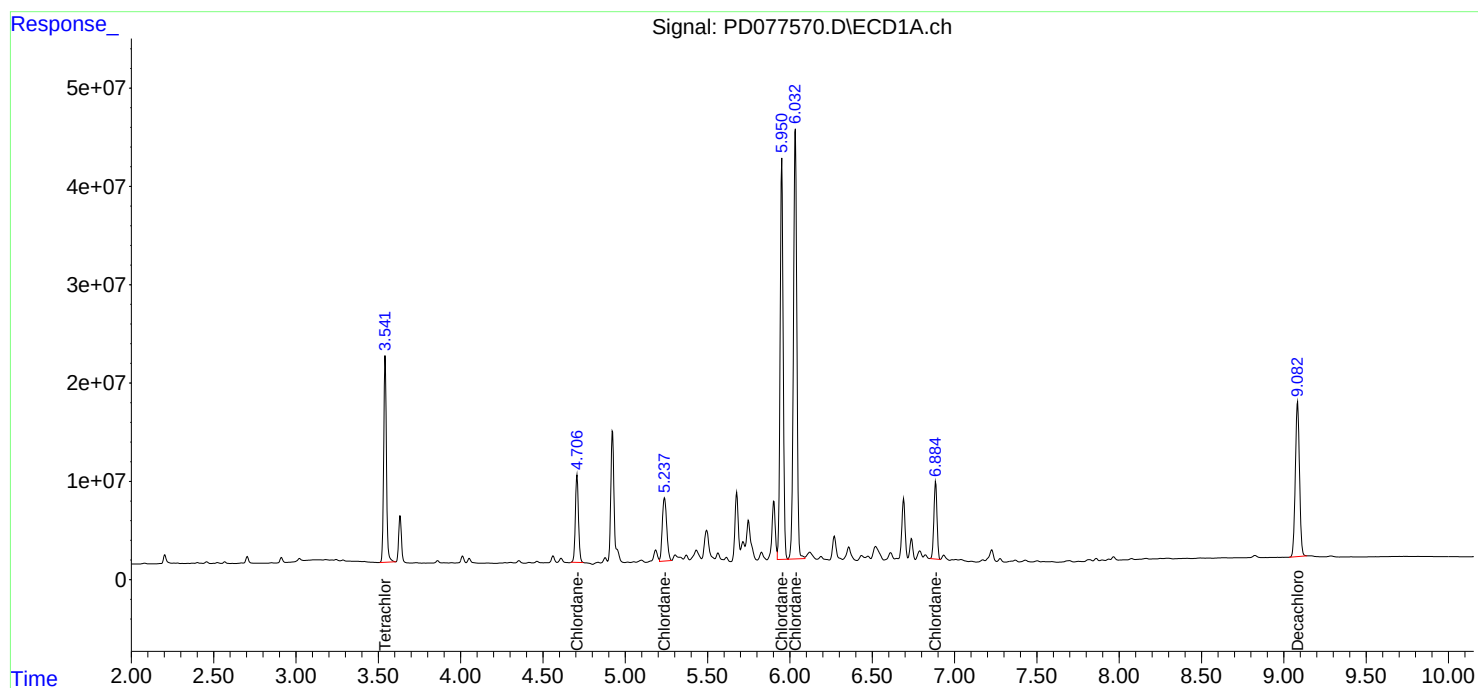


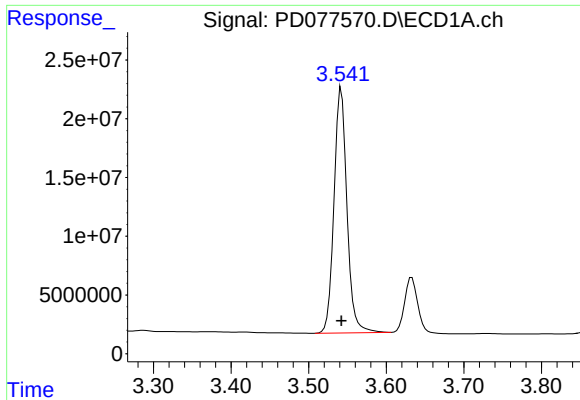

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 242116459
Conc: 103.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

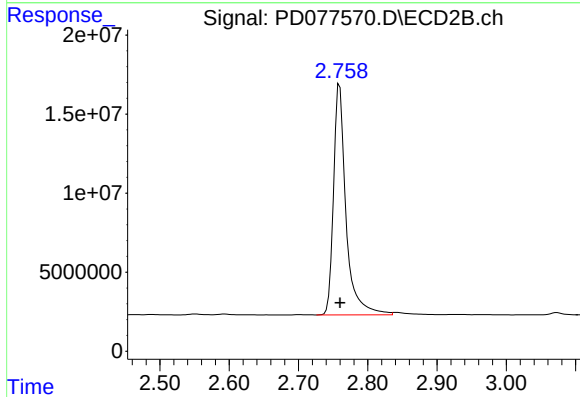


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: 0.000 min
Response: 182776788
Conc: 105.79 ng/ml

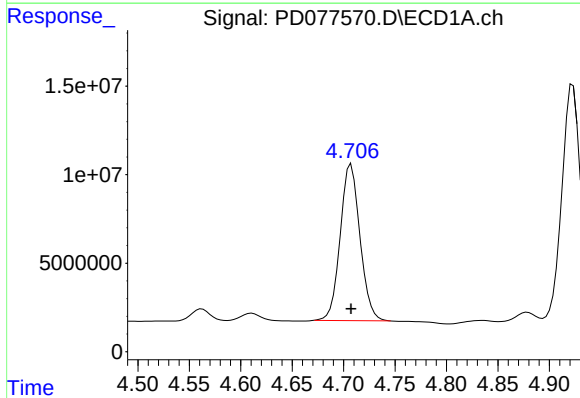


#23 Chlordane-1

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 118094983
Conc: 1049.11 ng/ml

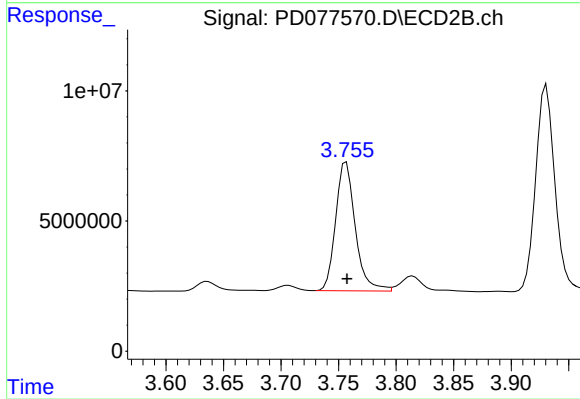

#23 Chlordane-1


R.T.: 3.757 min
Delta R.T.: 0.000 min
Response: 58728506
Conc: 1049.74 ng/ml

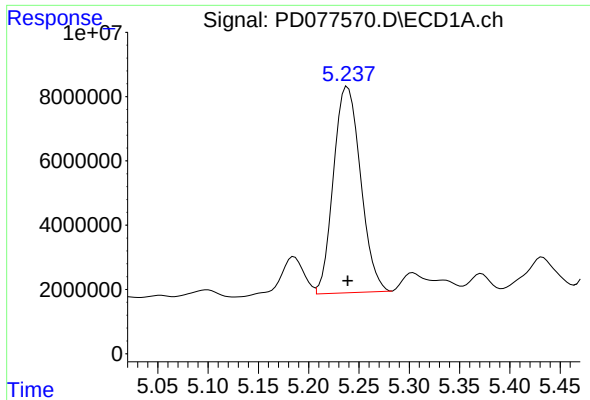

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 120147487
Conc: 986.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

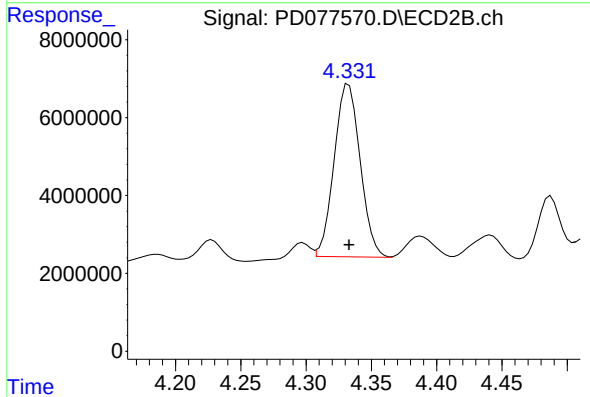


#24 Chlordane-2

R.T.: 4.333 min
Delta R.T.: 0.000 min
Response: 61521288
Conc: 991.64 ng/ml

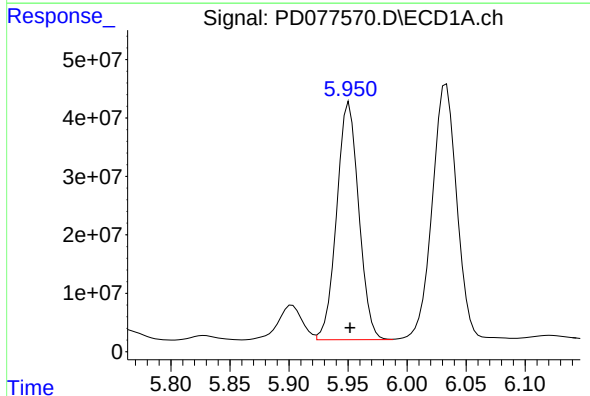


#25 Chlordane-3

R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 528431693
Conc: 1069.72 ng/ml

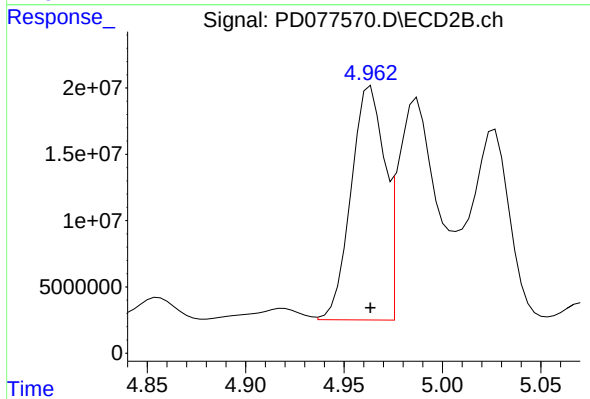

#25 Chlordane-3


R.T.: 4.964 min
Delta R.T.: 0.000 min
Response: 207635518
Conc: 1065.52 ng/ml

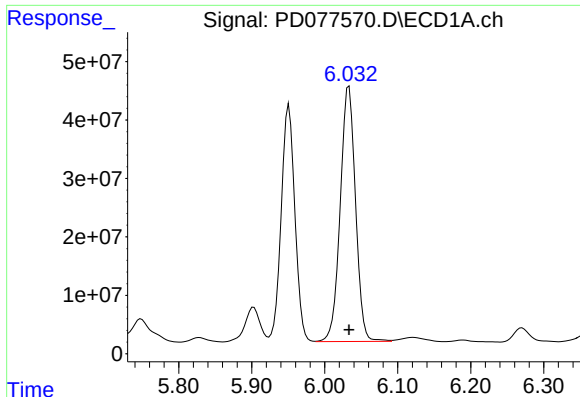

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 634646669
Conc: 1051.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

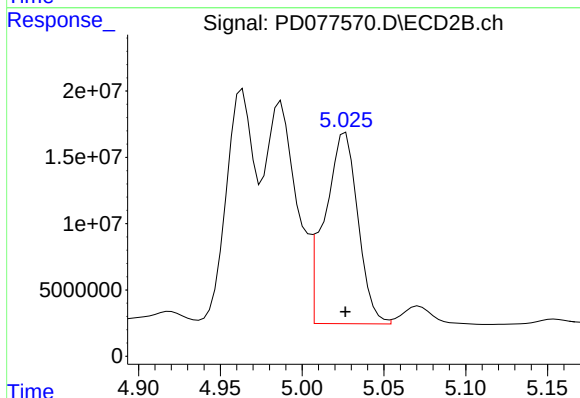


#26 Chlordane-4

R.T.: 5.027 min
Delta R.T.: 0.000 min
Response: 202635888
Conc: 1087.81 ng/ml

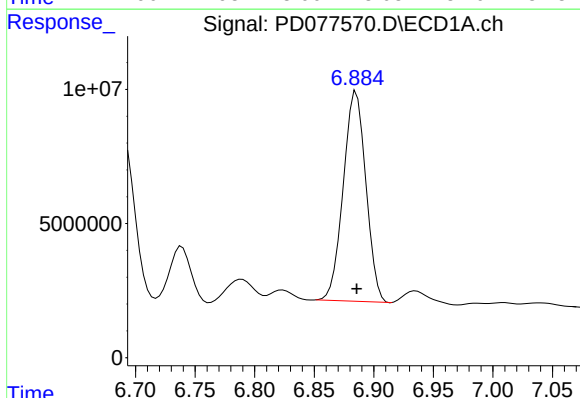


#27 Chlordane-5

R.T.: 6.885 min
Delta R.T.: 0.000 min
Response: 103519501
Conc: 1036.53 ng/ml

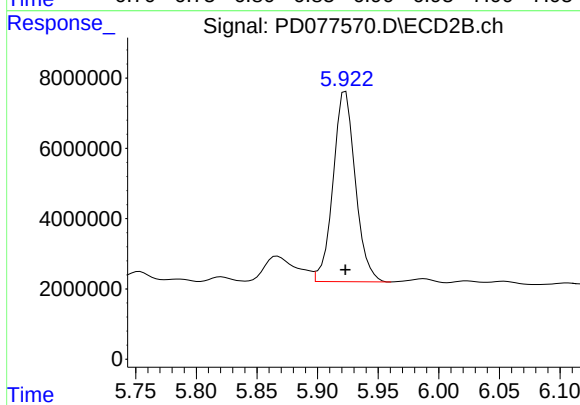

#27 Chlordane-5


R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 69113473
Conc: 1067.08 ng/ml

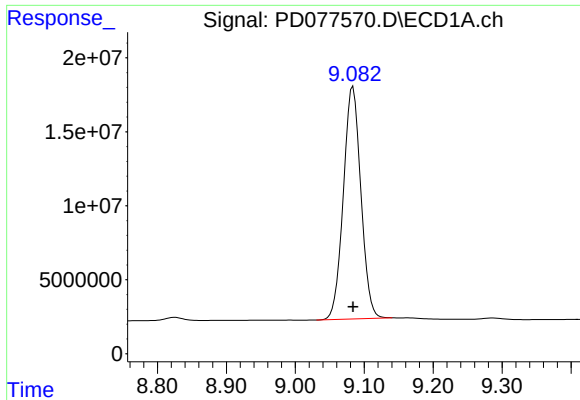

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 277734115
Conc: 99.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

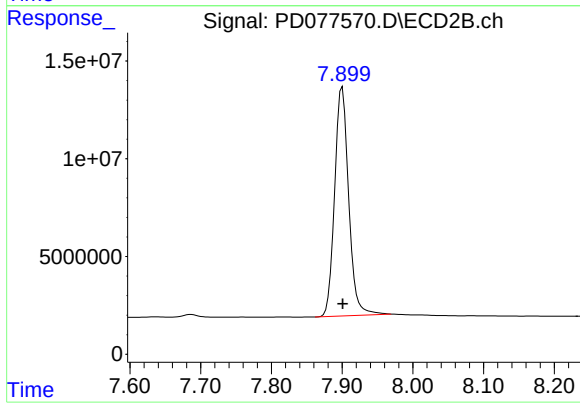

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 161706696
Conc: 101.39 ng/ml