

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
 Data File : PD077574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 15:34
 Operator : AR\AJ
 Sample : PCHLORICC50 (Sig #1); PTOXICC1000 (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC50

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 16:11:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 01 16:06:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.759	12770334	8803129	5.484	5.095
28)	SA Decachlor...	9.082	7.900	16415124	9092047	5.866	5.701
Target Compounds							
23)	Chlordane-1	4.707	3.756	6357833	2875152	56.481	51.392
24)	Chlordane-2	5.238	4.333	7482906	3565430	61.460	57.470
25)	Chlordane-3	5.950	4.963	24912970	9526472	50.432	48.887
26)	Chlordane-4	6.032	5.026	31537510	9074008	52.258	48.712
27)	Chlordane-5	6.884	5.923	5177711	2988348	51.844	46.139



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090323\
Data File : PD077574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 15:34
Operator : AR\AJ
Sample : PCHLORICC50 (Sig #1); PT0XICC1000 (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 16:11:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090323.M
Quant Title : GC Extractables
QLast Update : Fri Sep 01 16:06:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

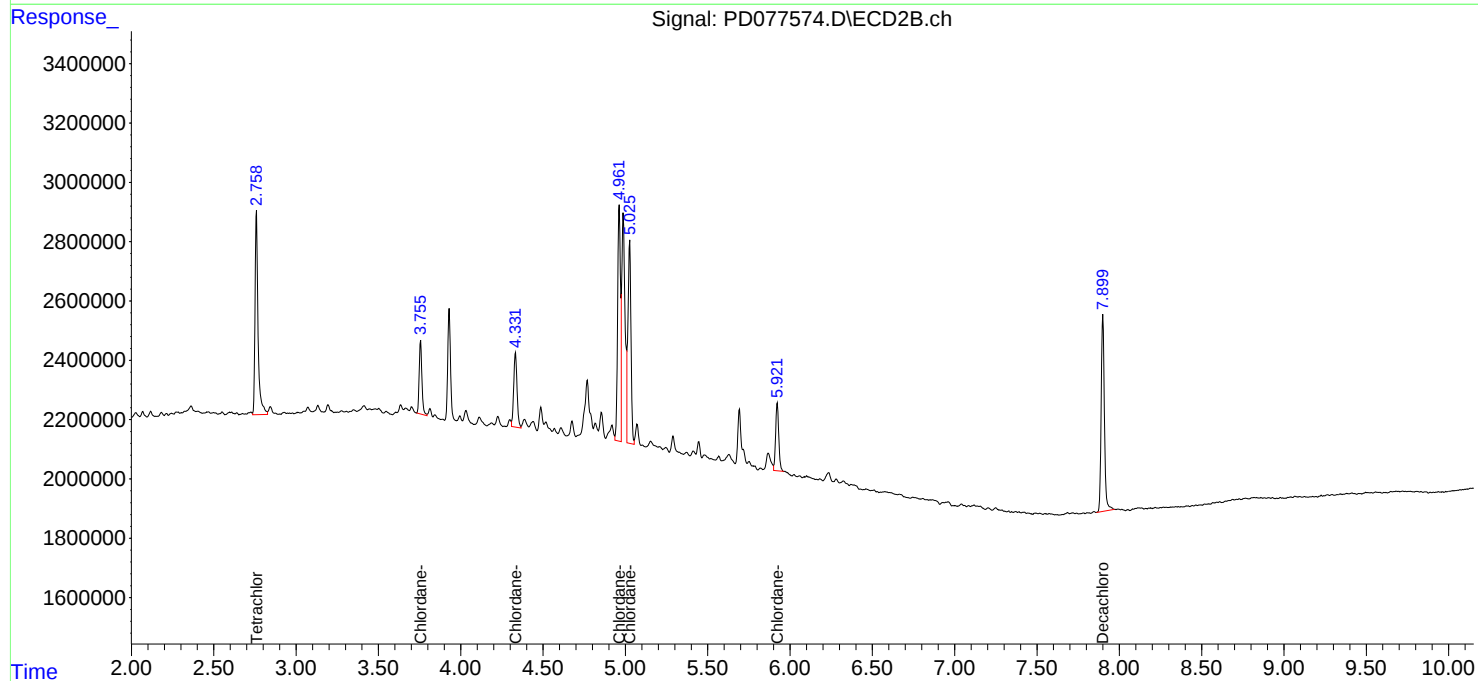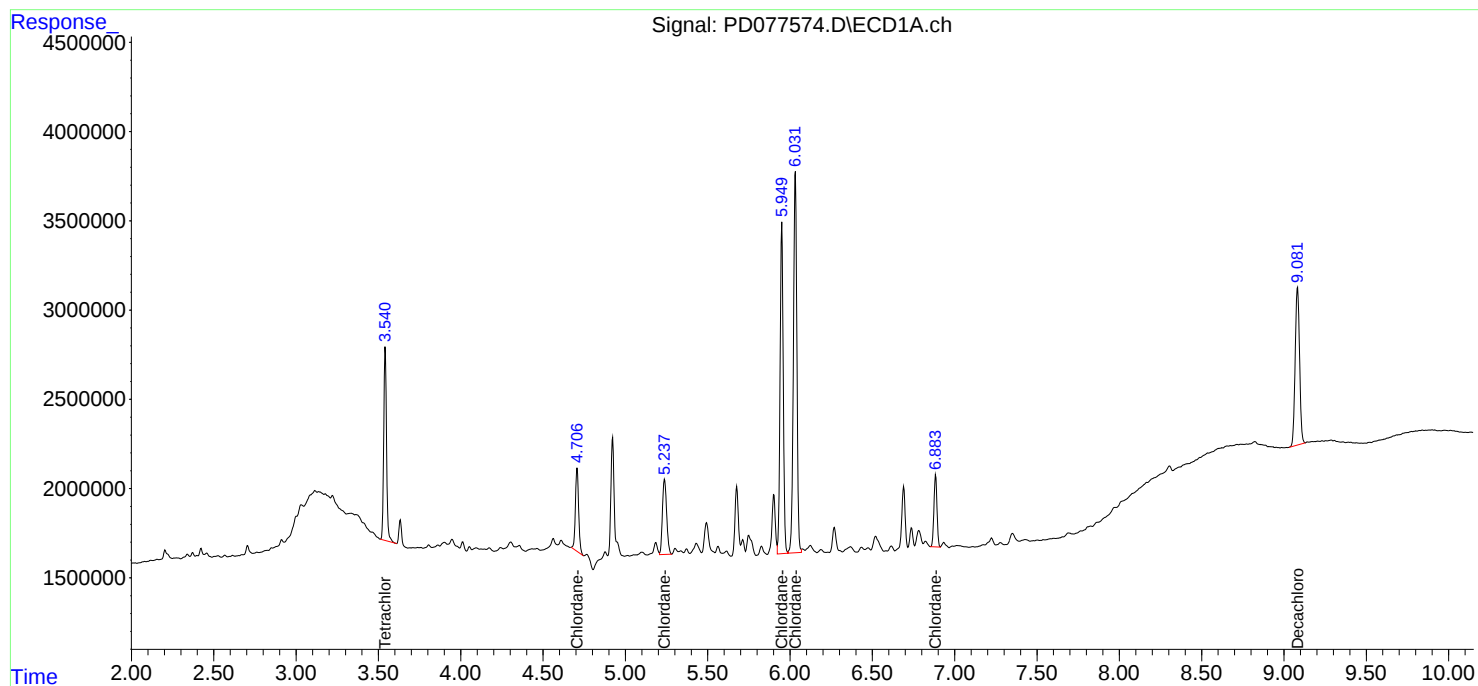


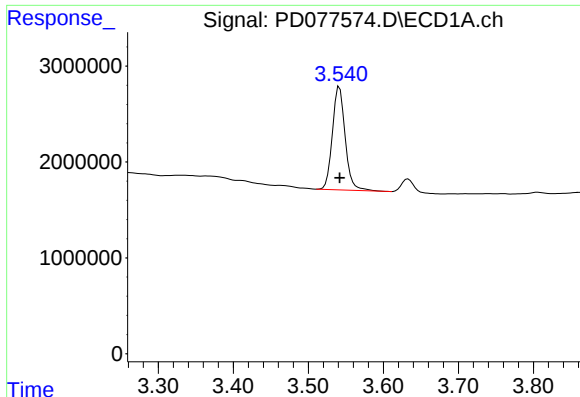

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 12770334
Conc: 5.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

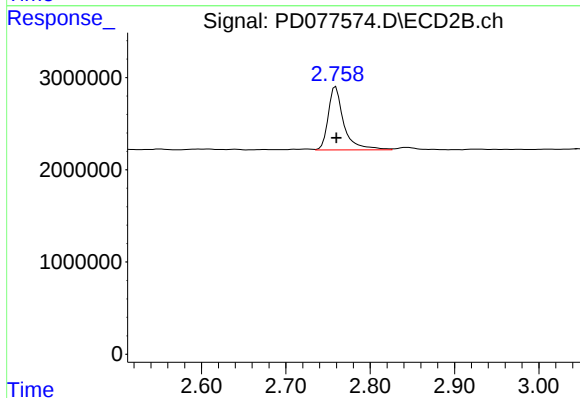


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: 0.000 min
Response: 8803129
Conc: 5.10 ng/ml

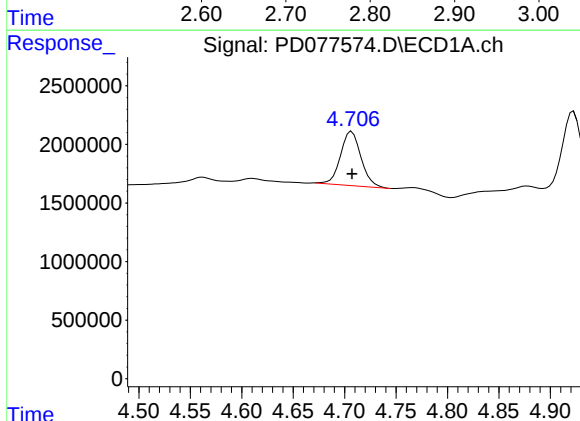


#23 Chlordane-1

R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 6357833
Conc: 56.48 ng/ml

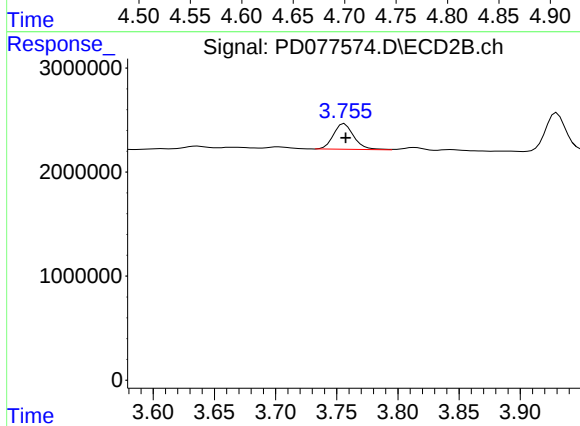

#23 Chlordane-1


R.T.: 3.756 min
Delta R.T.: 0.000 min
Response: 2875152
Conc: 51.39 ng/ml

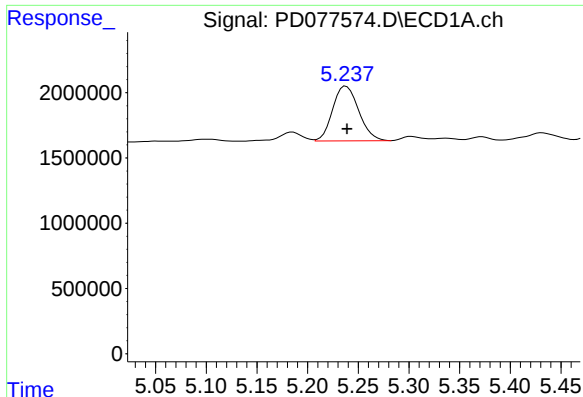

#24 Chlordane-2


R.T.: 5.238 min
Delta R.T.: 0.000 min
Response: 7482906
Conc: 61.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

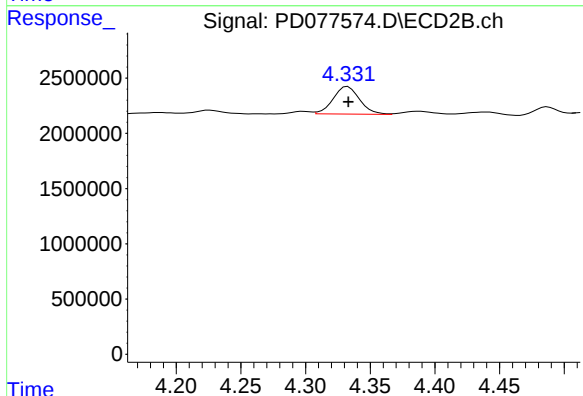


#24 Chlordane-2

R.T.: 4.333 min
Delta R.T.: 0.000 min
Response: 3565430
Conc: 57.47 ng/ml

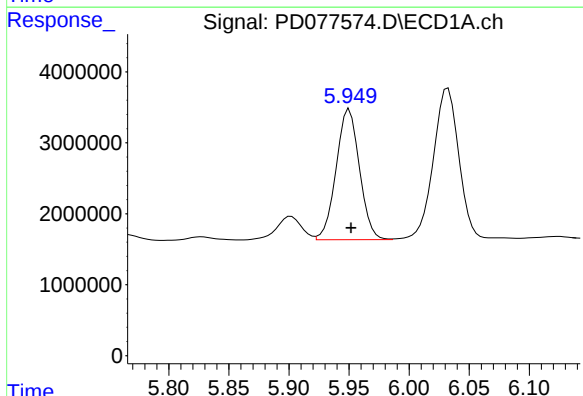


#25 Chlordane-3

R.T.: 5.950 min
Delta R.T.: -0.001 min
Response: 24912970
Conc: 50.43 ng/ml

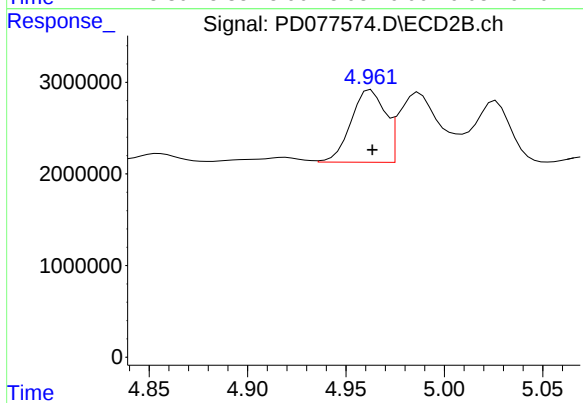

#25 Chlordane-3


R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 9526472
Conc: 48.89 ng/ml

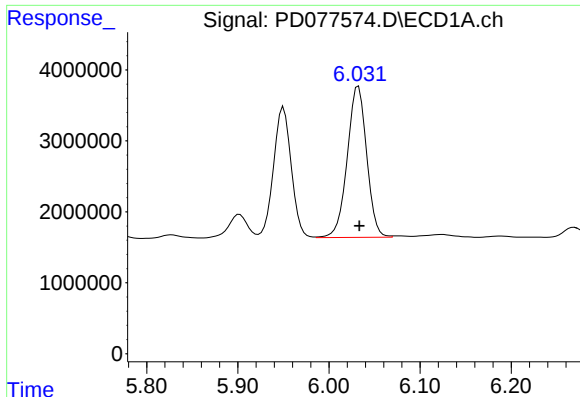

#26 Chlordane-4


R.T.: 6.032 min
Delta R.T.: -0.001 min
Response: 31537510
Conc: 52.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

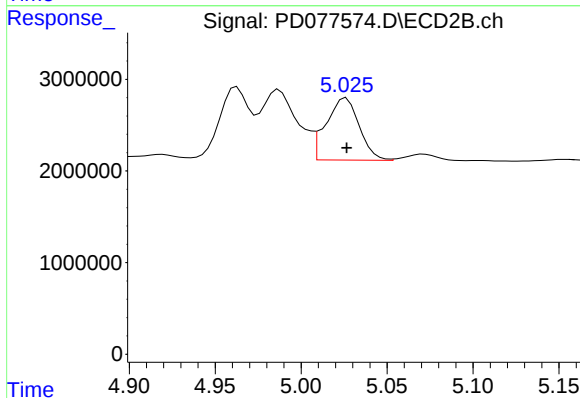


#26 Chlordane-4

R.T.: 5.026 min
Delta R.T.: 0.000 min
Response: 9074008
Conc: 48.71 ng/ml

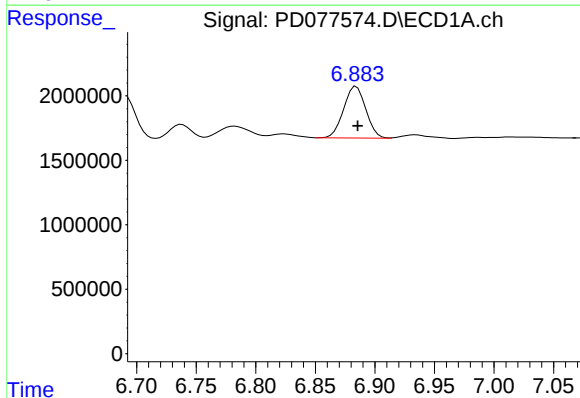


#27 Chlordane-5

R.T.: 6.884 min
Delta R.T.: -0.001 min
Response: 5177711
Conc: 51.84 ng/ml

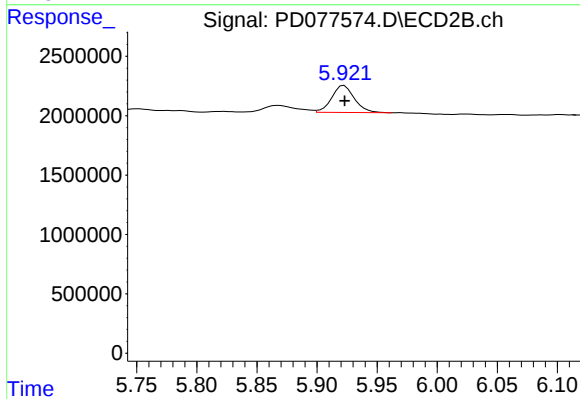

#27 Chlordane-5


R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 2988348
Conc: 46.14 ng/ml

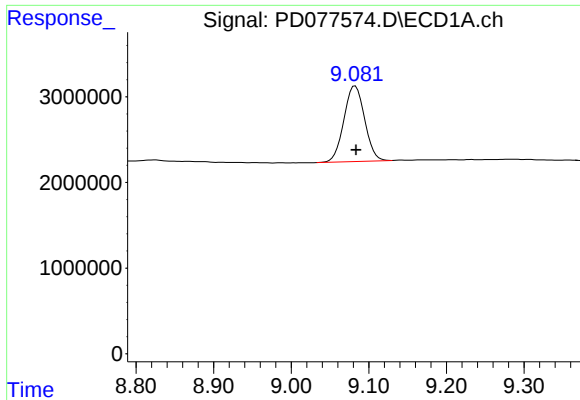

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.001 min
Response: 16415124
Conc: 5.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC50

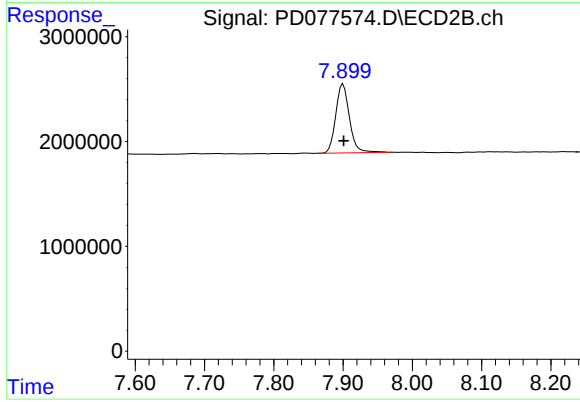

#28 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: 0.000 min
Response: 9092047
Conc: 5.70 ng/ml