

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
 Data File : PD078024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2023 08:26
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 20:09:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.713f	0	42280	N.D.	<MDL
Target Compounds						
3) MA gamma-BHC...	0.000	3.543f	0	94272	N.D.	<MDL
4) MA Heptachlor	0.000	3.972f	0	302271	N.D.	0.136
6) B beta-BHC	0.000	3.874	0	108089	N.D.	0.109


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
Data File : PD078024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2023 08:26
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 20:09:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

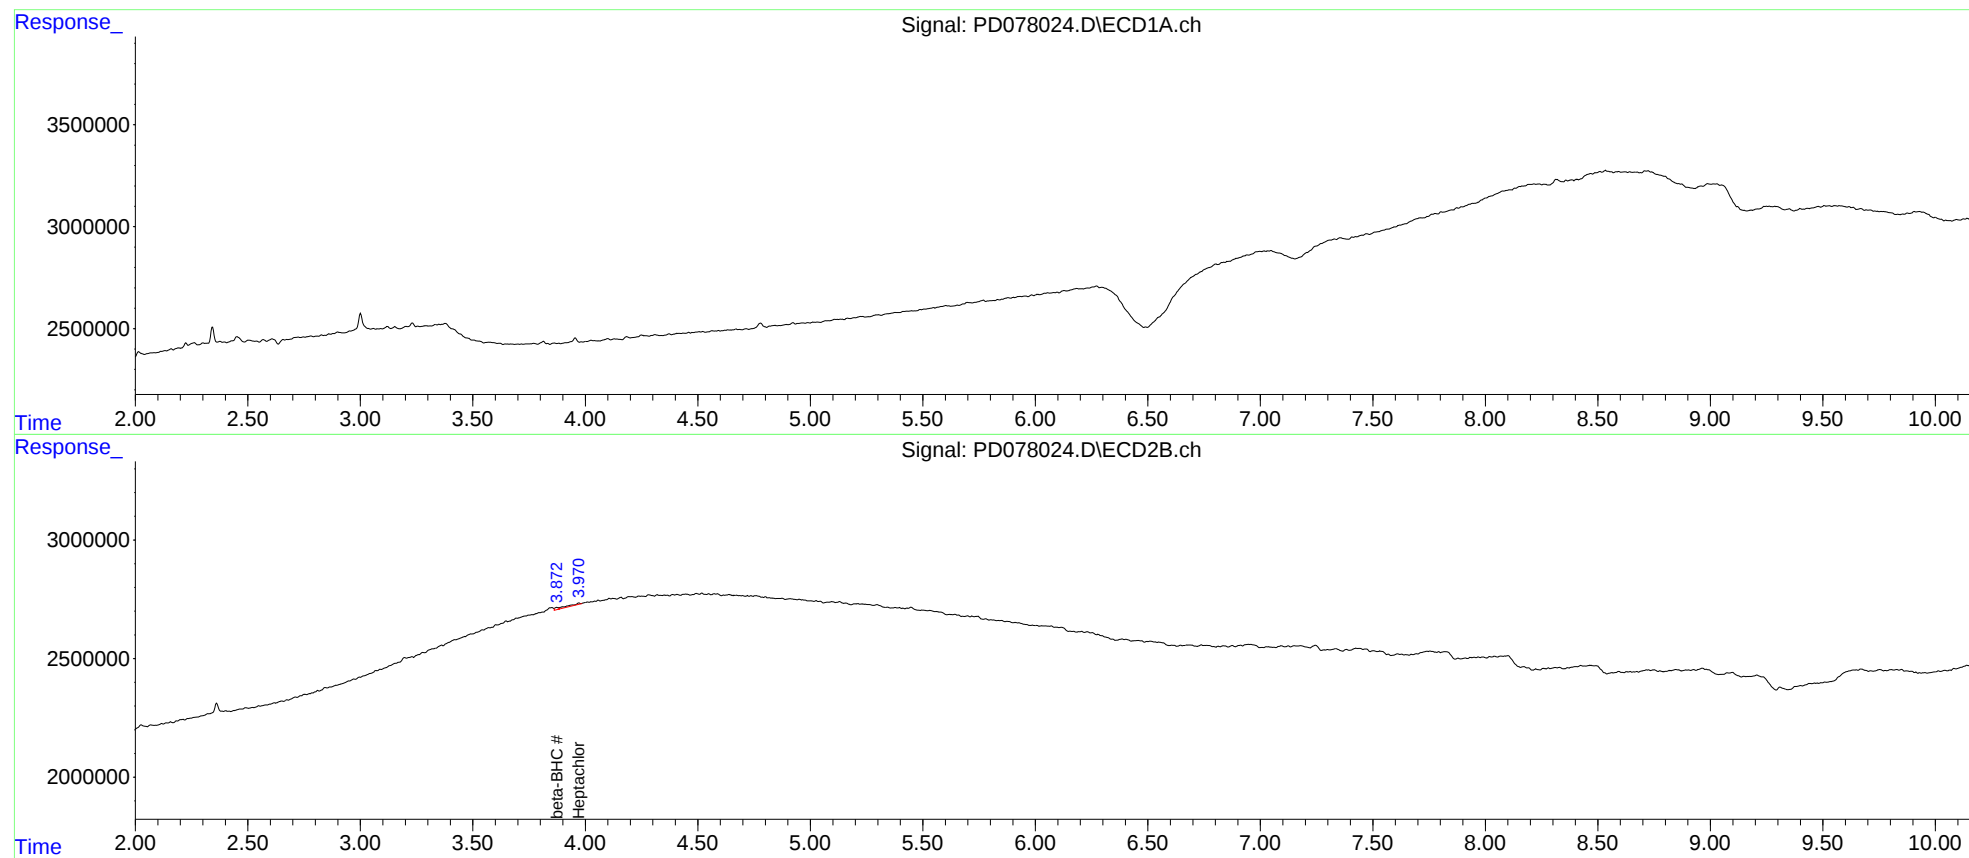

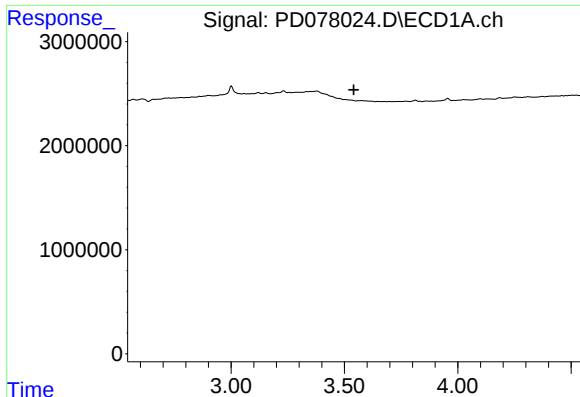


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.542 min
Response: 0
Conc: N.D.

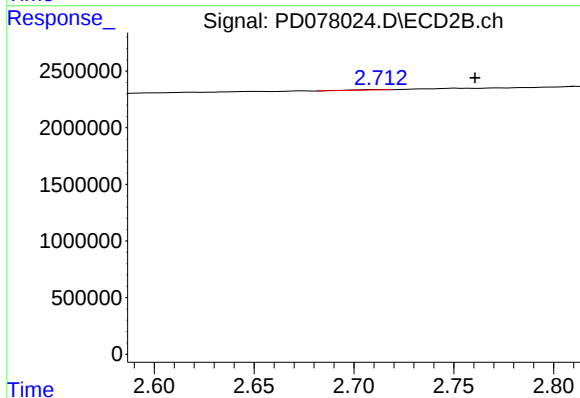


#1 Tetrachloro-m-xylene

R.T.: 2.713 min
Delta R.T.: -0.048 min
Response: 42280
Conc: N.D.

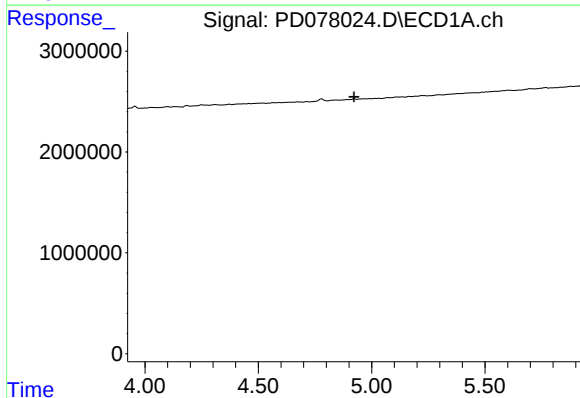


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.923 min
Response: 0
Conc: N.D.

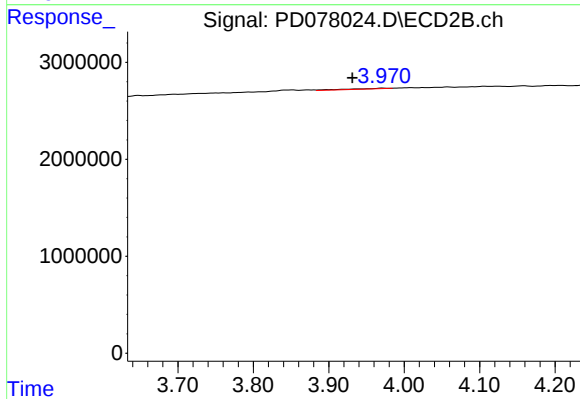


#4 Heptachlor

R.T.: 3.972 min
Delta R.T.: 0.041 min
Response: 302271
Conc: 0.14 ng/ml

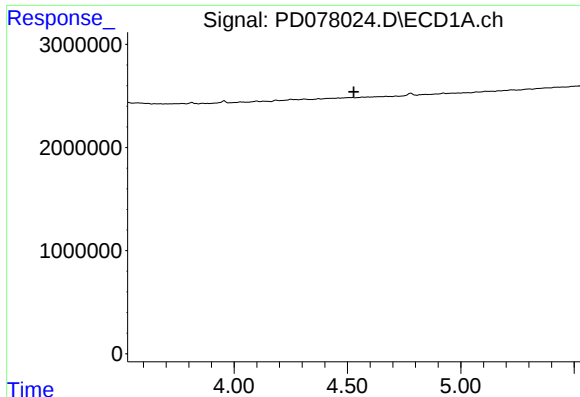


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

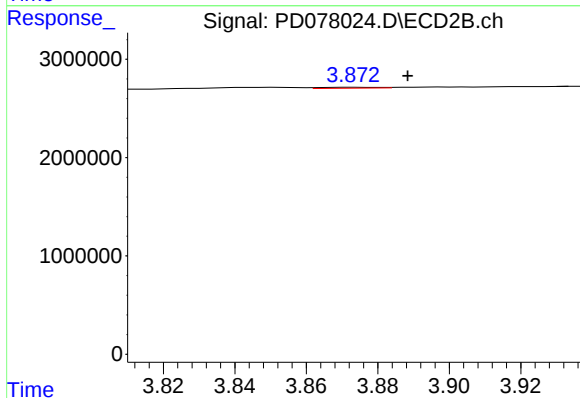


#6 beta-BHC

R.T.: 3.874 min
Delta R.T.: -0.015 min
Response: 108089
Conc: 0.11 ng/ml

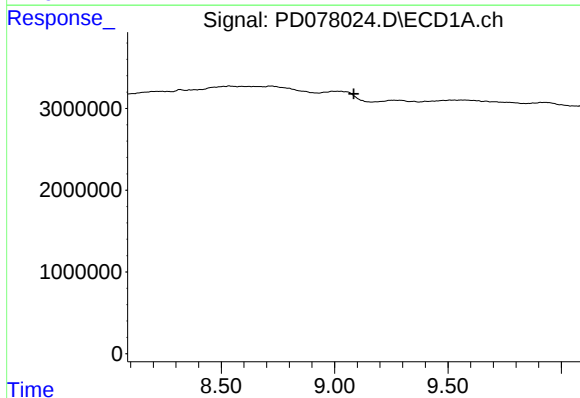

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.

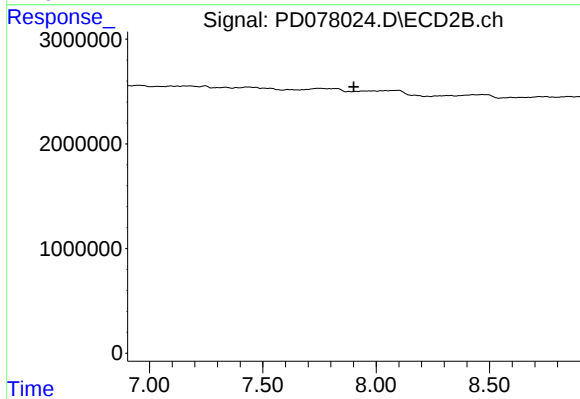

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.901 min
Response: 0
Conc: N.D.