

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
 Data File : PD078027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2023 13:58
 Operator : AR\AJ
 Sample : PB155623BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 20:10:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.771	49542800	28902739	19.523	19.557
2)	SA Decachlor...	9.097	7.916	68715819	34437016	21.997	21.264
Target Compounds							
2)	A alpha-BHC	0.000	3.311f	0	67899	N.D.	<MDL
4)	MA Heptachlor	0.000	3.925	0	199426	N.D.	<MDL
6)	B beta-BHC	0.000	3.860f	0	674801	N.D.	0.683
7)	B delta-BHC	0.000	4.070f	0	167634	N.D.	<MDL
8)	B Heptachlo...	0.000	4.642f	0	91363	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
Data File : PD078027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2023 13:58
Operator : AR\AJ
Sample : PB155623BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 20:10:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

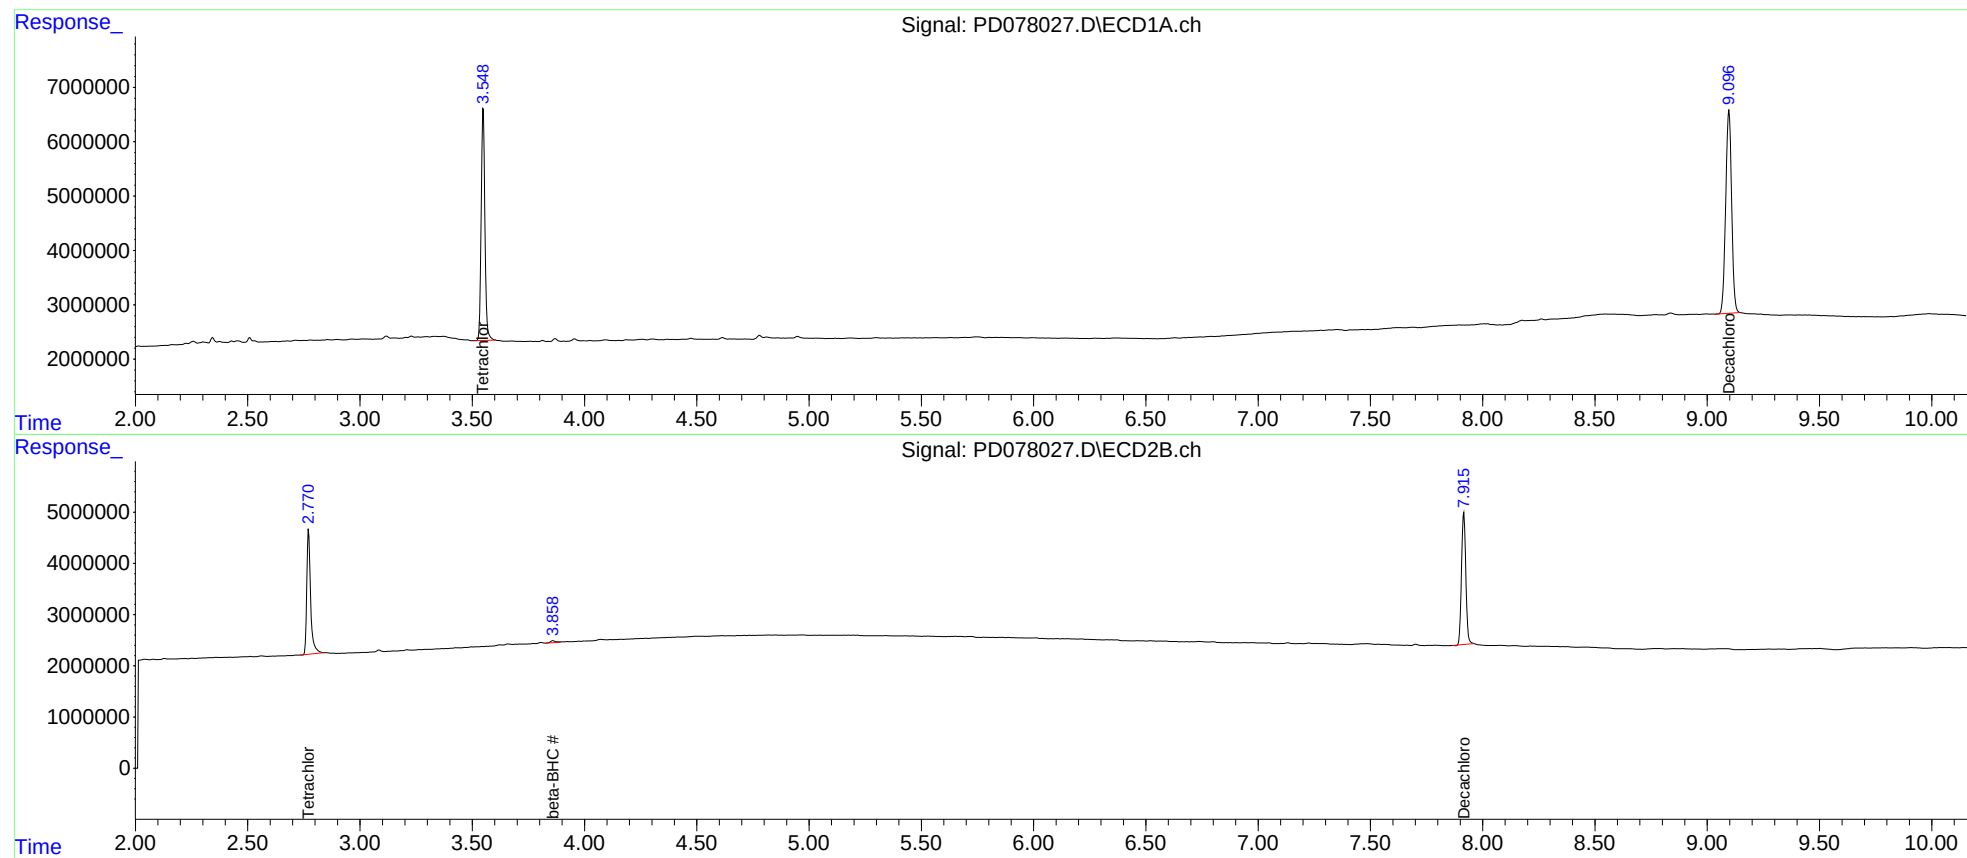

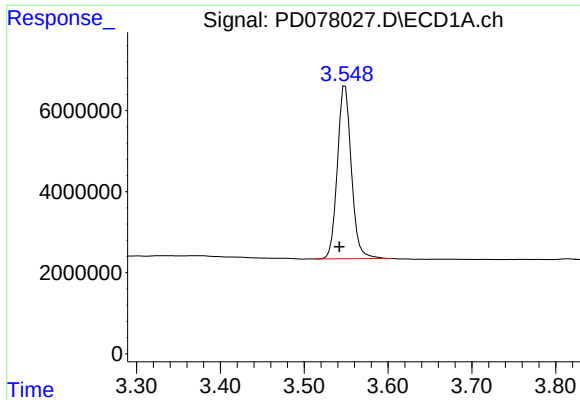


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: 0.007 min
Response: 49542800
Conc: 19.52 ng/ml

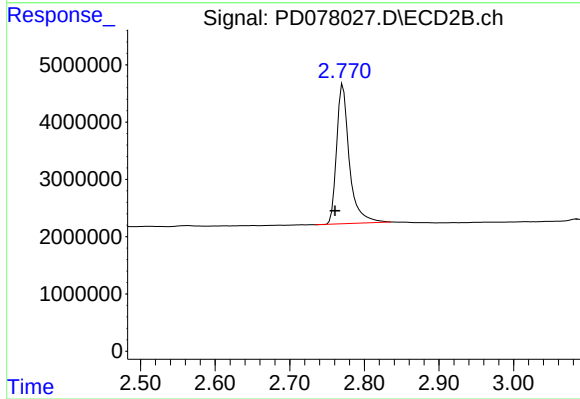


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.011 min
Response: 28902739
Conc: 19.56 ng/ml

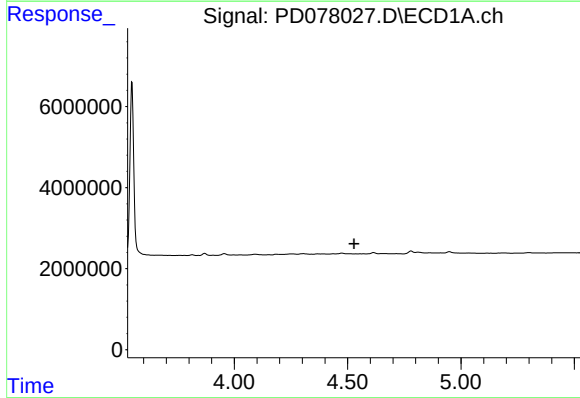


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

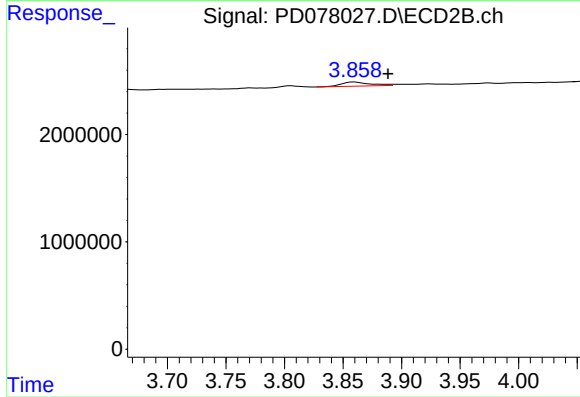


#6 beta-BHC

R.T.: 3.860 min
Delta R.T.: -0.029 min
Response: 674801
Conc: 0.68 ng/ml

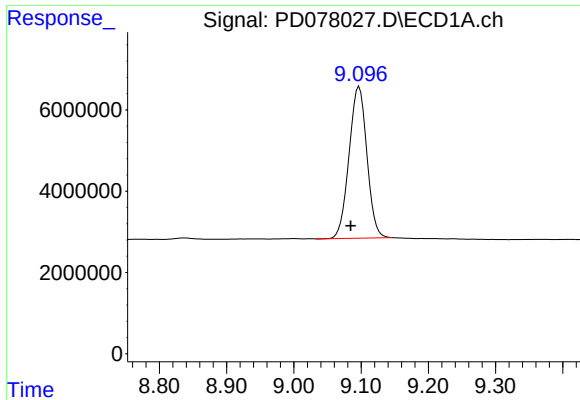

#27 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.012 min
Response: 68715819
Conc: 22.00 ng/ml

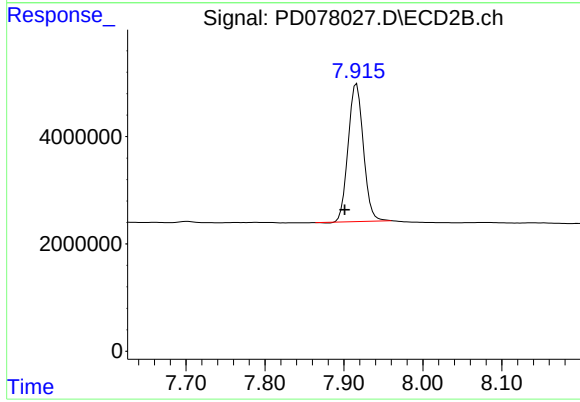

#27 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.015 min
Response: 34437016
Conc: 21.26 ng/ml