

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
 Data File : PD078036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2023 16:00
 Operator : AR\AJ
 Sample : PIBLK280
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 20:16:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.759	47782555	28571200	18.829	19.333
27)	SA Decachlor...	9.088	7.901	116.8E6	61846762	37.384	38.188
Target Compounds							
3)	MA gamma-BHC...	0.000	3.603	0	28532	N.D.	<MDL
4)	MA Heptachlor	0.000	3.915	0	45863	N.D.	<MDL
5)	MB Aldrin	0.000	4.216	0	583078	N.D.	0.260
6)	B beta-BHC	0.000	3.894	0	191963	N.D.	0.194
7)	B delta-BHC	4.767	0.000	3279771	0	0.817	N.D. #
8)	B Heptachlo...	0.000	4.645f	0	35881	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
Data File : PD078036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2023 16:00
Operator : AR\AJ
Sample : PIBLK280
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 20:16:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

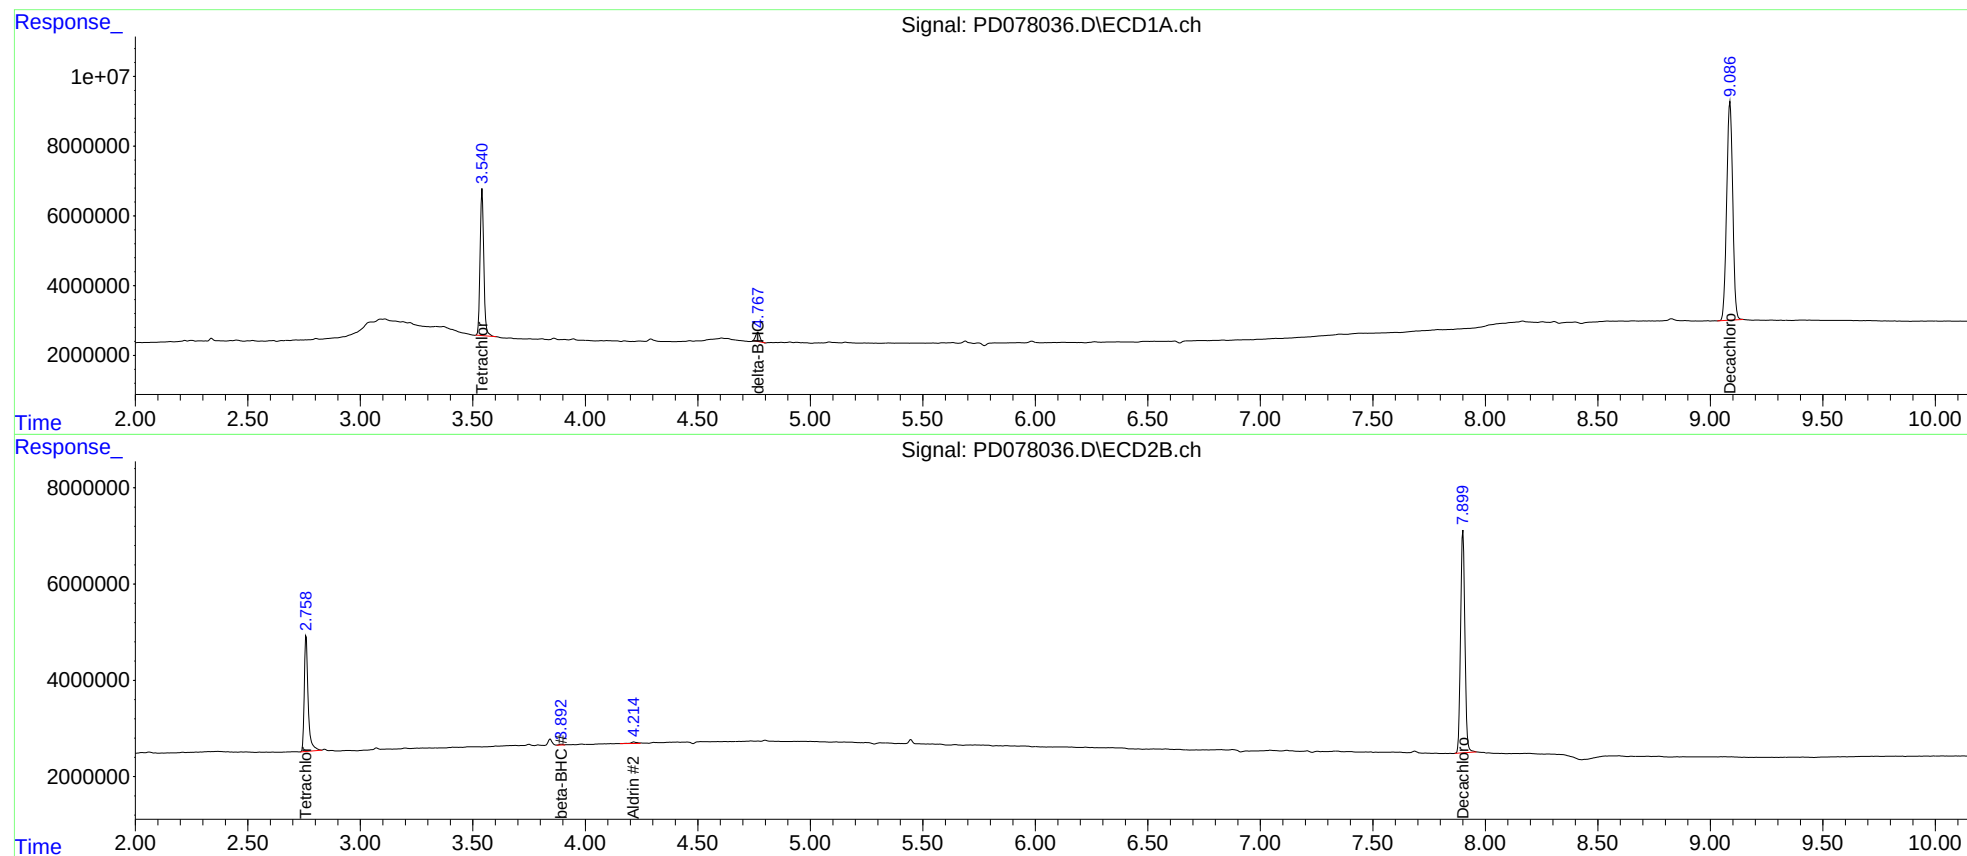

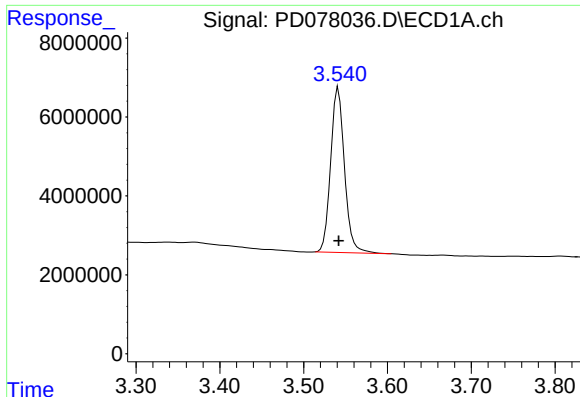


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 47782555
Conc: 18.83 ng/ml

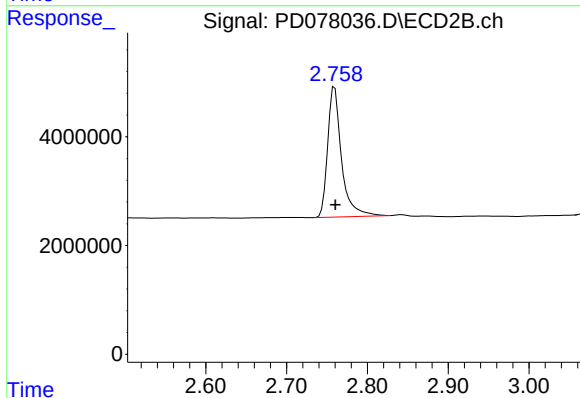


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: -0.001 min
Response: 28571200
Conc: 19.33 ng/ml

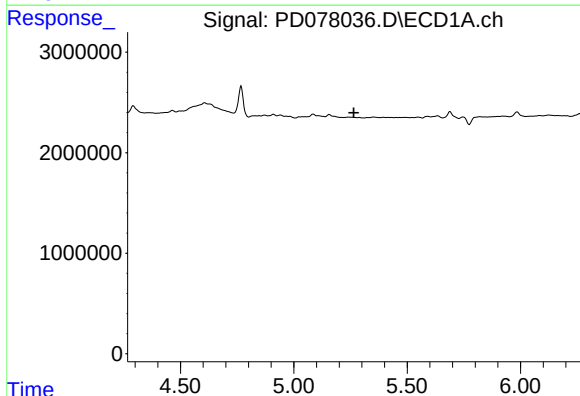


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.264 min
Response: 0
Conc: N.D.

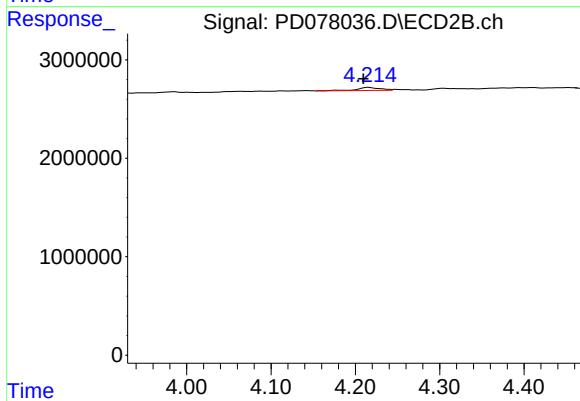


#5 Aldrin

R.T.: 4.216 min
Delta R.T.: 0.006 min
Response: 583078
Conc: 0.26 ng/ml

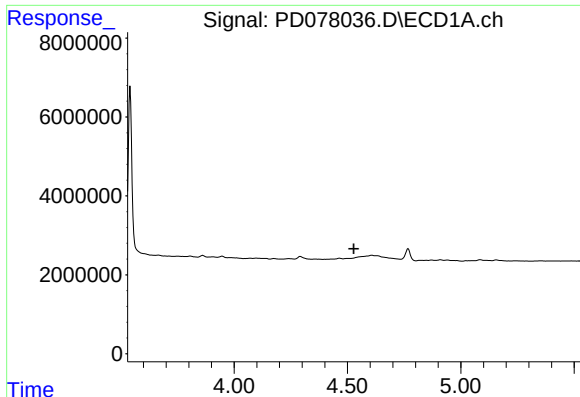


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

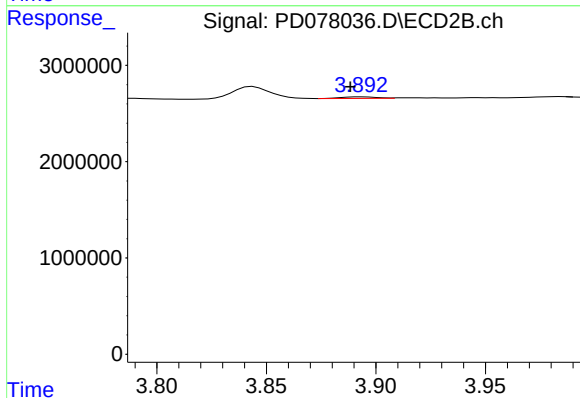


#6 beta-BHC

R.T.: 3.894 min
Delta R.T.: 0.005 min
Response: 191963
Conc: 0.19 ng/ml

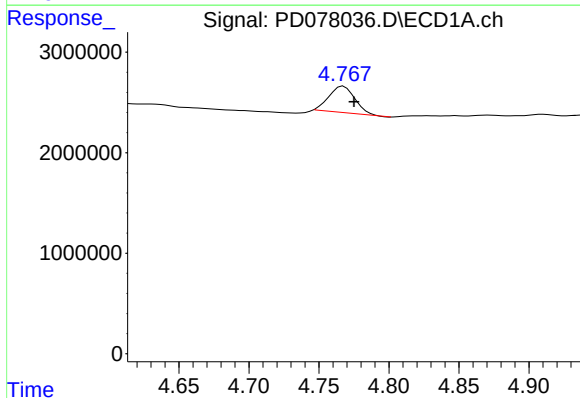


#7 delta-BHC

R.T.: 4.767 min
Delta R.T.: -0.008 min
Response: 3279771
Conc: 0.82 ng/ml

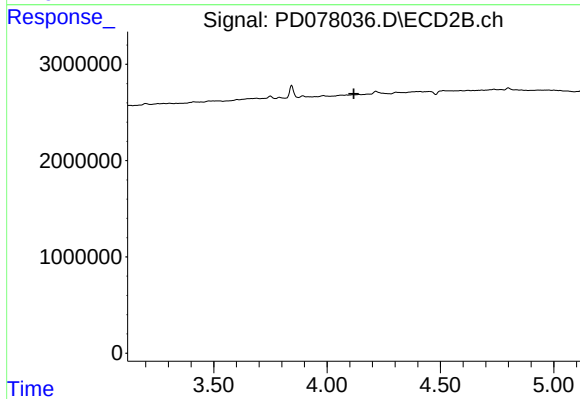


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.118 min
Response: 0
Conc: N.D.

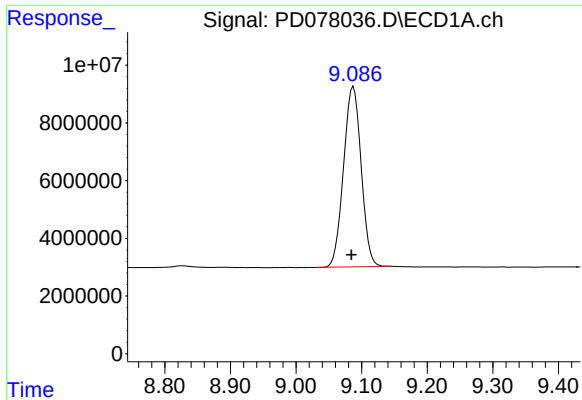

#27 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.003 min
Response: 116784916
Conc: 37.38 ng/ml

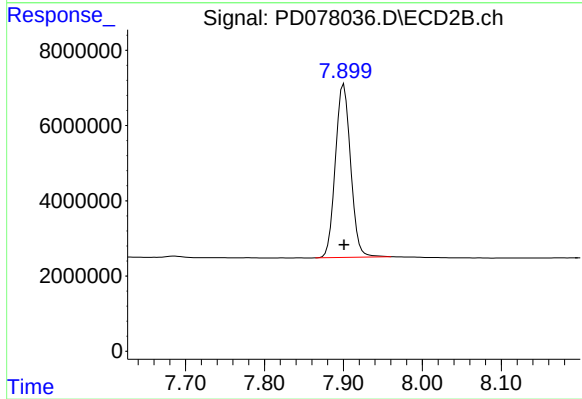

#27 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 61846762
Conc: 38.19 ng/ml