

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
 Data File : PD078056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2023 20:49
 Operator : AR\AJ
 Sample : 04385-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:11:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.759	58802473	35167518	23.172	23.796
27)	SA Decachlor...	9.083	7.898	54294703	27178160	17.380	16.782
Target Compounds							
6)	B beta-BHC	0.000	3.844f	0	408878	N.D.	0.414


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
Data File : PD078056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2023 20:49
Operator : AR\AJ
Sample : 04385-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:11:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

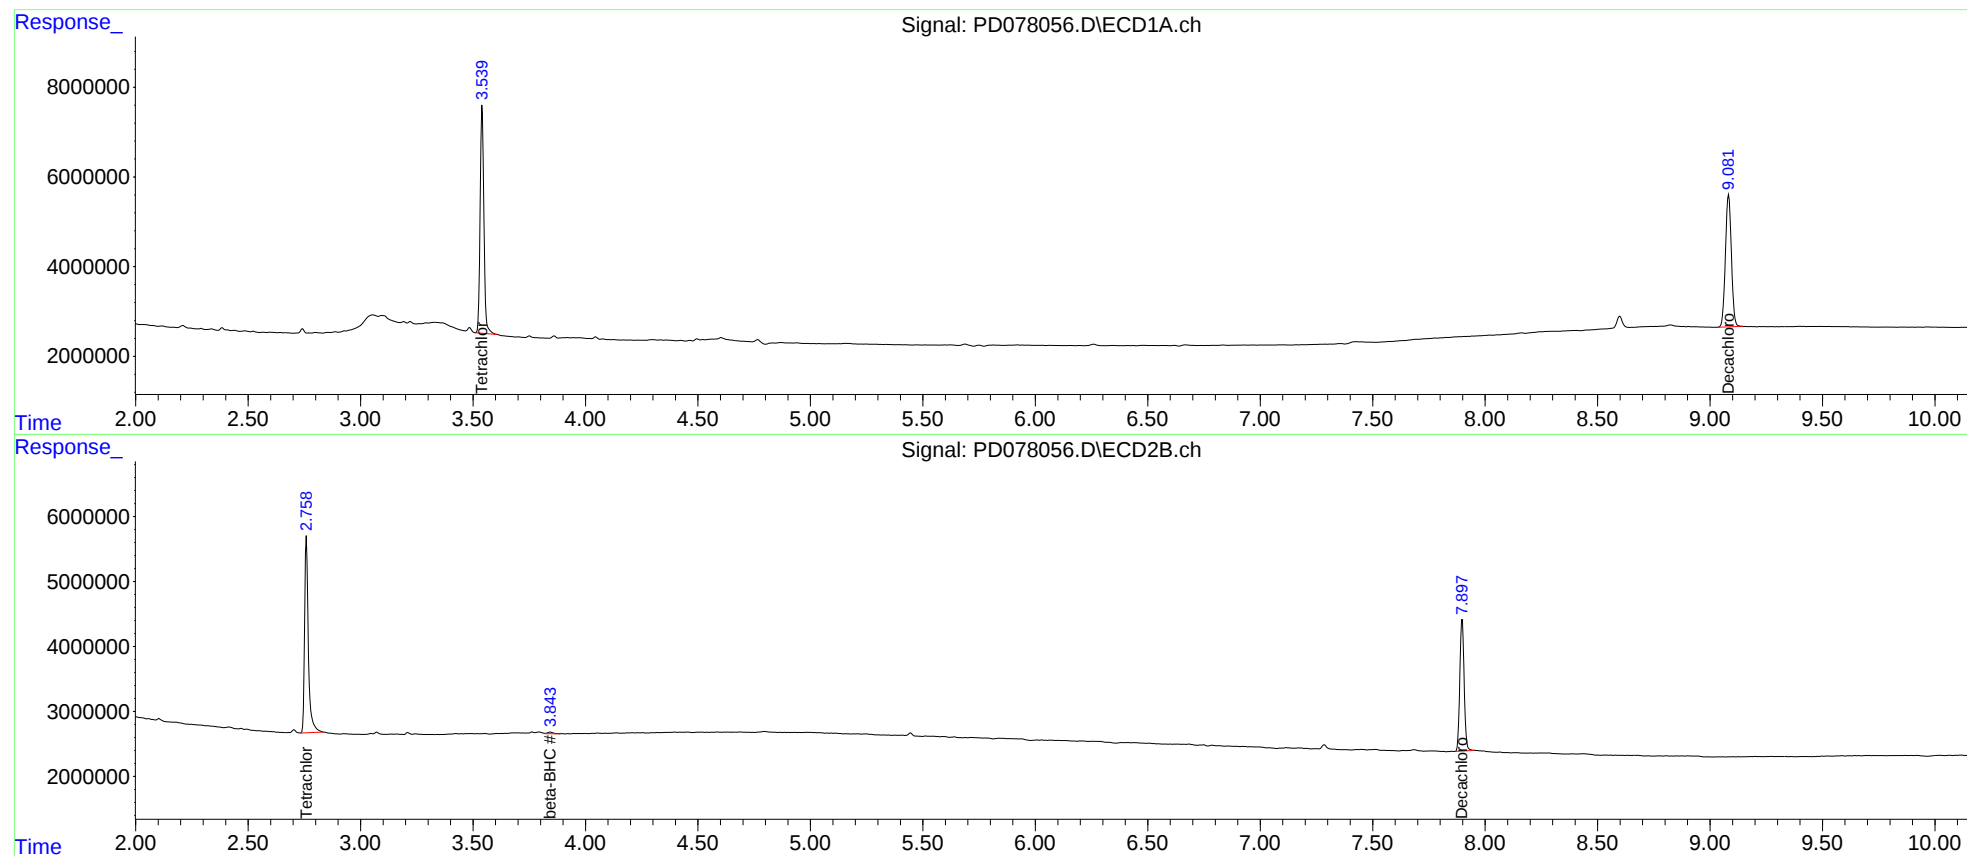

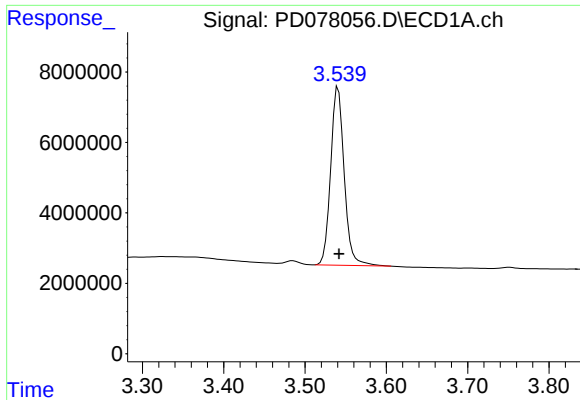


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: -0.001 min
Response: 58802473
Conc: 23.17 ng/ml

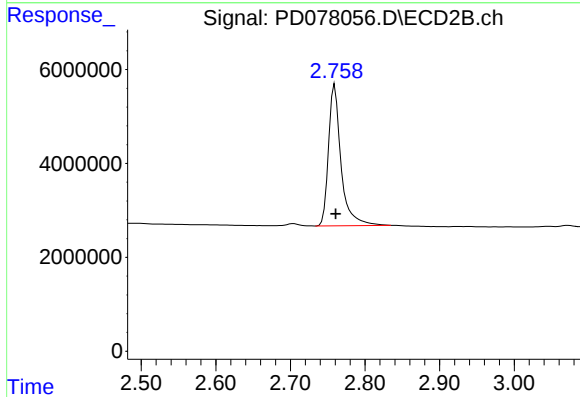


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: -0.001 min
Response: 35167518
Conc: 23.80 ng/ml

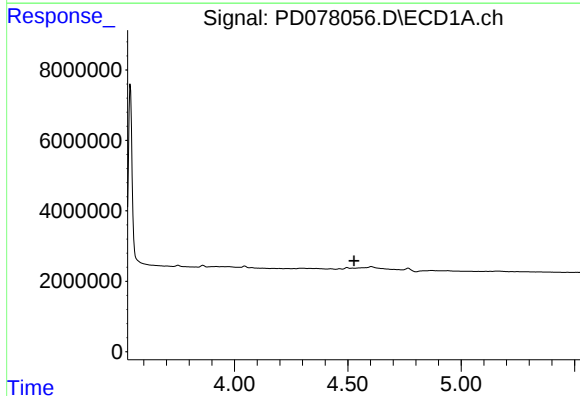


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

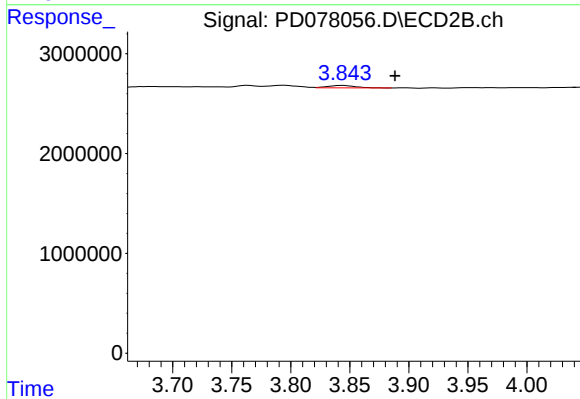


#6 beta-BHC

R.T.: 3.844 min
Delta R.T.: -0.044 min
Response: 408878
Conc: 0.41 ng/ml

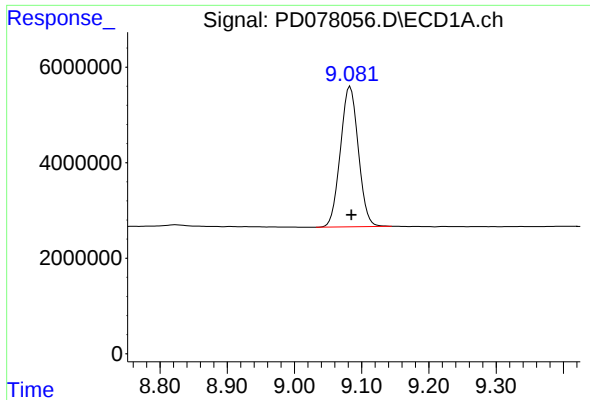

#27 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.002 min
Response: 54294703
Conc: 17.38 ng/ml

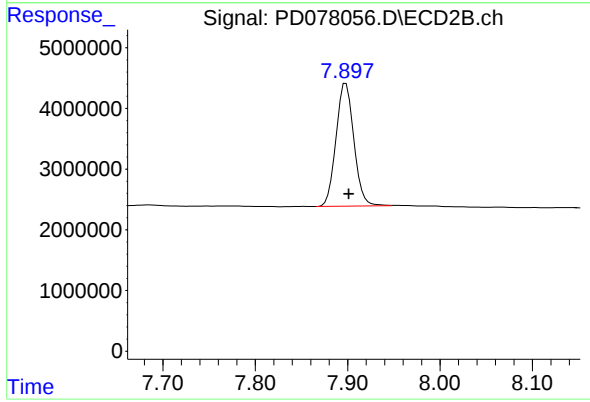

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 27178160
Conc: 16.78 ng/ml