

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
 Data File : PD078090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 04:23
 Operator : AR\AJ
 Sample : 04429-19
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:47:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	54778492	34027927	21.586	23.025
27)	SA Decachlor...	9.082	7.898	63996077	33184295	20.486	20.490
Target Compounds							
3)	MA gamma-BHC...	4.325	0.000	2393875	0	0.592	N.D. #
6)	B beta-BHC	0.000	3.846f	0	531738	N.D.	0.538
8)	B Heptachlo...	0.000	4.703	0	369925	N.D.	0.176
9)	A Endosulfan I	0.000	5.036f	0	239366	N.D.	0.133
11)	B cis-Chlor...	0.000	5.036	0	239366	N.D.	0.117
15)	B Endosulfa...	0.000	5.851f	0	513699	N.D.	0.284
19)	B Endosulfa...	0.000	6.252f	0	545602	N.D.	0.330
22)	Toxaphene-1	0.000	5.036f	0	239366	N.D.	22.933


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
Data File : PD078090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 04:23
Operator : AR\AJ
Sample : 04429-19
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:47:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

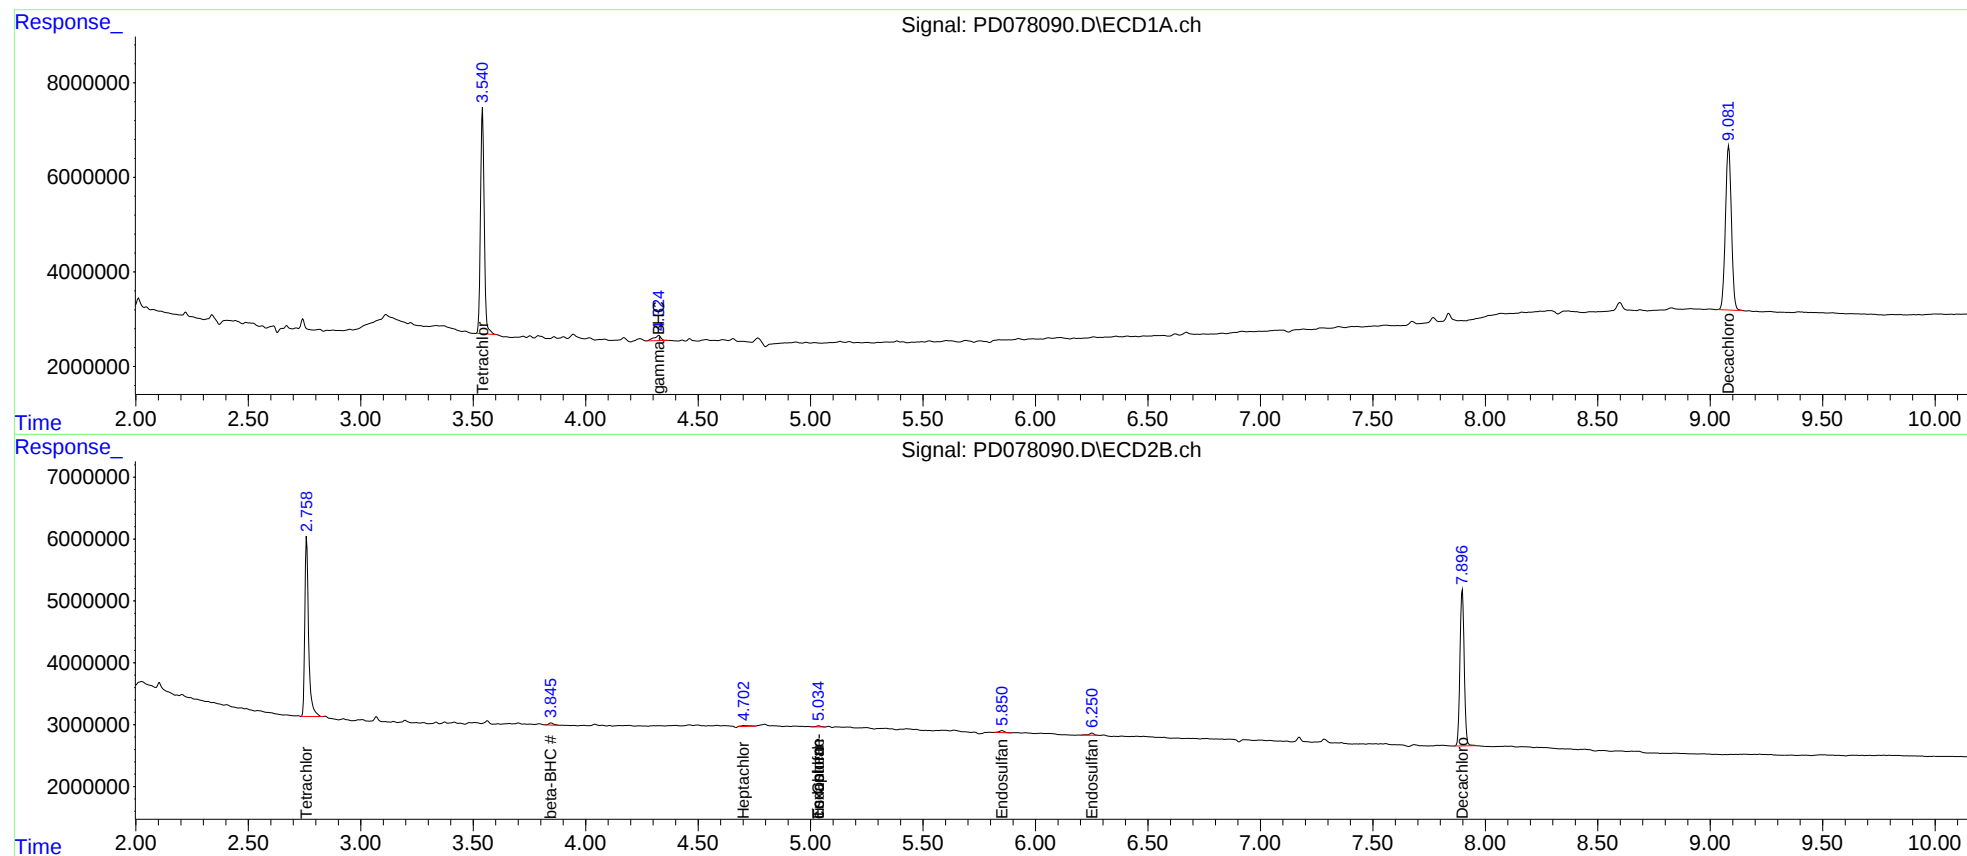

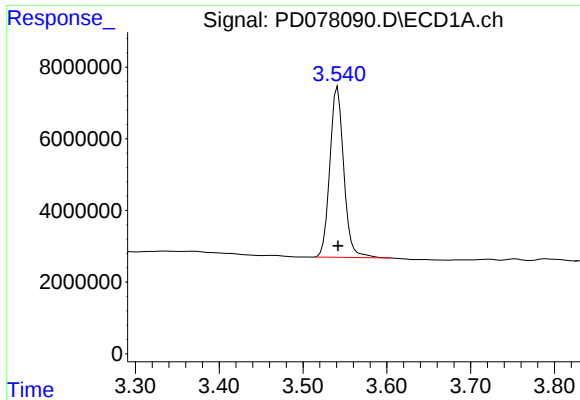


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 54778492
Conc: 21.59 ng/ml

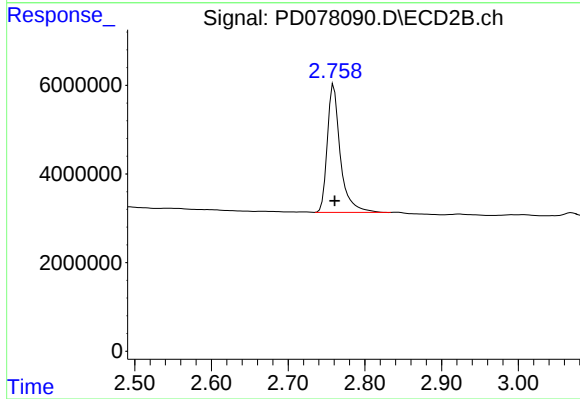


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: -0.001 min
Response: 34027927
Conc: 23.02 ng/ml

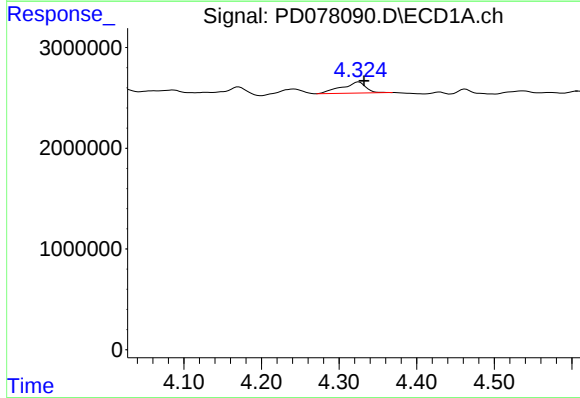


#3 gamma-BHC (Lindane)

R.T.: 4.325 min
Delta R.T.: -0.007 min
Response: 2393875
Conc: 0.59 ng/ml

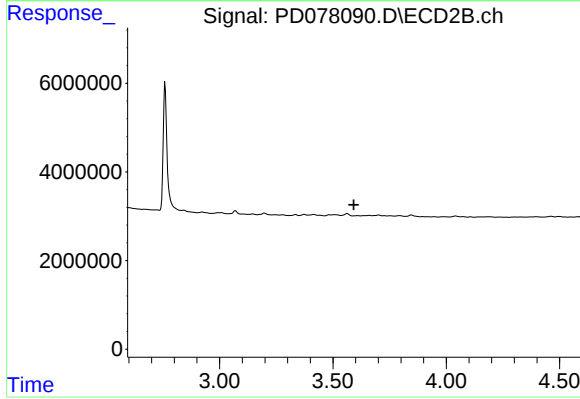


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.592 min
Response: 0
Conc: N.D.

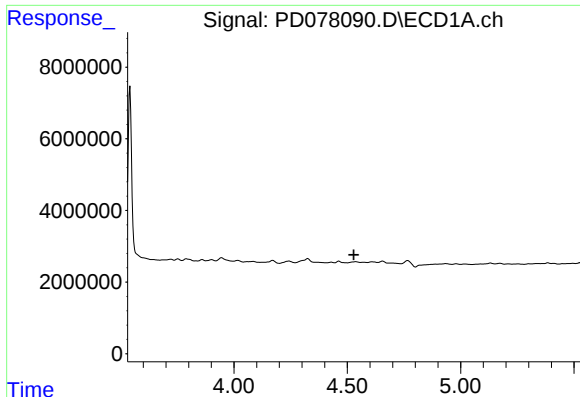


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

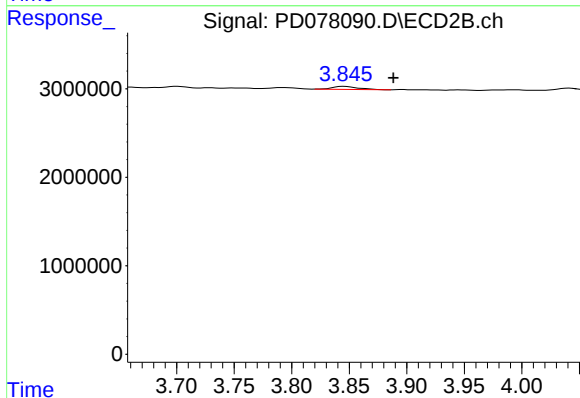


#6 beta-BHC

R.T.: 3.846 min
Delta R.T.: -0.042 min
Response: 531738
Conc: 0.54 ng/ml

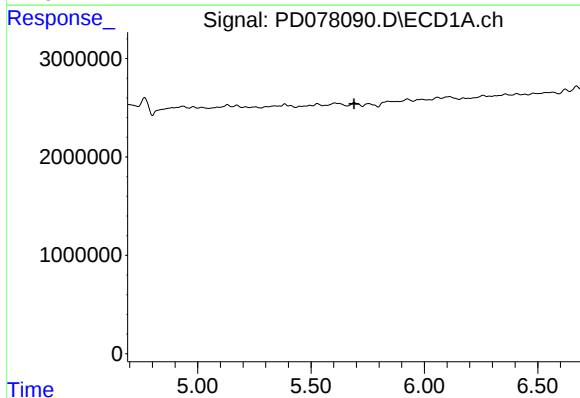


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.690 min
Response: 0
Conc: N.D.

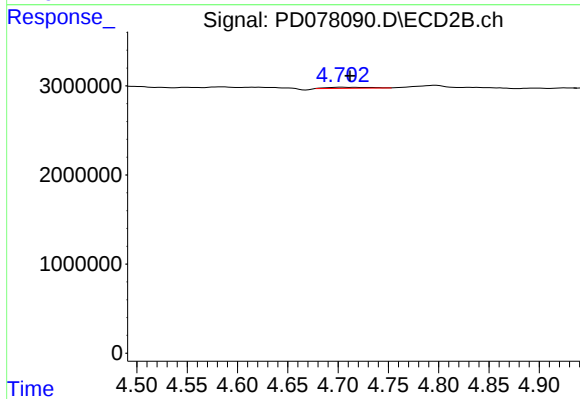


#8 Heptachlor epoxide

R.T.: 4.703 min
Delta R.T.: -0.008 min
Response: 369925
Conc: 0.18 ng/ml

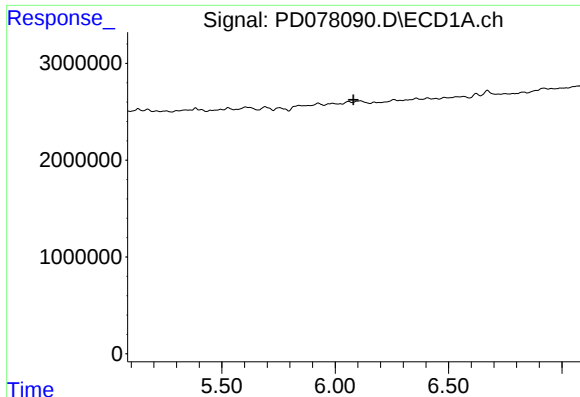


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.081 min
Response: 0
Conc: N.D.

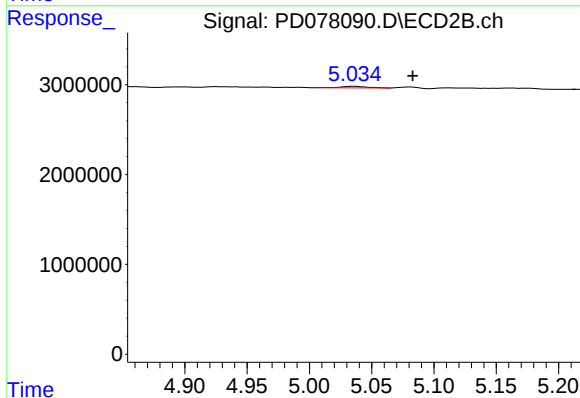


#9 Endosulfan I

R.T.: 5.036 min
Delta R.T.: -0.047 min
Response: 239366
Conc: 0.13 ng/ml

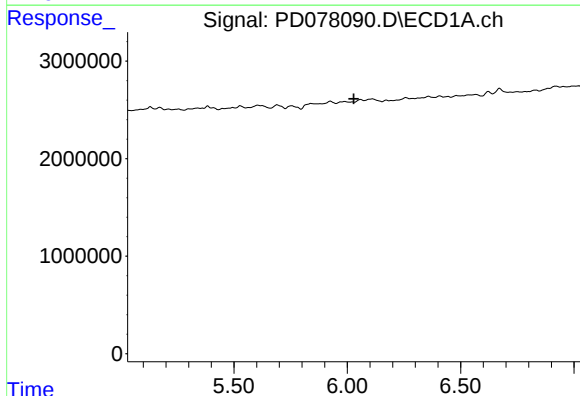


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.029 min
Response: 0
Conc: N.D.

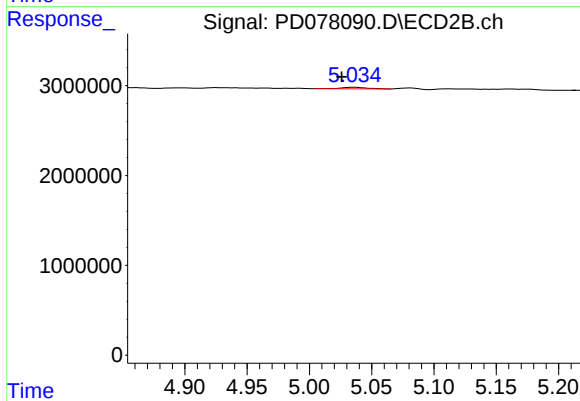


#11 cis-Chlordane

R.T.: 5.036 min
Delta R.T.: 0.010 min
Response: 239366
Conc: 0.12 ng/ml

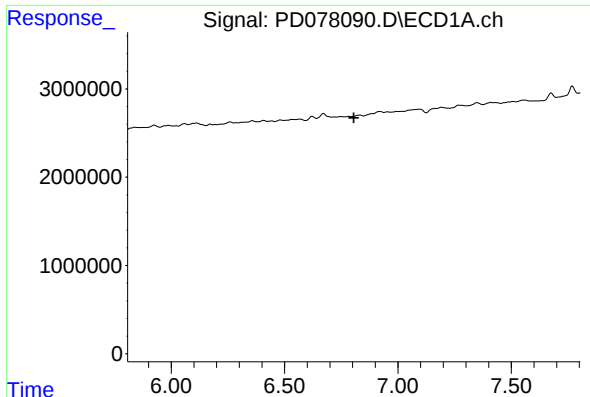


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.806 min
Response: 0
Conc: N.D.

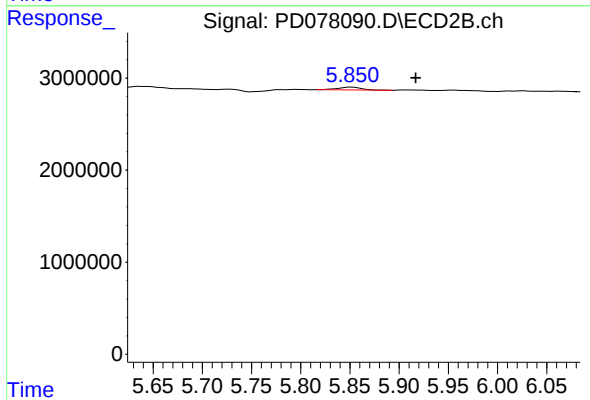


#15 Endosulfan II

R.T.: 5.851 min
Delta R.T.: -0.066 min
Response: 513699
Conc: 0.28 ng/ml

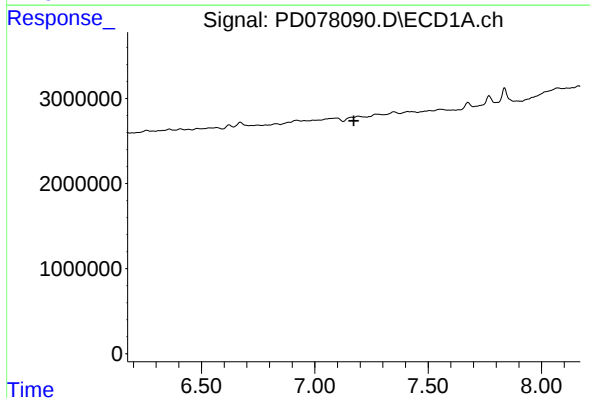


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

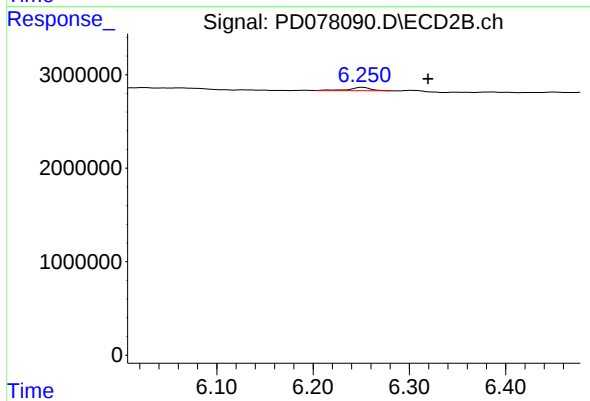


#19 Endosulfan Sulfate

R.T.: 6.252 min
Delta R.T.: -0.067 min
Response: 545602
Conc: 0.33 ng/ml

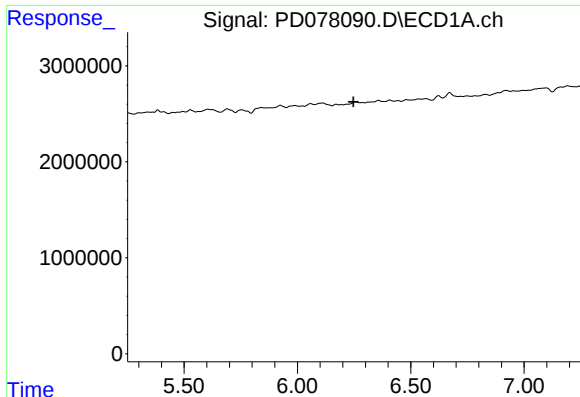


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 6.247 min
Response: 0
Conc: N.D.

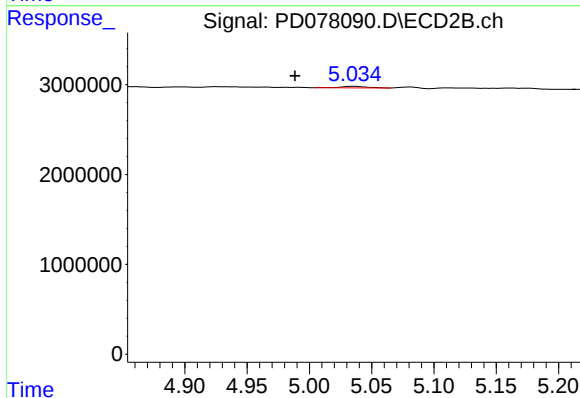


#22 Toxaphene-1

R.T.: 5.036 min
Delta R.T.: 0.047 min
Response: 239366
Conc: 22.93 ng/ml

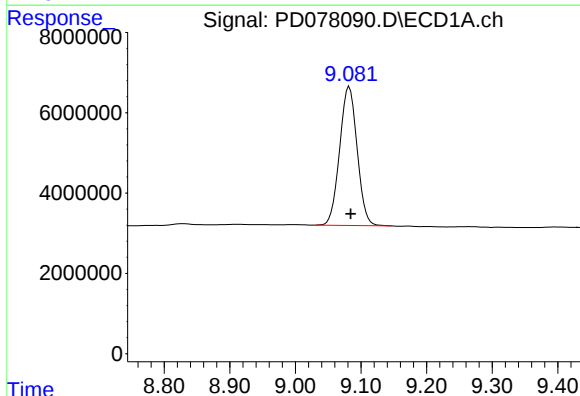

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.003 min
Response: 63996077
Conc: 20.49 ng/ml

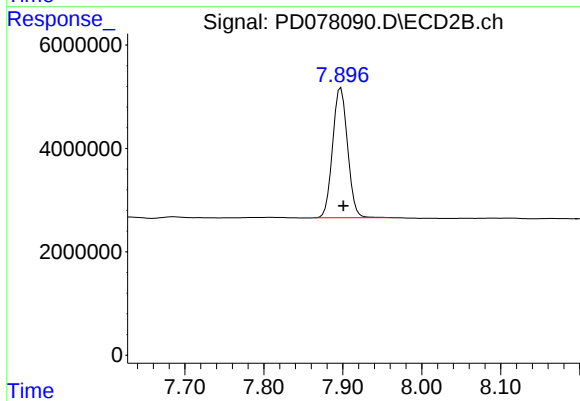

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 33184295
Conc: 20.49 ng/ml