

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
 Data File : PD078091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 04:36
 Operator : AR\AJ
 Sample : 04429-20
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:47:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.759	56208263	34659275	22.149	23.452
27)	SA Decachlor...	9.083	7.898	71787142	37087370	22.980	22.900
Target Compounds							
3)	MA gamma-BHC...	4.325	0.000	5460304	0	1.350	N.D. #
4)	MA Heptachlor	4.937	0.000	1250529	0	0.299	N.D. #
5)	MB Aldrin	0.000	4.190	0	444053	N.D.	0.198
6)	B beta-BHC	0.000	3.846f	0	696720	N.D.	0.705
7)	B delta-BHC	0.000	4.128	0	163180	N.D.	<MDL
19)	B Endosulfa...	0.000	6.253f	0	404865	N.D.	0.245


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
Data File : PD078091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 04:36
Operator : AR\AJ
Sample : 04429-20
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:47:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

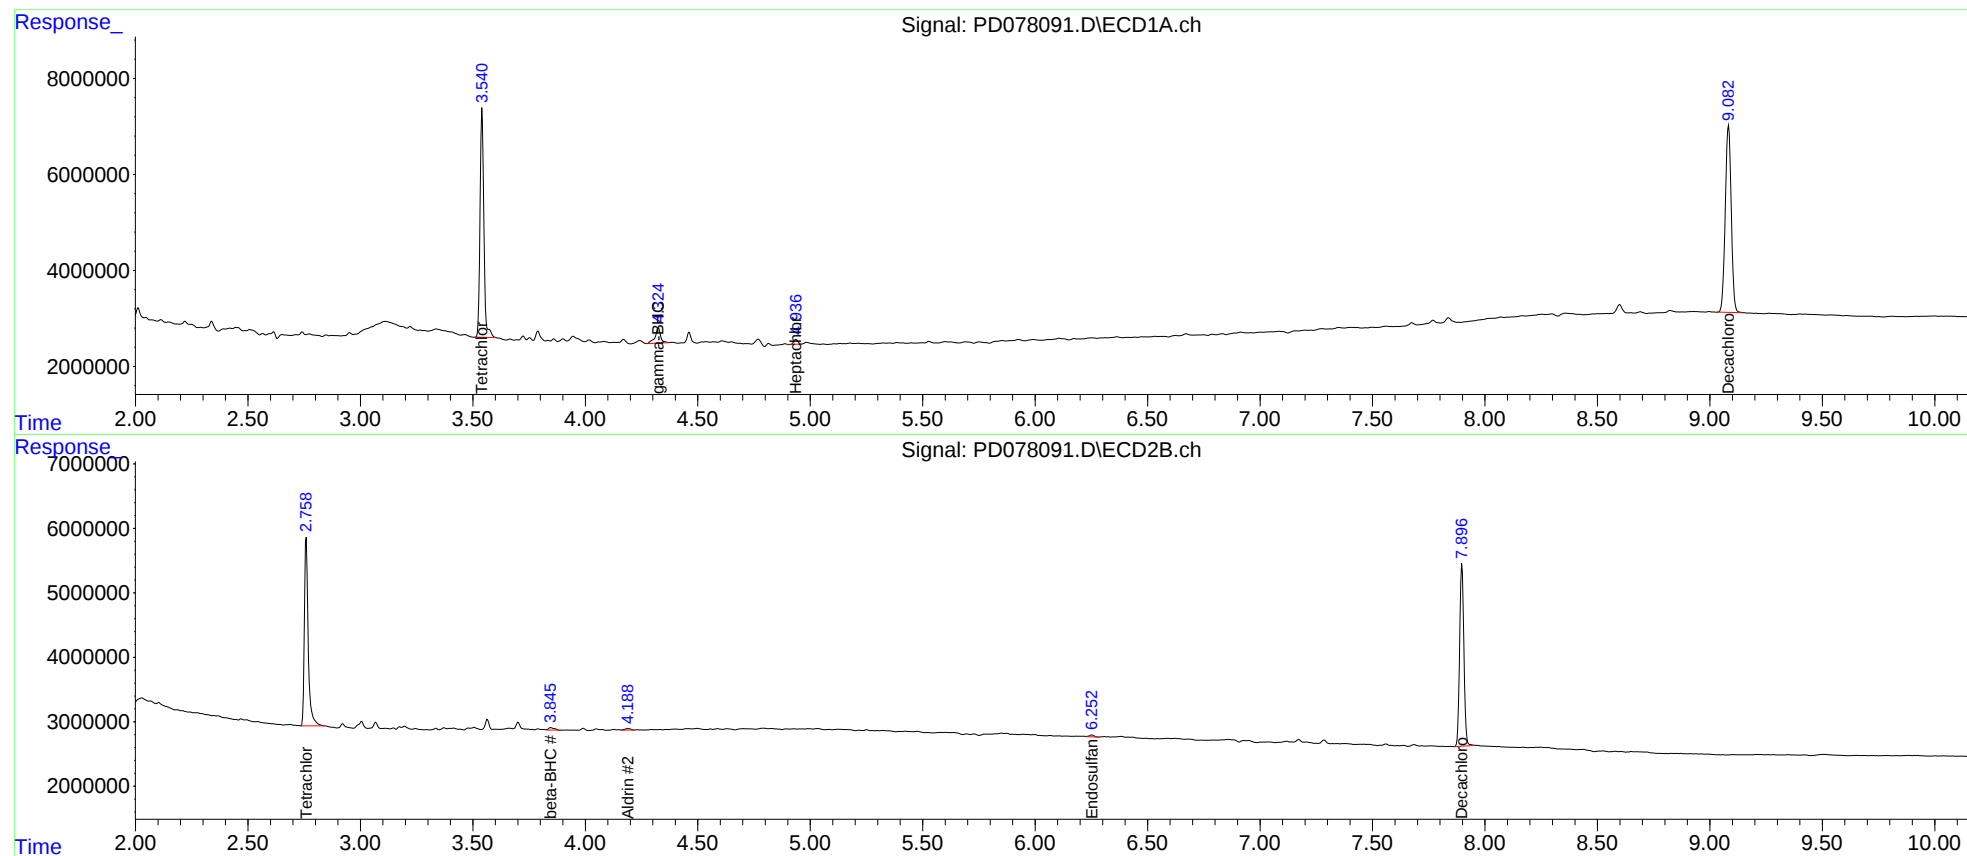

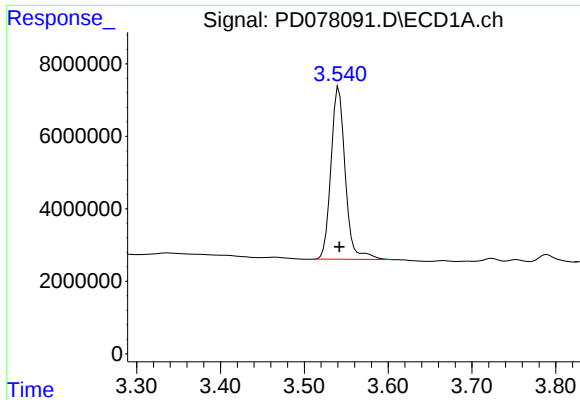


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 56208263
Conc: 22.15 ng/ml

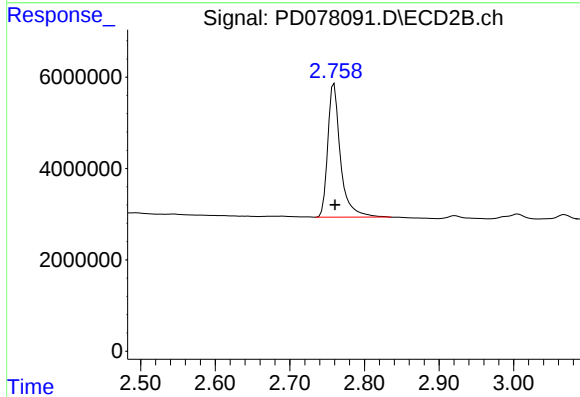


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: -0.001 min
Response: 34659275
Conc: 23.45 ng/ml

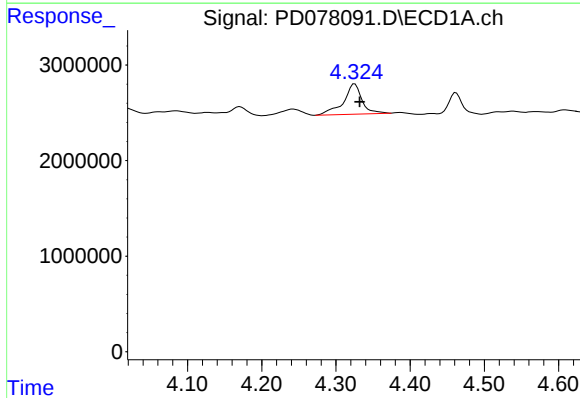


#3 gamma-BHC (Lindane)

R.T.: 4.325 min
Delta R.T.: -0.007 min
Response: 5460304
Conc: 1.35 ng/ml

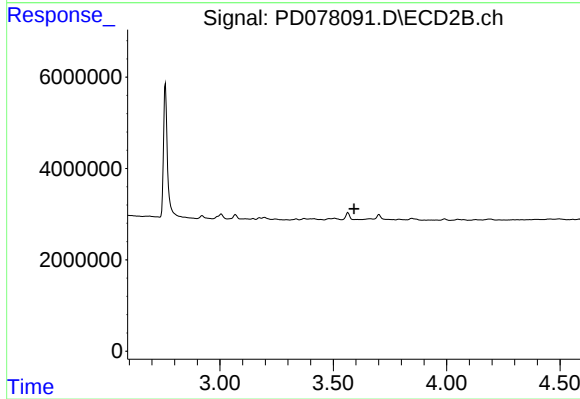


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 3.592 min
Response: 0
Conc: N.D.

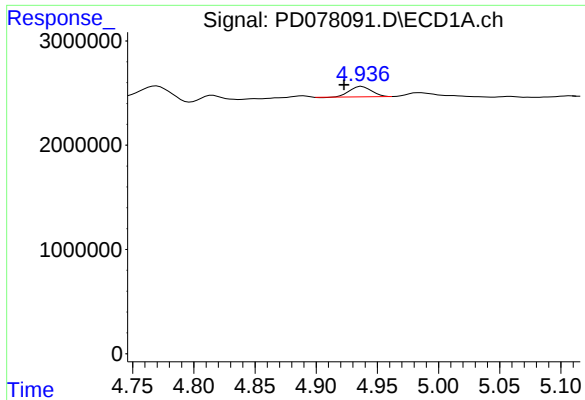


#4 Heptachlor

R.T.: 4.937 min
Delta R.T.: 0.015 min
Response: 1250529
Conc: 0.30 ng/ml

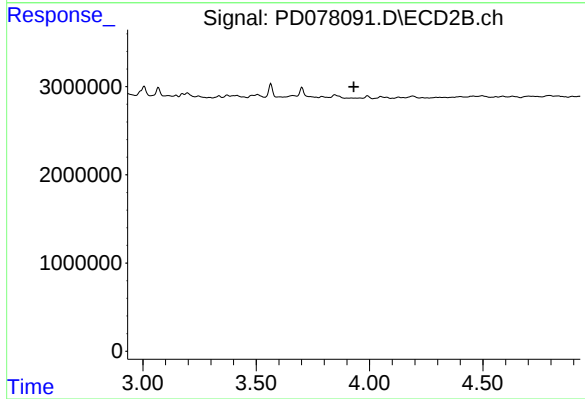


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.931 min
Response: 0
Conc: N.D.

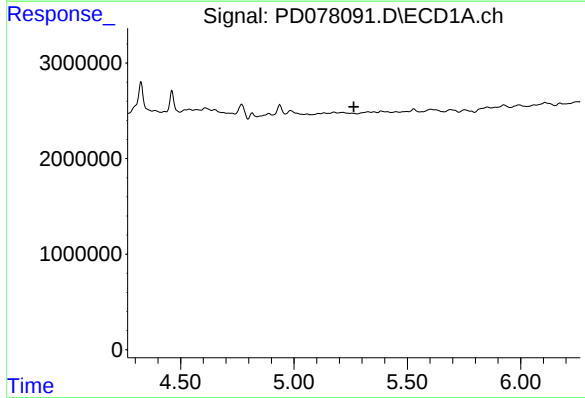


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.264 min
Response: 0
Conc: N.D.

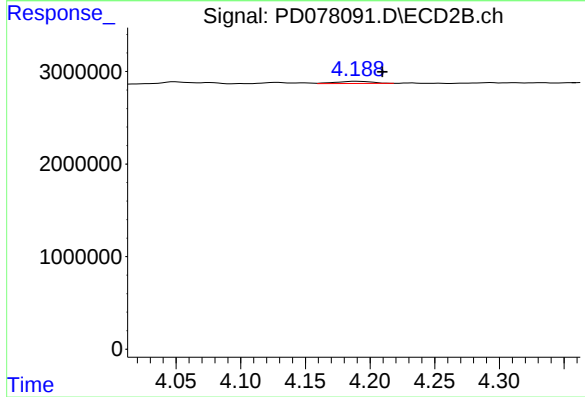


#5 Aldrin

R.T.: 4.190 min
Delta R.T.: -0.020 min
Response: 444053
Conc: 0.20 ng/ml

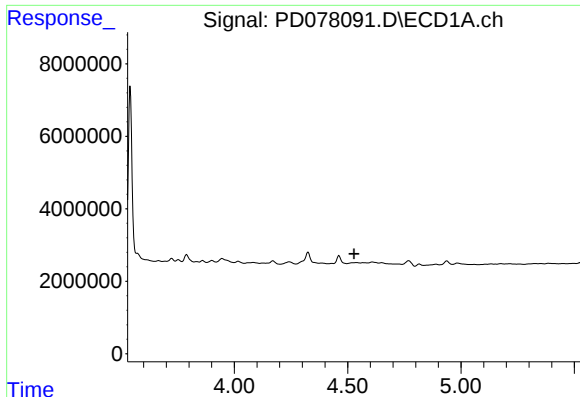


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.528 min
Response: 0
Conc: N.D.

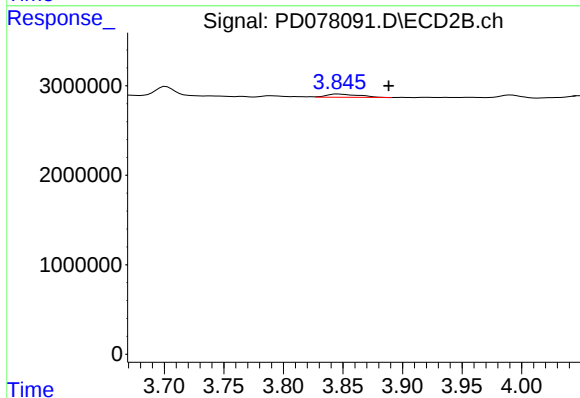


#6 beta-BHC

R.T.: 3.846 min
Delta R.T.: -0.042 min
Response: 696720
Conc: 0.71 ng/ml

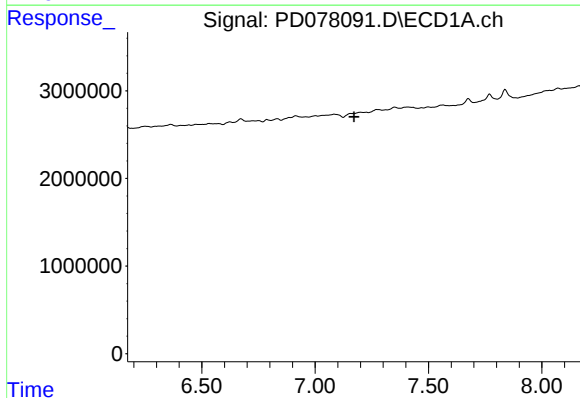


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

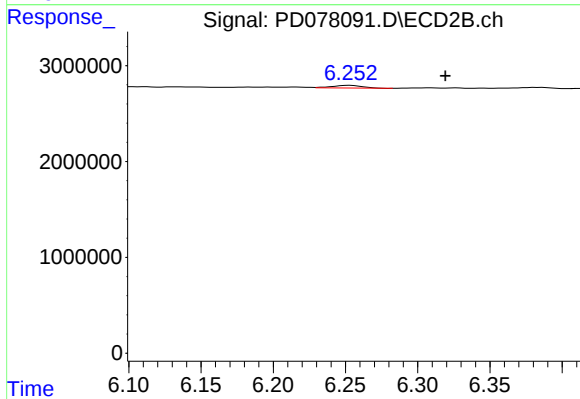


#19 Endosulfan Sulfate

R.T.: 6.253 min
Delta R.T.: -0.066 min
Response: 404865
Conc: 0.25 ng/ml

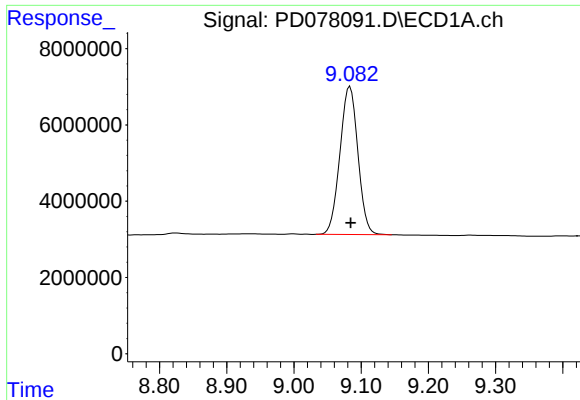

#27 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.001 min
Response: 71787142
Conc: 22.98 ng/ml

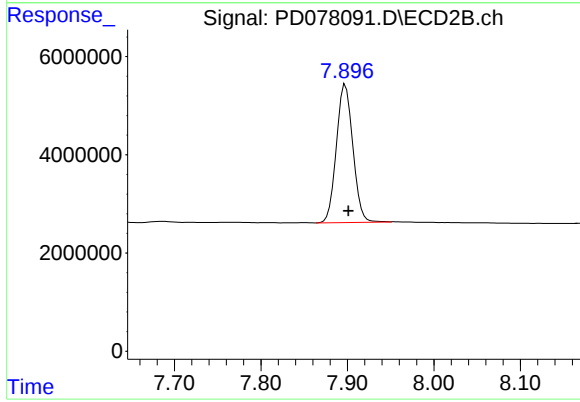

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 37087370
Conc: 22.90 ng/ml