

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
 Data File : PD078043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2023 17:55
 Operator : AR\AJ
 Sample : 04410-12MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBJM0MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 20:19:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.760	50513734	30605373	19.905	20.709
2)	SA Decachlor...	9.084	7.898	62624514	31788639	20.047	19.628
Target Compounds							
2)	A alpha-BHC	3.998	3.261	115.4E6	62438818	26.948	27.546
3)	MA gamma-BHC...	4.332	3.591	106.9E6	55003461	26.436	25.475
4)	MA Heptachlor	4.923	3.930	105.7E6	59485303	25.286	26.756
5)	MB Aldrin	5.266	4.209	104.4E6	56312306	25.010	25.124
6)	B beta-BHC	4.529	3.888	43605814	24476891	23.735	24.772
7)	B delta-BHC	4.777	4.117	101.0E6	56141689	25.141	25.187
8)	B Heptachlo...	5.693	4.711	97660034	53711410	25.270	25.571
9)	A Endosulfan I	6.080	5.081	89055404	52879704	26.531	29.460
10)	B trans-Chl...	5.950	4.961	93373311	52574850	25.078	26.328
11)	B cis-Chlor...	6.029	5.026	94605079	55055133	24.547	26.922
12)	B 4,4'-DDE	6.202	5.214	183.4E6	99364075	51.742	52.306
13)	MA Dieldrin	6.356	5.346	198.8E6	111.2E6	53.101	53.813
14)	MA Endrin	6.587	5.622	169.0E6	100.8E6	54.774	55.120
15)	B Endosulfa...	6.807	5.917	166.7E6	95937464	50.353	53.013
16)	A 4,4'-DDD	6.720	5.769	143.4E6	78438503	53.912	58.277
17)	MA 4,4'-DDT	7.036	6.020	154.7E6	82659183	56.469	58.484
18)	B Endrin al...	6.937	6.096	121.8E6	68948692	46.855	49.016
19)	B Endosulfa...	7.173	6.319	153.5E6	88575326	50.641	53.609
20)	A Methoxychlor	7.512	6.595	414.3E6	225.5E6	265.632	289.026
21)	B Endrin ke...	7.659	6.825	172.2E6	103.9E6	50.025	54.251

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
Data File : PD078043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2023 17:55
Operator : AR\AJ
Sample : 04410-12MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 20:19:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

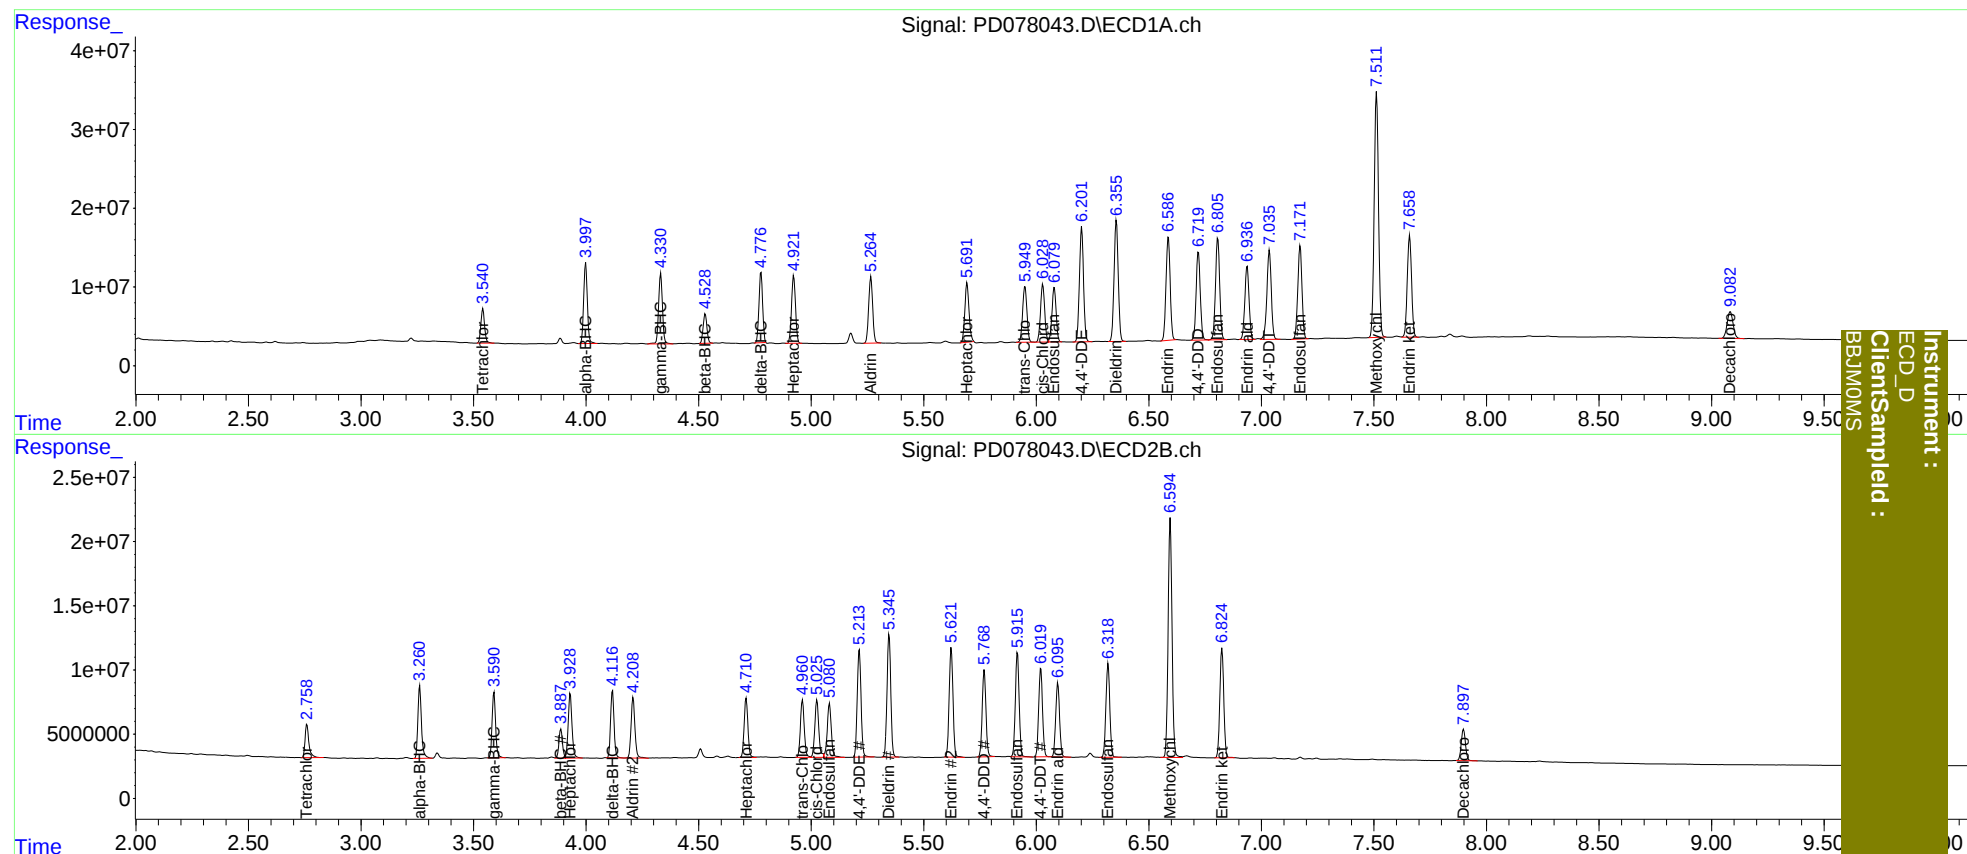

Instrument :
ECD_D
ClientSampled :
BBJMONS