

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
 Data File : PD078084.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 03:03
 Operator : AR\AJ
 Sample : 04429-13MS
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBKK1MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2023
 Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:42:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.764	68523620	26218621	27.002m	17.741m#
27)	SA Decachlor...	9.083	7.897	41199643	19056098	13.189	11.767m
Target Compounds							
2)	A alpha-BHC	3.998	3.260	65320259	40388955	15.255	17.818
3)	MA gamma-BHC...	4.332	3.592	77051068	52565816	19.057	24.346 #
4)	MA Heptachlor	4.922	3.928	76949884	37940915	18.414m	17.065m
5)	MB Aldrin	5.265	4.209	74202856	39442758	17.774	17.597
6)	B beta-BHC	4.527	3.884	42719476	24890446	23.253	25.191m
7)	B delta-BHC	4.777	4.117	91870960	36894579	22.880	16.552 #
8)	B Heptachlo...	5.693	4.711	63834763	46910532	16.517	22.333 #
9)	A Endosulfan I	6.078	5.081	75144286	27083849	22.386m	15.089 #
10)	B trans-Chl...	5.951	4.961	112.5E6	31797598	30.215m	15.923 #
11)	B cis-Chlor...	6.025	5.026	98342463	34068849	25.517m	16.659 #
12)	B 4,4'-DDE	6.200	5.212	111.8E6	57896878	31.524m	30.478m
13)	MA Dieldrin	6.355	5.346	144.5E6	79805310	38.604	38.620
14)	MA Endrin	6.585	5.621	124.4E6	81177066	40.308m	44.400
15)	B Endosulfa...	6.806	5.916	157.6E6	62441510	47.606	34.504 #
16)	A 4,4'-DDD	6.720	5.769	106.2E6	34291058	39.927	25.477 #
17)	MA 4,4'-DDT	7.035	6.020	120.7E6	54961569	44.049	38.887
18)	B Endrin al...	6.936	6.095	85465449	45356605	32.890	32.244
19)	B Endosulfa...	7.172	6.318	135.5E6	65575783	44.705	39.689
20)	A Methoxychlor	7.512	6.595	329.0E6	176.3E6	210.910	225.975
21)	B Endrin ke...	7.658	6.825	147.3E6	79324394	42.780	41.401

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091823\
Data File : PD078084.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 03:03
Operator : AR\AJ
Sample : 04429-13MS
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:42:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

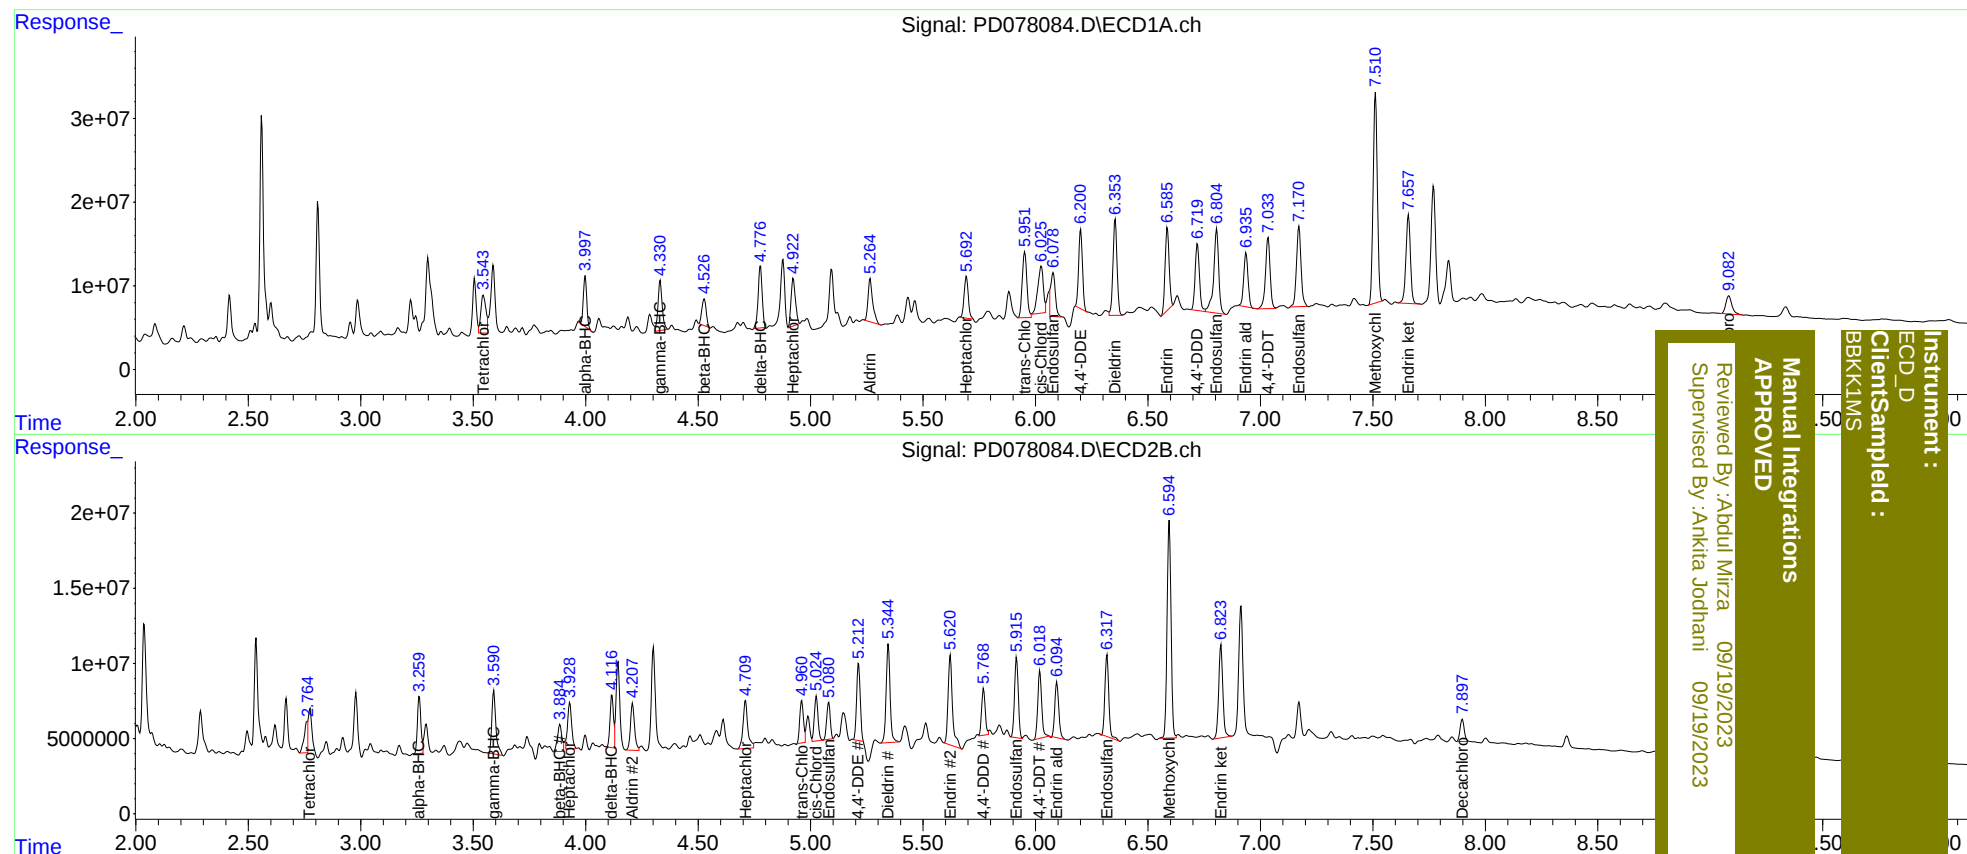

Instrument :
ECD_D
ClientSampled :
BBK1MS
Manual Integrations
APPROVED
Reviewed By :Abdul Mirza 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023