

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100224\
 Data File : PD085852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2024 10:30
 Operator : AR\AJ
 Sample : P4018-02RE
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCA0RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/02/2024
 Supervised By :Ankita Jodhani 10/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 20:57:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.440	2.889	14792262	1259.1E6	12.930m	296.916m#
2)	SA Decachlor...	8.890	8.062	24493937	29077099	13.468m	7.910 #
Target Compounds							
15)	B Endosulfa...	6.680	6.062	9821361	37233353	5.774m	8.193m#
16)	A 4,4'-DDD	6.591	5.916	72141940	80525509	57.847m	20.585 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100224\
Data File : PD085852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2024 10:30
Operator : AR\AJ
Sample : P4018-02RE
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 20:57:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

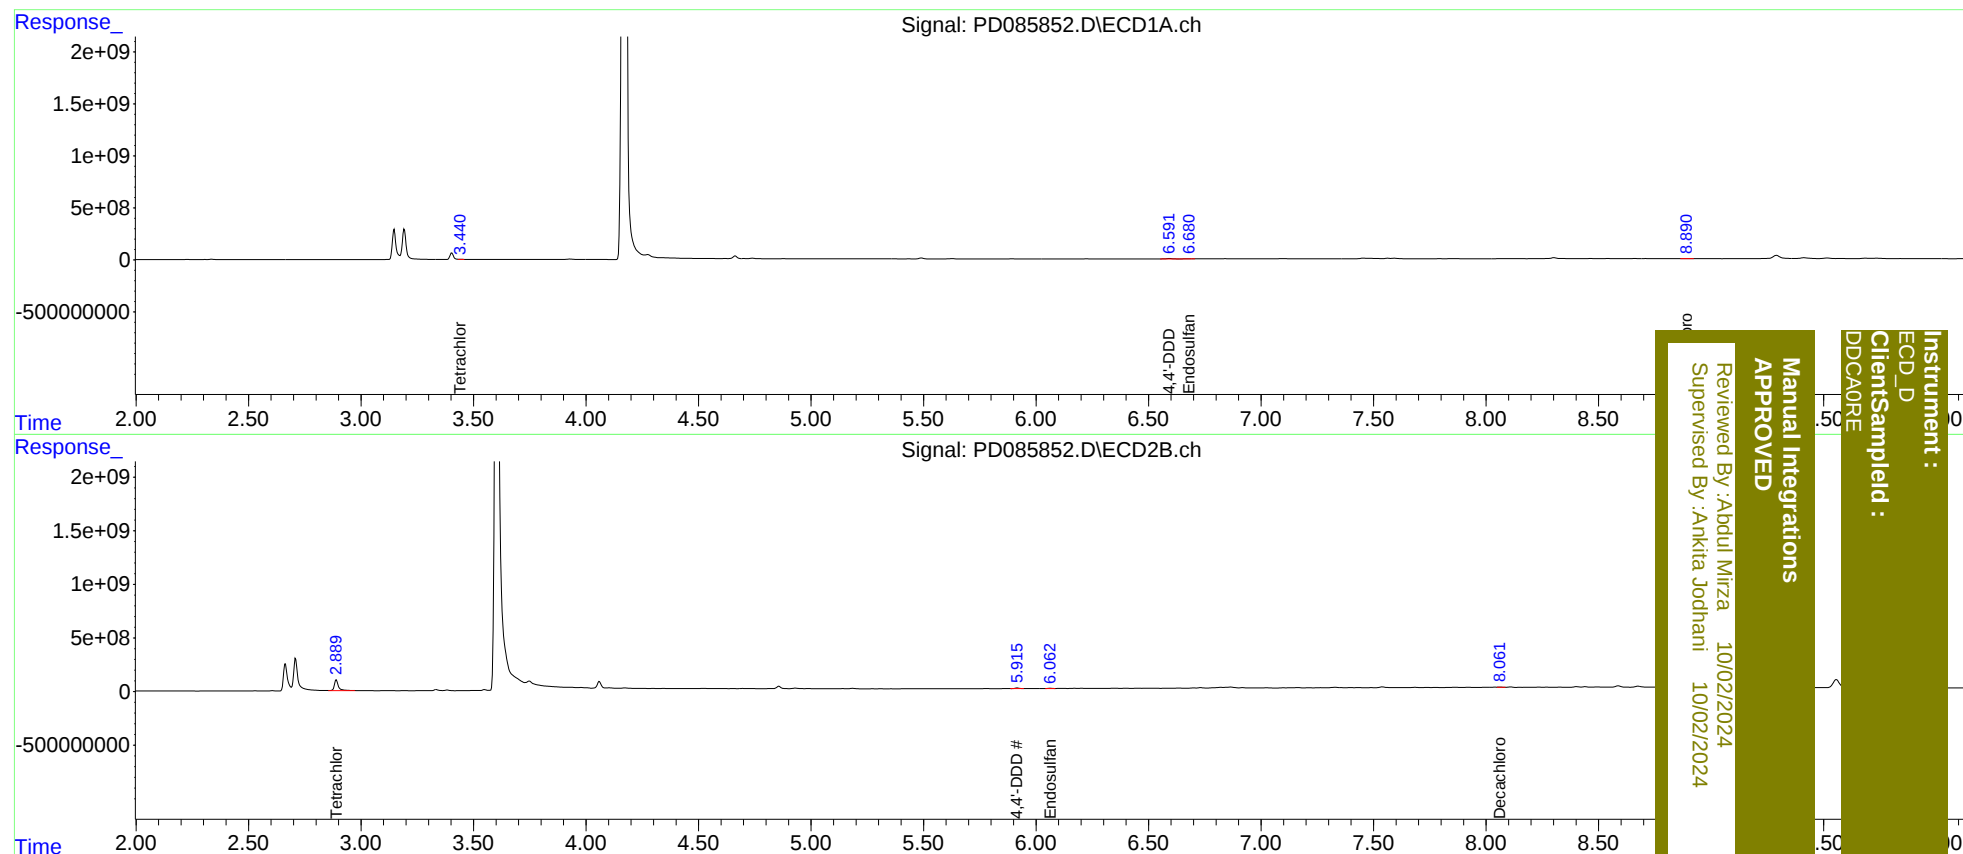

Reviewed By: Abdul Mirza 10/02/2024
Supervised By: Ankita Jodhani 10/02/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDCA0RE