

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100224\
 Data File : PD085856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2024 11:24
 Operator : AR\AJ
 Sample : P4018-07RE
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCB3RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/02/2024
 Supervised By :Ankita Jodhani 10/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 20:58:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	2.888	19498780	539.6E6	17.044m	127.259m#
2)	SA Decachlor...	8.890	8.061	26872469	43541378	14.776m	11.845m
Target Compounds							
2)	A alpha-BHC	3.885	3.386	14923327	80526657	7.168	12.763 #
7)	B delta-BHC	4.662	4.254	191.2E6	139.8E6	99.508	23.554 #
11)	B cis-Chlor...	5.894	5.184	9365525	31401513	4.854m	5.719

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100224\
Data File : PD085856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2024 11:24
Operator : AR\AJ
Sample : P4018-07RE
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 20:58:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

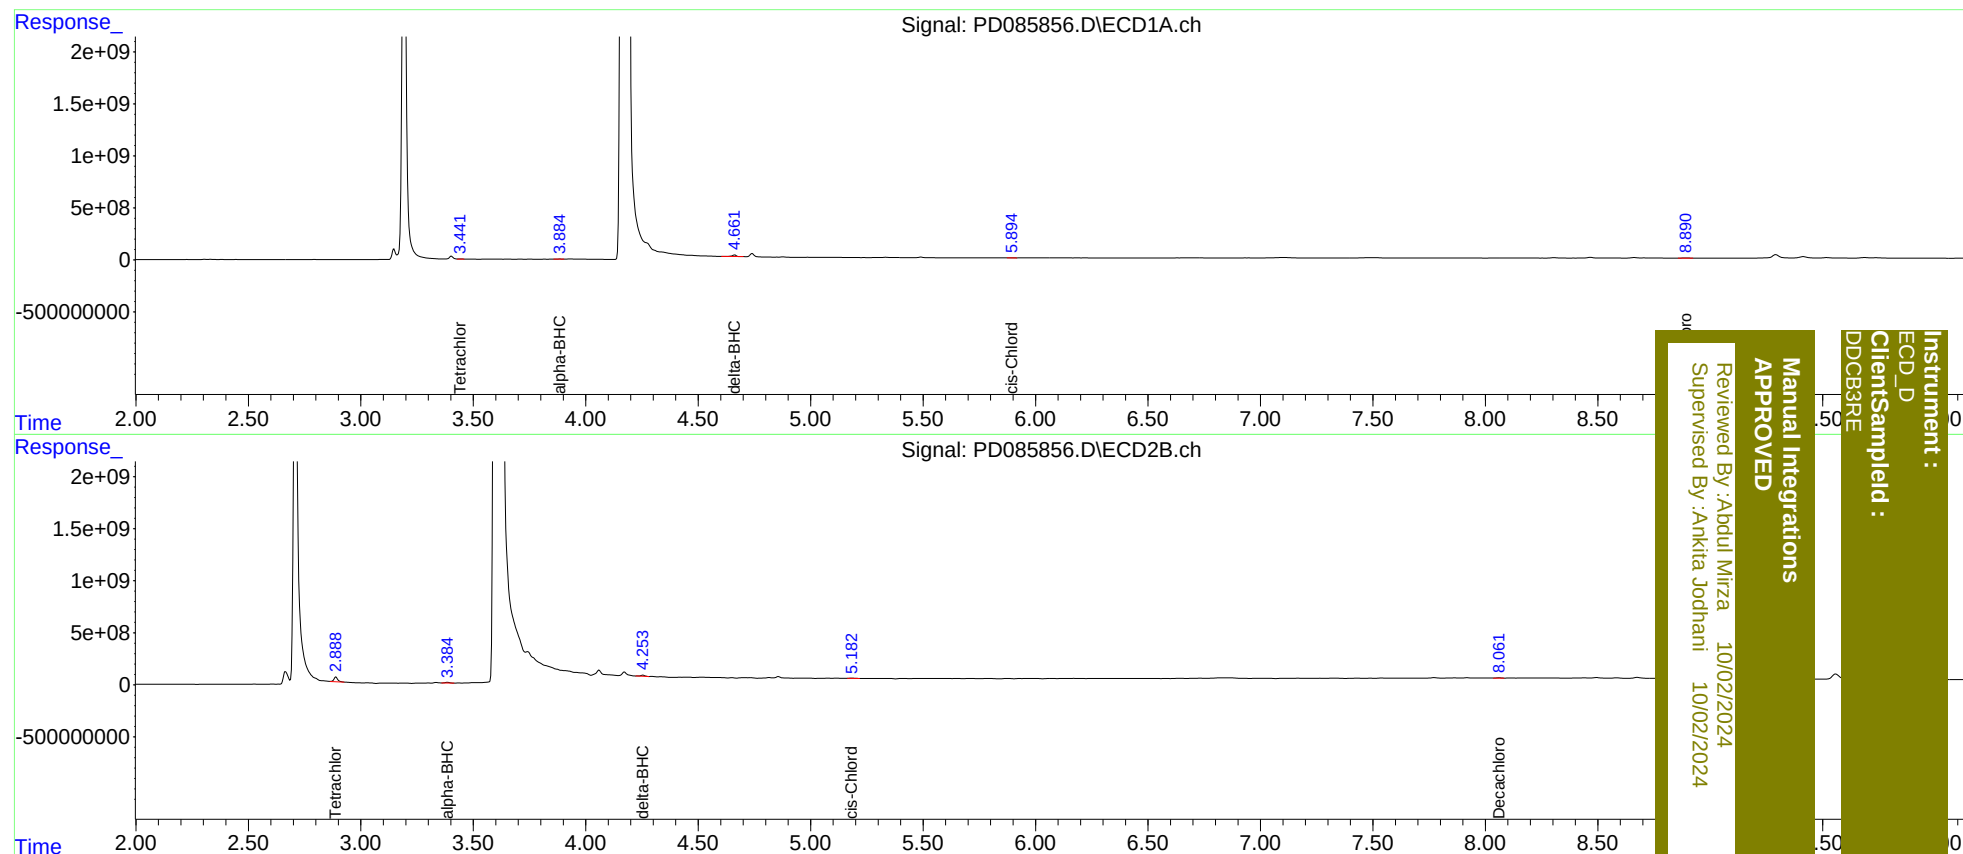

Reviewed By: Abdul Mirza 10/02/2024
Supervised By: Ankita Jodhani 10/02/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDCB3RE