

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100224\
 Data File : PD085862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Oct 2024 12:58
 Operator : AR\AJ
 Sample : P4018-18MSDRE
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCE2MSDRE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/02/2024
 Supervised By :Ankita Jodhani 10/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 01 20:59:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 08:04:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	2.888	23904536	943.0E6	20.895m	222.381m#
27)	SA Decachlor...	8.892	8.062	22682002	58456374	12.472	15.903 #
Target Compounds							
2)	A alpha-BHC	3.886	3.387	101.3E6	289.8E6	48.661	45.937
3)	MA gamma-BHC...	4.156f	3.709	57777.8E6	289.8E6	26458.949m	48.007m#
4)	MA Heptachlor	4.805	4.061	106.6E6	574.5E6	51.837	99.931m#
5)	MB Aldrin	5.145	4.358	123.1E6	264.9E6	58.661	45.084
6)	B beta-BHC	4.398	4.012	37088961	66588639	41.560m	25.441 #
7)	B delta-BHC	4.660	4.252	240.1E6	323.3E6	124.935	54.485 #
8)	B Heptachlo...	5.563	4.859	94921807	288.7E6	49.719	53.177m
9)	A Endosulfan I	5.942	5.234	92987088	213.2E6	51.129m	42.964m
10)	B trans-Chl...	5.817	5.113	102.5E6	225.8E6	55.052	42.163
11)	B cis-Chlor...	5.898	5.178	91157132	246.7E6	47.243	44.923
12)	B 4,4'-DDE	6.069	5.363	190.6E6	456.5E6	115.931	94.481
13)	MA Dieldrin	6.216	5.502	217.8E6	487.1E6	108.683	87.881
14)	MA Endrin	6.442	5.777	182.8E6	456.1E6	115.057	95.274m
15)	B Endosulfa...	6.654	6.071	205.1E6	407.5E6	120.597	89.663 #
16)	A 4,4'-DDD	6.576	5.919	138.2E6	340.8E6	110.779	87.106
17)	MA 4,4'-DDT	6.891	6.173	146.2E6	411.8E6	105.163	97.273
18)	B Endrin al...	6.781	6.250	127.6E6	298.1E6	96.936m	82.684
19)	B Endosulfa...	7.016	6.474	149.0E6	388.2E6	94.594	90.865
20)	A Methoxychlor	7.363	6.745	416.4E6	890.8E6	509.092	431.771
21)	B Endrin ke...	7.491	6.985	218.0E6	457.4E6	126.094m	87.291 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100224\
Data File : PD085862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Oct 2024 12:58
Operator : AR\AJ
Sample : P4018-18MSDRE
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 01 20:59:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100124CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 08:04:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

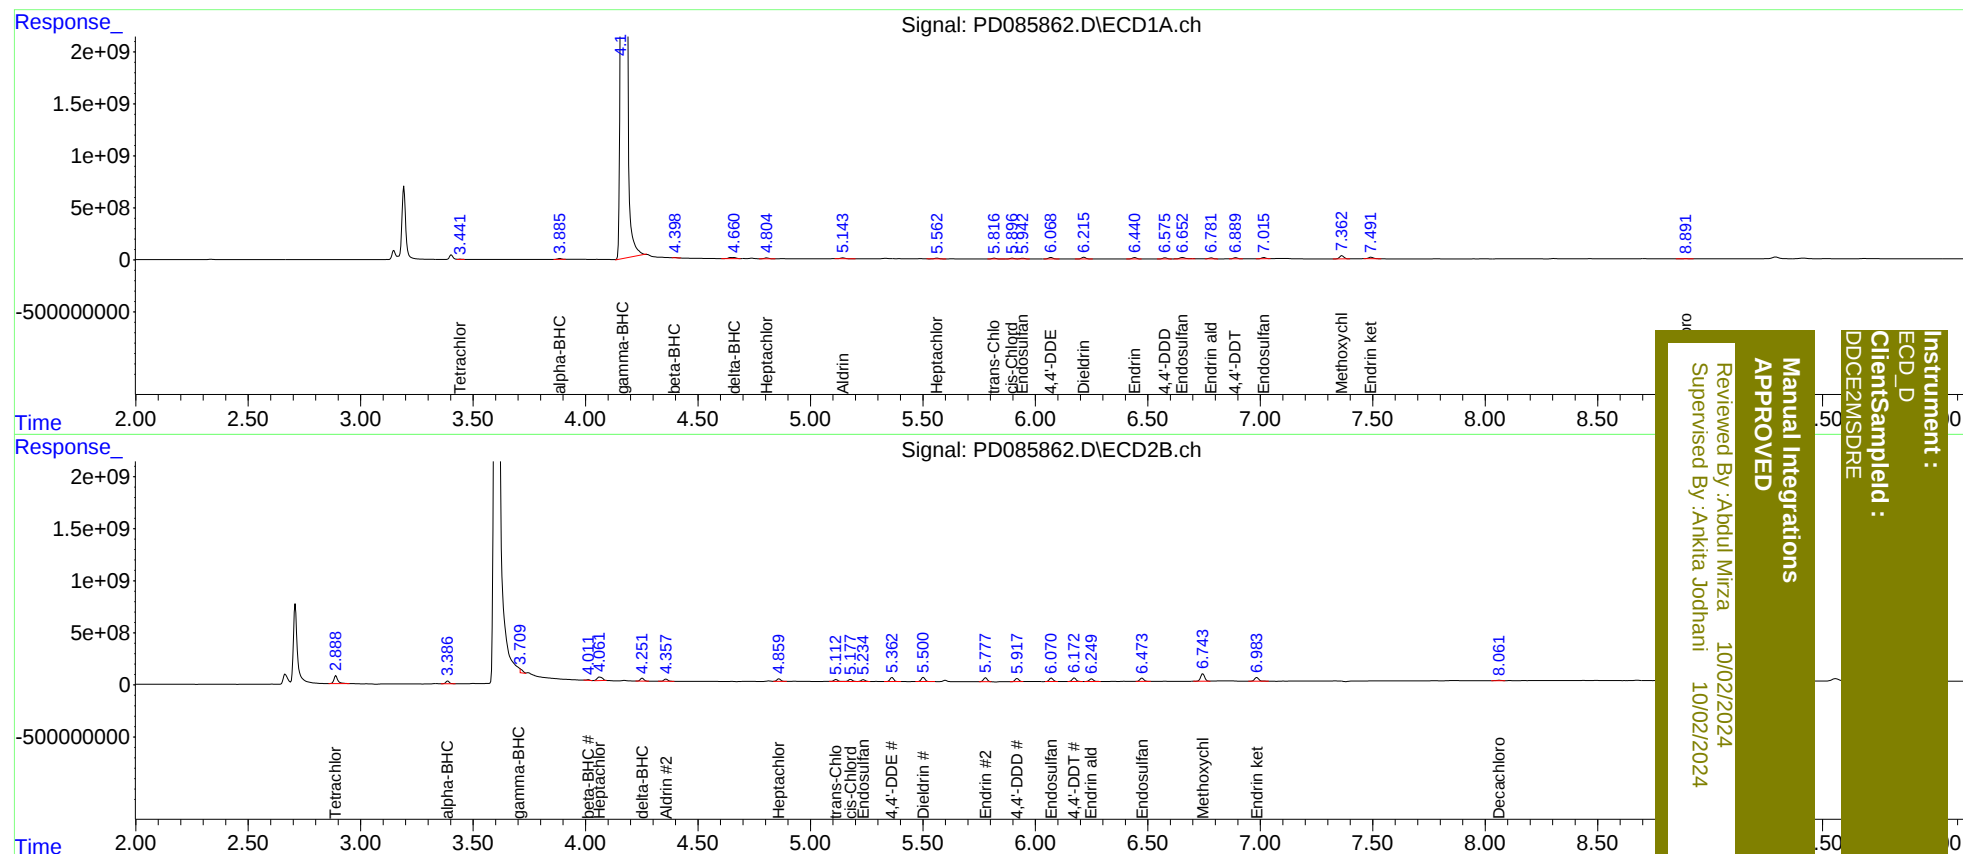

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/02/2024
Supervised By: Ankita Jodhani 10/02/2024

Instrument :
ECD_D
Client Sampled :
DDCE2MSDRE