

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD100918\  
 Data File : PD049724.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 09 Oct 2018 10:53  
 Operator : AJ\SJ  
 Sample : J5258-04  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 09 11:36:14 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD100918CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Oct 09 09:02:50 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|--------|----------|----------|--------|--------|
| -----                       |                 |       |        |          |          |        |        |
| System Monitoring Compounds |                 |       |        |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.284 | 4.035  | 25549317 | 368.2E6  | 18.453 | 20.724 |
| 27)                         | SA Decachlor... | 7.876 | 9.126  | 36109877 | 476.6E6  | 25.809 | 29.652 |
| Target Compounds            |                 |       |        |          |          |        |        |
| 4)                          | MA Heptachlor   | 0.000 | 5.184f | 0        | 2373716  | N.D.   | <MDL   |
| 6)                          | B beta-BHC      | 0.000 | 4.840f | 0        | 5636352  | N.D.   | 0.555  |
| 9)                          | A Endosulfan I  | 0.000 | 6.250  | 0        | 2105524  | N.D.   | 0.110  |
| 11)                         | B cis-Chlor...  | 0.000 | 6.230  | 0        | 1123132  | N.D.   | <MDL   |
| 13)                         | MA Dieldrin     | 0.000 | 6.537  | 0        | 1504349  | N.D.   | <MDL   |
| 15)                         | B Endosulfa...  | 0.000 | 6.968  | 0        | 13783219 | N.D.   | 0.821  |
| 18)                         | B Endrin al...  | 0.000 | 7.030f | 0        | 2858027  | N.D.   | 0.214  |
| -----                       |                 |       |        |          |          |        |        |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD100918\  
Data File : PD049724.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 09 Oct 2018 10:53  
Operator : AJ\SJ  
Sample : J5258-04  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 09 11:36:14 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD100918CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 09 09:02:50 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

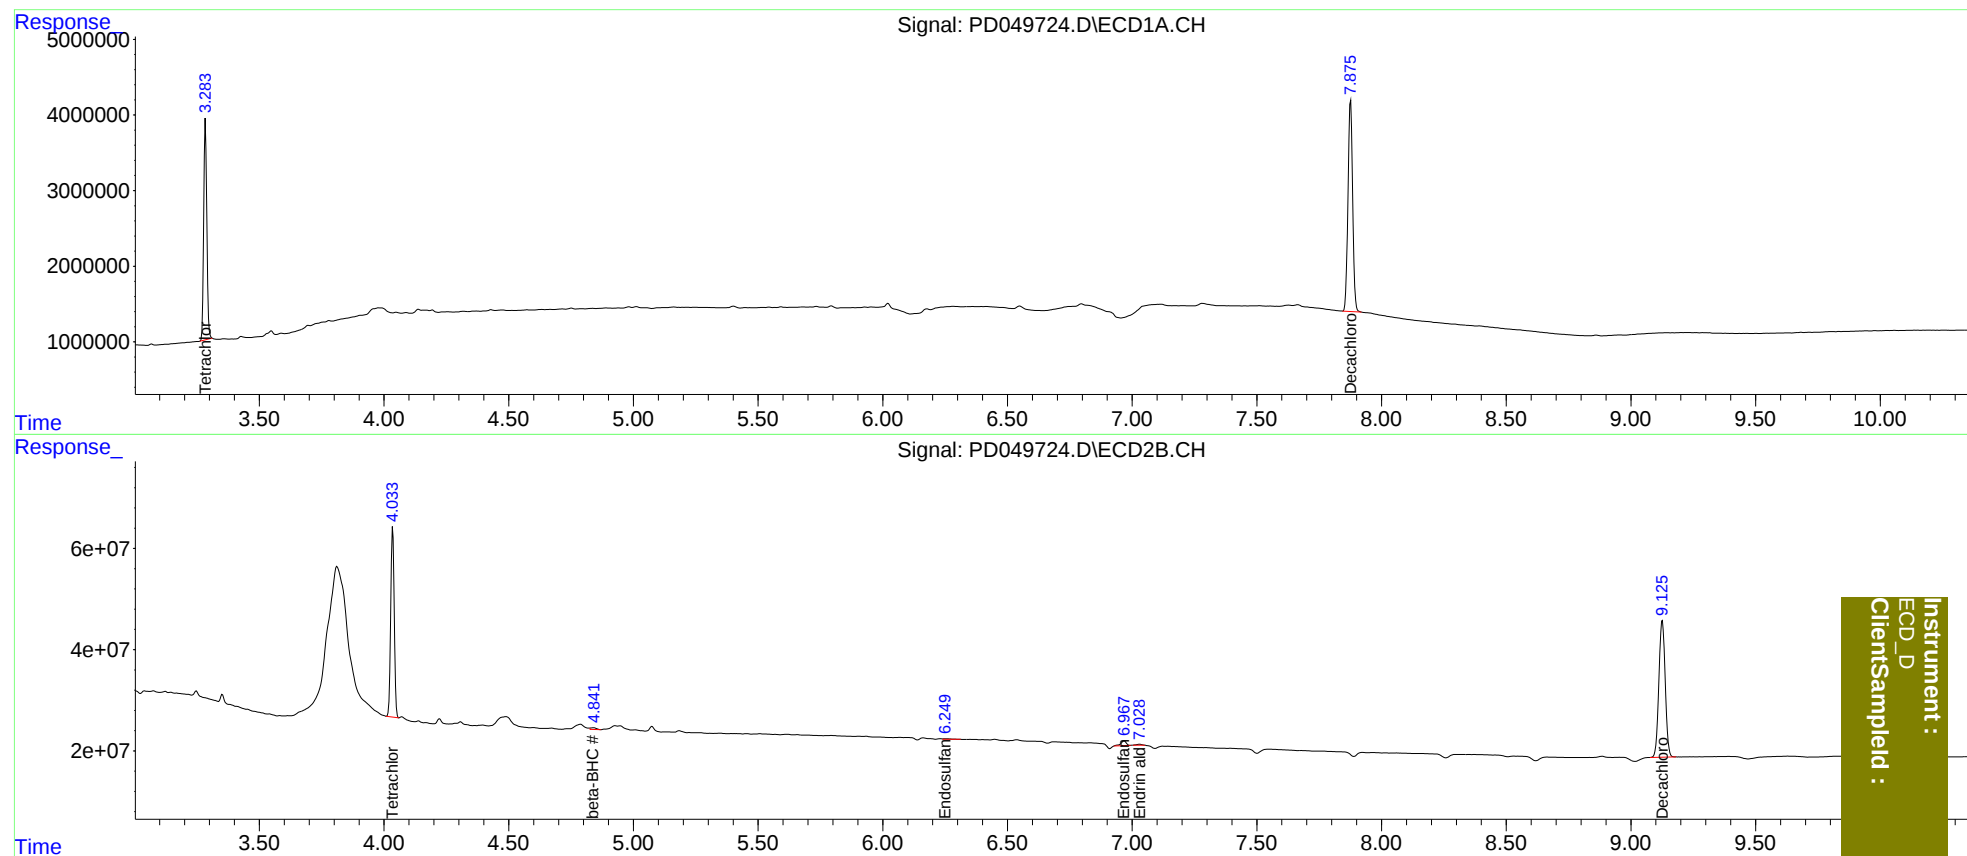


Instrument :  
ECD\_D  
ClientSampleId :

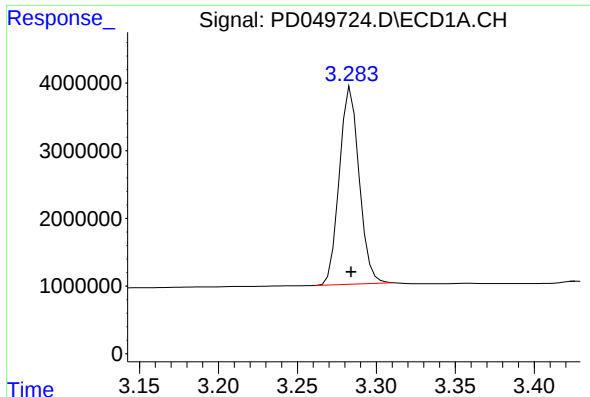

#1 Tetrachloro-m-xylene


R.T.: 3.284 min  
Delta R.T.: 0.000 min  
Response: 25549317  
Conc: 18.45 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :

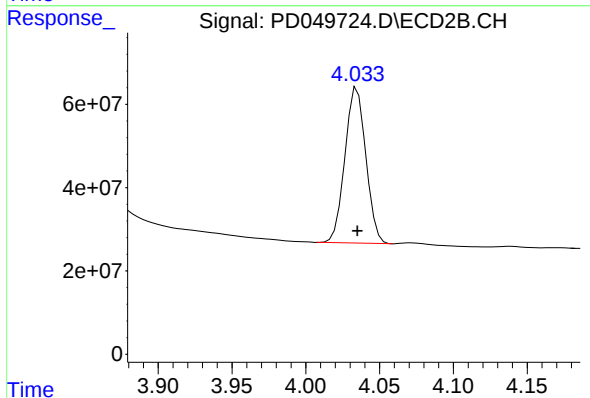


#1 Tetrachloro-m-xylene

R.T.: 4.035 min  
Delta R.T.: 0.000 min  
Response: 368193809  
Conc: 20.72 ng/ml

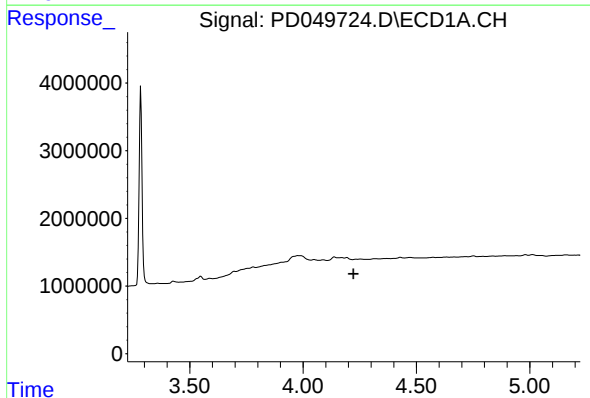


#6 beta-BHC

R.T.: 0.000 min  
Exp R.T. : 4.223 min  
Response: 0  
Conc: N.D.

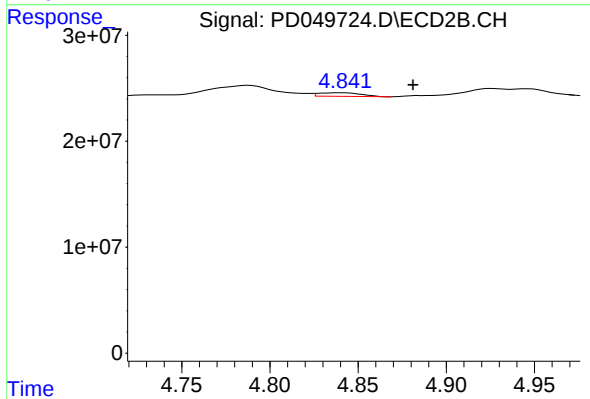

#6 beta-BHC


R.T.: 4.840 min  
Delta R.T.: -0.041 min  
Response: 5636352  
Conc: 0.56 ng/ml

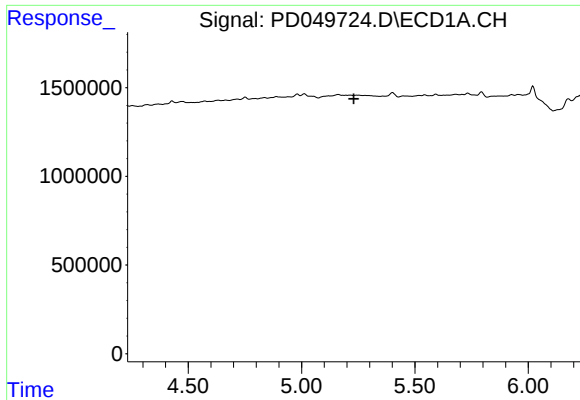

#9 Endosulfan I


R.T.: 0.000 min  
Exp R.T.: 5.231 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_D  
ClientSampleId :

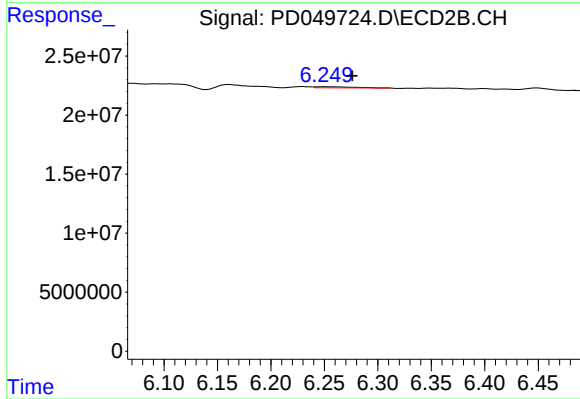


#9 Endosulfan I

R.T.: 6.250 min  
Delta R.T.: -0.026 min  
Response: 2105524  
Conc: 0.11 ng/ml

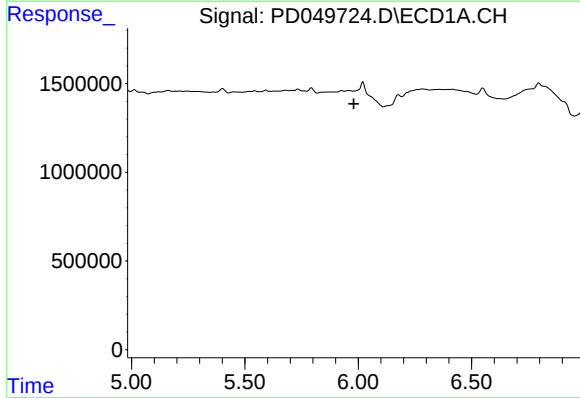


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T.: 5.980 min  
Response: 0  
Conc: N.D.

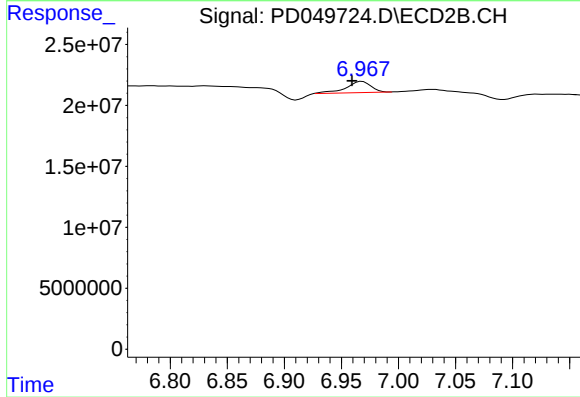

#15 Endosulfan II


R.T.: 6.968 min  
Delta R.T.: 0.009 min  
Response: 13783219  
Conc: 0.82 ng/ml

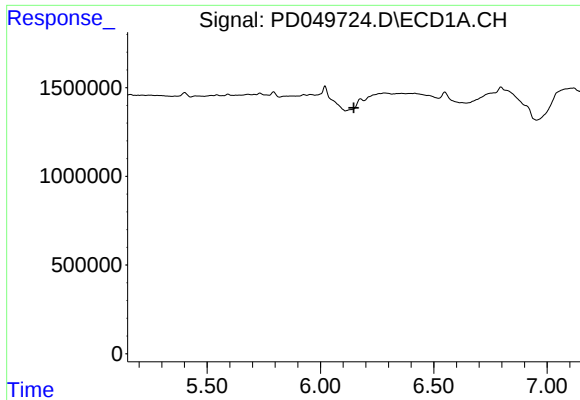

#18 Endrin aldehyde


R.T.: 0.000 min  
Exp R.T.: 6.147 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_D  
ClientSampleId :

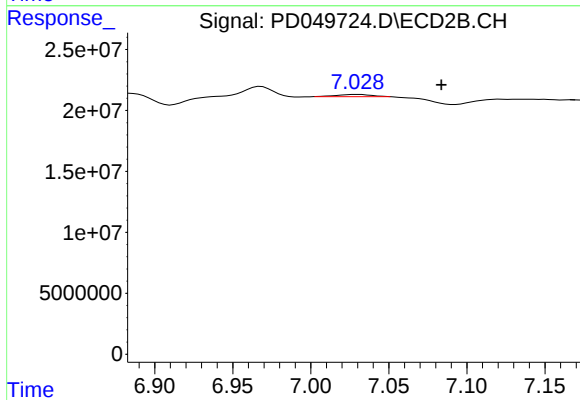


#18 Endrin aldehyde

R.T.: 7.030 min  
Delta R.T.: -0.054 min  
Response: 2858027  
Conc: 0.21 ng/ml

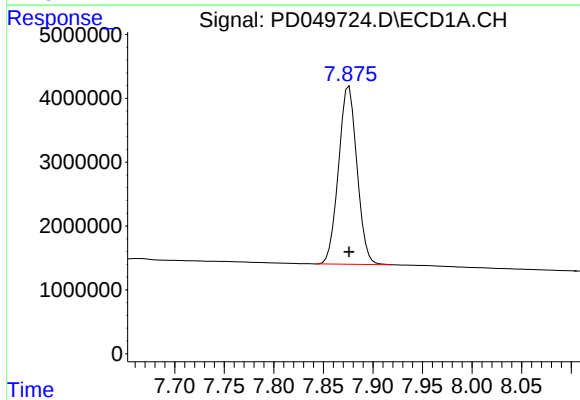

#27 Decachlorobiphenyl

R.T.: 7.876 min  
Delta R.T.: 0.000 min  
Response: 36109877  
Conc: 25.81 ng/ml

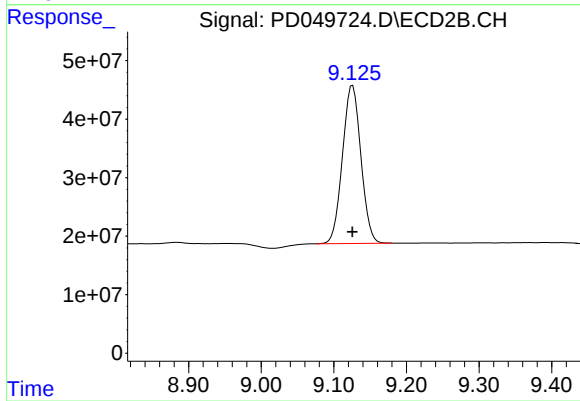

#27 Decachlorobiphenyl

R.T.: 9.126 min  
Delta R.T.: 0.000 min  
Response: 476641361  
Conc: 29.65 ng/ml