

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100918\
 Data File : PD049738.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Oct 2018 15:00
 Operator : AJ\SJ
 Sample : J5295-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A3YY3

Manual Integrations
 APPROVED

Sohil
 10/11/2018 2:41:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 04:13:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100918CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 09 09:02:50 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.283	4.033	17126152	211.7E6	12.369	11.916m
27)	SA Decachlor...	7.875	9.125	29013250	418.9E6	20.737	26.057m#
Target Compounds							
12)	B 4,4'-DDE	5.351	6.377	20309856	229.5E6	12.737m	11.748m
16)	A 4,4'-DDD	5.847	6.871	17031755	589.7E6	12.660m	37.452m#
17)	MA 4,4'-DDT	6.080	7.168	129.1E6	737.0E6	92.267	50.898m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD100918\
Data File : PD049738.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Oct 2018 15:00
Operator : AJ\SJ
Sample : J5295-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 04:13:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD100918CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 09 09:02:50 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

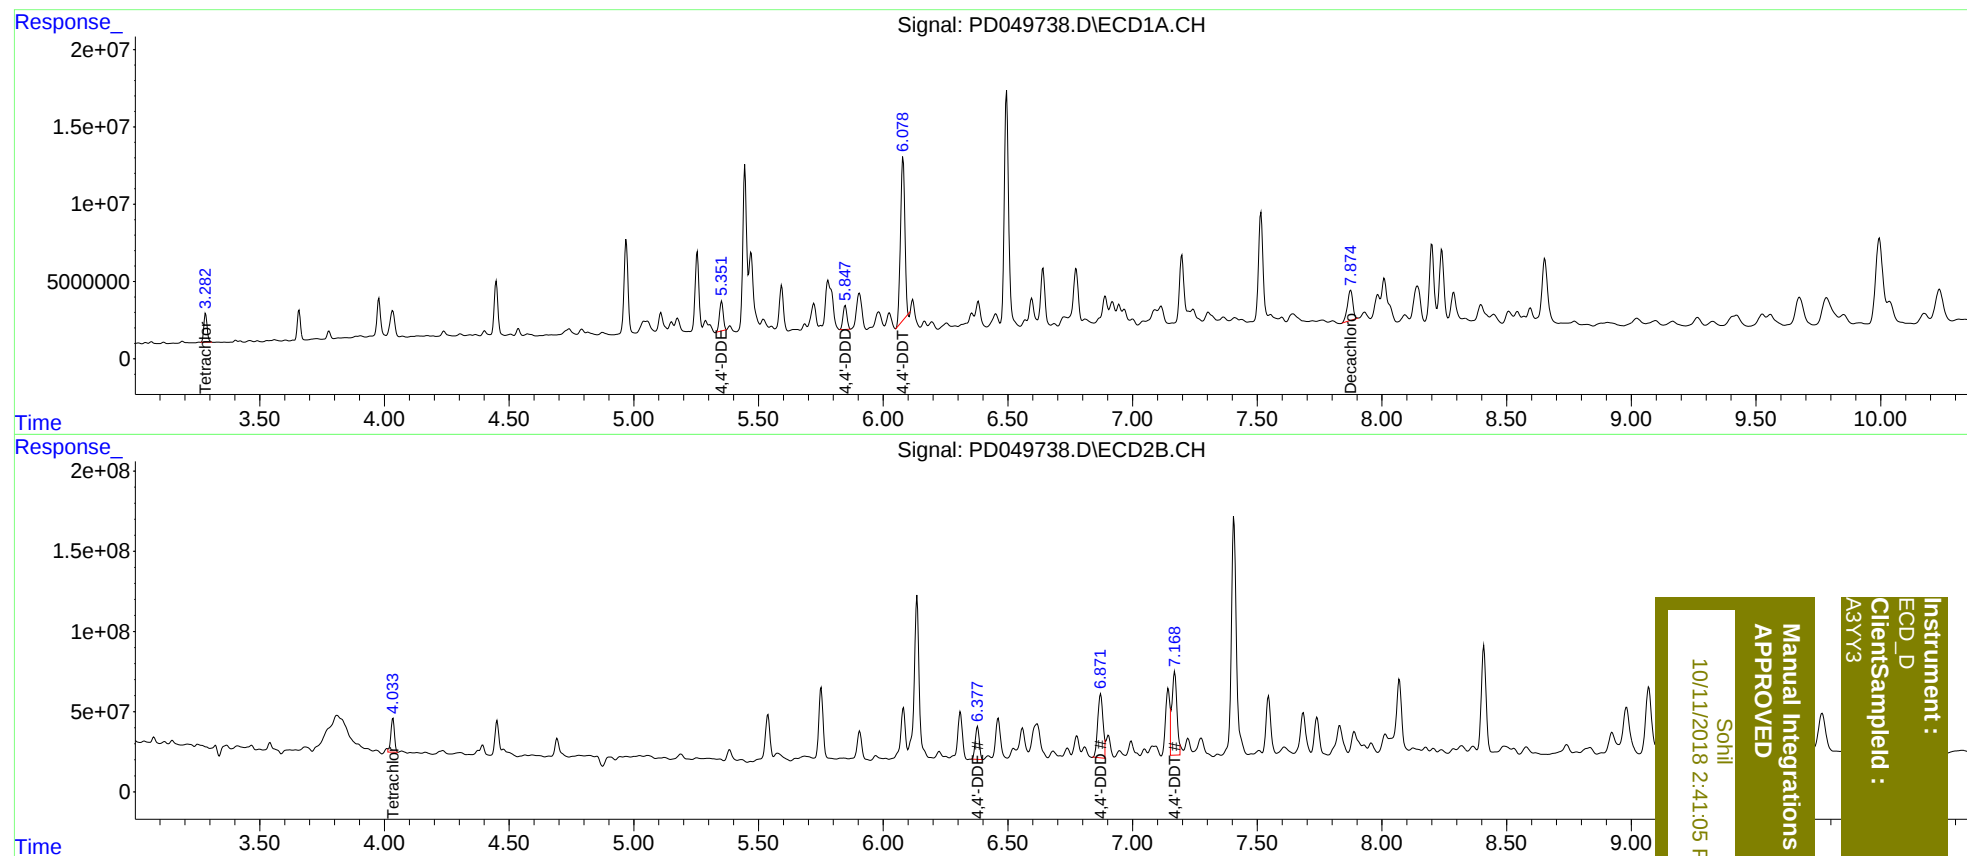

10/11/2018 2:41:05 PM

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
A3YV3