

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101824\
 Data File : PD086105.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2024 15:17
 Operator : AR\AJ
 Sample : P4368-07
 Misc : TOX LOD 50PPB WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/18/2024
 Supervised By :Ankita Jodhani 10/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 03:19:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX101124.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 11 14:34:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.447	2.876	21520116	117.3E6	17.186	18.263
7) SA Decachlor...	8.901	8.058	38758794	115.9E6	17.925	20.033
Target Compounds						
2) Toxaphene-1	5.729	5.133	295057	3337760	43.500m	56.473 #
3) Toxaphene-2	6.318	5.460	1323597	3831619	55.712	64.880
4) Toxaphene-3	6.930	5.822	2603535	2576398	44.576	48.535
5) Toxaphene-4	7.020	6.743	1863950	8367808	44.467	50.029
6) Toxaphene-5	7.431	7.185	2855880	5410161	50.319	48.327

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101824\
Data File : PD086105.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2024 15:17
Operator : AR\AJ
Sample : P4368-07
Misc : TOX LOD 50PPB WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 03:19:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX101124.M
Quant Title : GC Extractables
QLast Update : Fri Oct 11 14:34:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

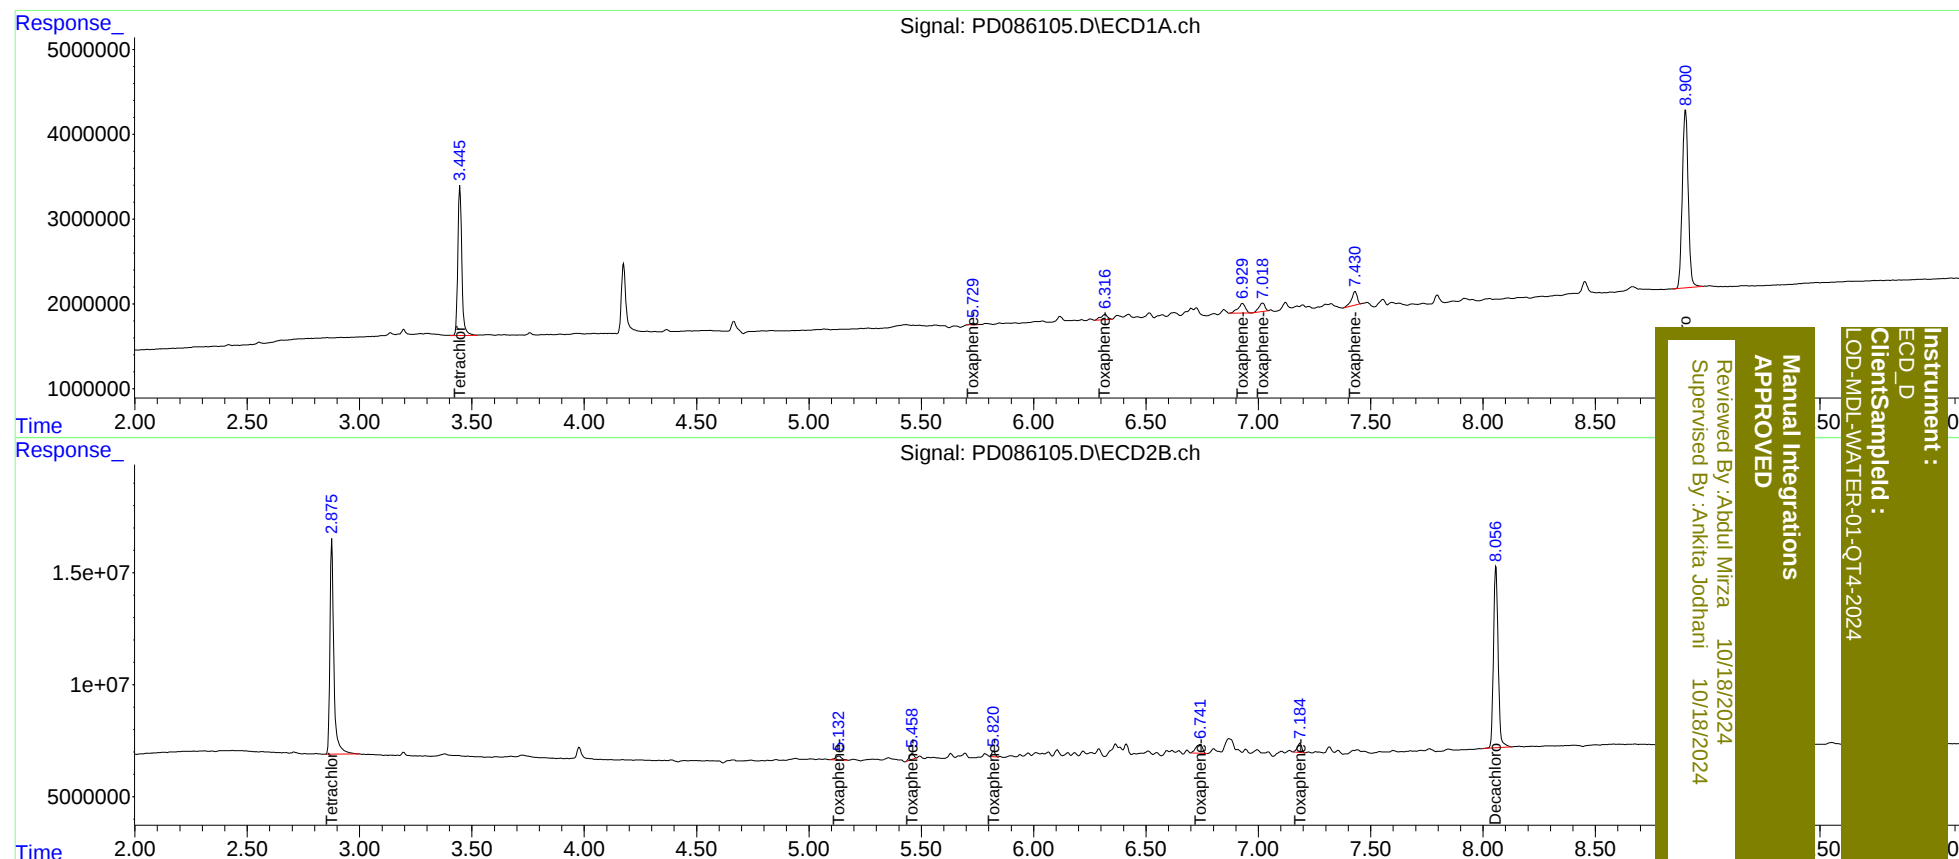

Reviewed By: Abdul Mirza 10/18/2024
Supervised By: Ankita Jodhani 10/18/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
LOD-MDL-WATER-01-QT4-2024