

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
 Data File : PD072500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2022 08:59
 Operator : AR\AJ
 Sample : PIBLK373
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 05:01:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.466	54770839	860.2E6	21.480	22.904
27)	SA Decachlor...	7.844	8.925	84388187	413.0E6	42.160	45.875
Target Compounds							
2)	A alpha-BHC	3.204	0.000	151107	0	<MDL	N.D. #
3)	MA gamma-BHC...	0.000	4.222f	0	4768235	N.D.	0.114
4)	MA Heptachlor	3.869	0.000	20403	0	<MDL	N.D. #
5)	MB Aldrin	4.137	0.000	246005	0	<MDL	N.D. #
6)	B beta-BHC	3.869	0.000	20403	0	<MDL	N.D. #
7)	B delta-BHC	4.075	4.678f	357101	12393318	0.101	0.389 #
8)	B Heptachlo...	0.000	5.603	0	45765332	N.D.	2.352
9)	A Endosulfan I	5.064	0.000	253740	0	<MDL	N.D. #
10)	B trans-Chl...	4.895	0.000	532456	0	0.171	N.D. #
11)	B cis-Chlor...	4.955	0.000	418794	0	0.139	N.D. #
12)	B 4,4'-DDE	5.145	0.000	2151518	0	0.739	N.D. #
16)	A 4,4'-DDD	5.672f	0.000	82227	0	<MDL	N.D. #
19)	B Endosulfa...	6.296	0.000	263640	0	0.109	N.D. #
23)	Toxaphene-2	5.672f	0.000	82227	0	6.012	N.D. #
25)	Toxaphene-4	6.660	0.000	178886	0	2.374	N.D. #
26)	Toxaphene-5	6.922f	0.000	122678	0	2.988	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
Data File : PD072500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2022 08:59
Operator : AR\AJ
Sample : PIBLK373
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 05:01:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

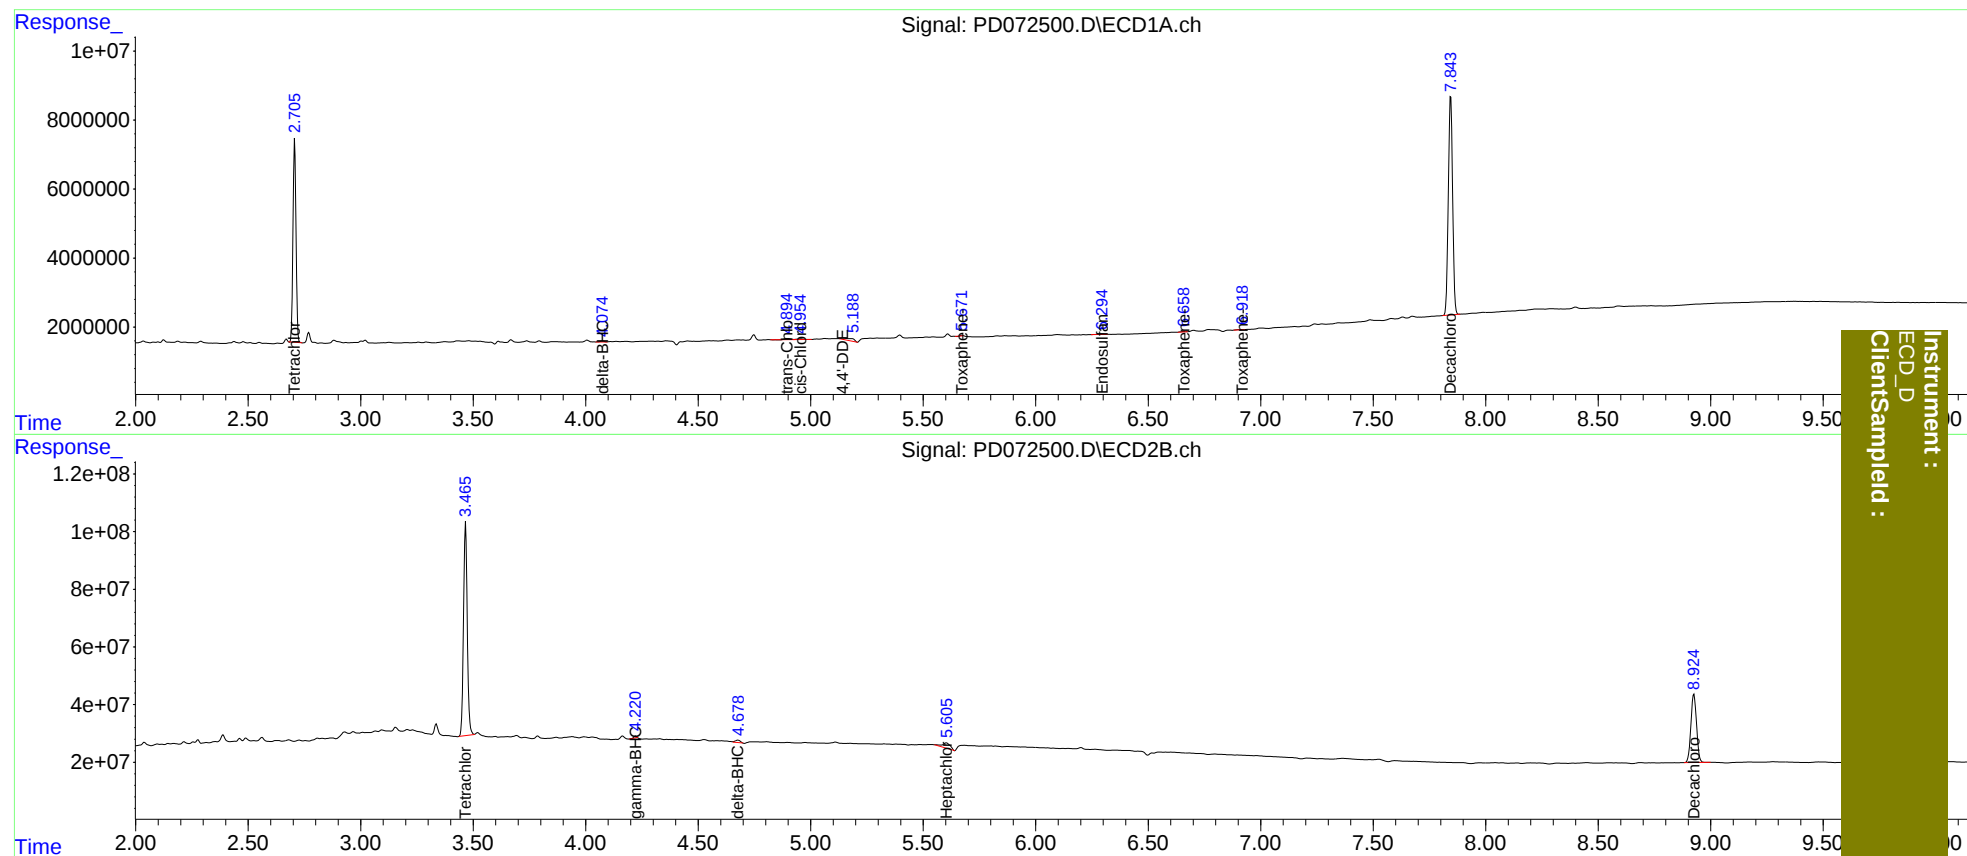


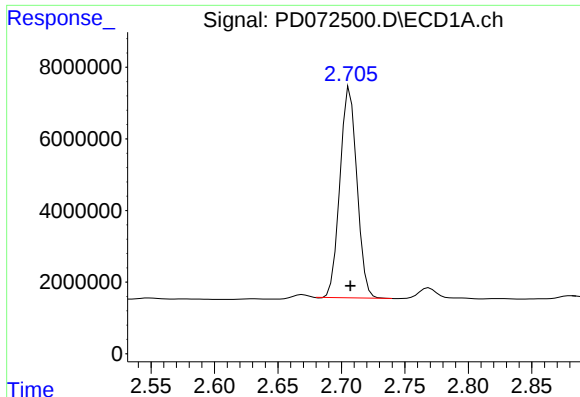

#1 Tetrachloro-m-xylene


R.T.: 2.707 min
Delta R.T.: 0.000 min
Response: 54770839
Conc: 21.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

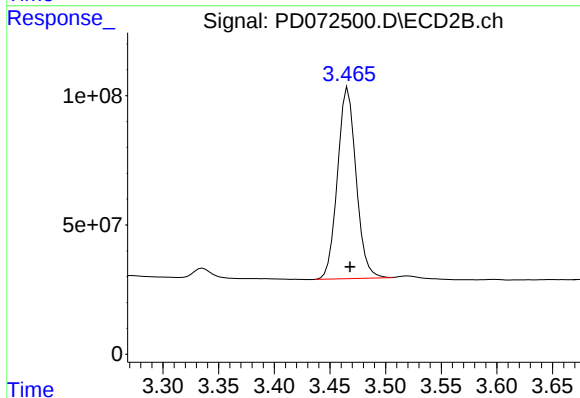


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 860248810
Conc: 22.90 ng/ml

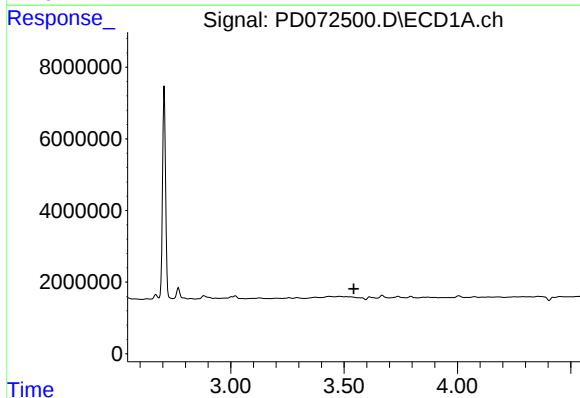


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.543 min
Response: 0
Conc: N.D.

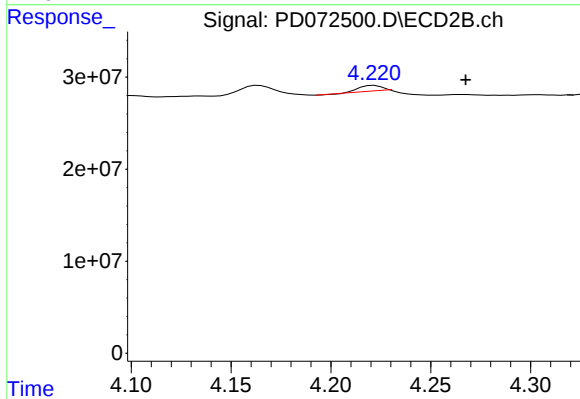

#3 gamma-BHC (Lindane)


R.T.: 4.222 min
Delta R.T.: -0.046 min
Response: 4768235
Conc: 0.11 ng/ml

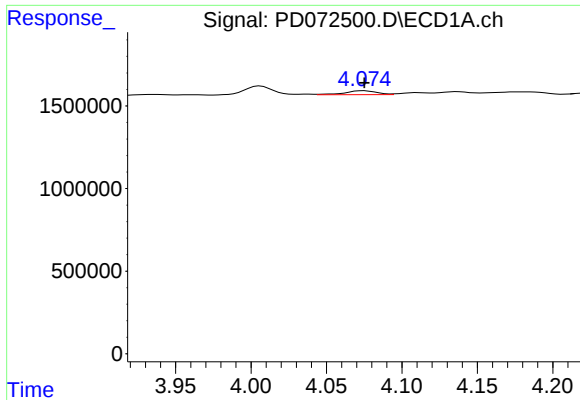

#7 delta-BHC


R.T.: 4.075 min
Delta R.T.: 0.000 min
Response: 357101
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

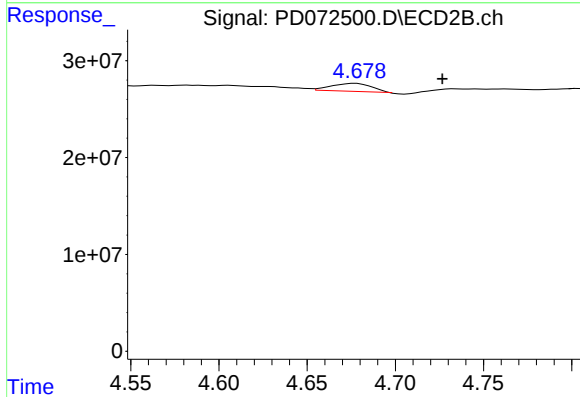


#7 delta-BHC

R.T.: 4.678 min
Delta R.T.: -0.049 min
Response: 12393318
Conc: 0.39 ng/ml

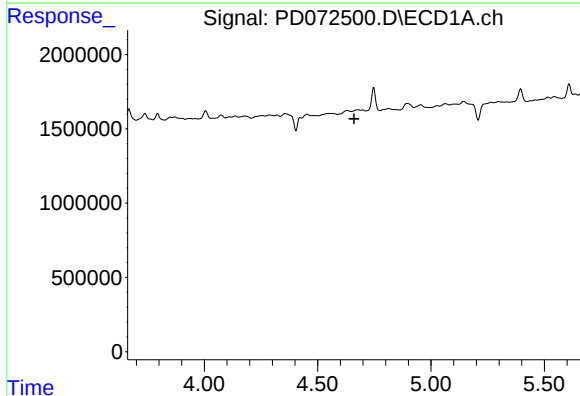


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.660 min
Response: 0
Conc: N.D.

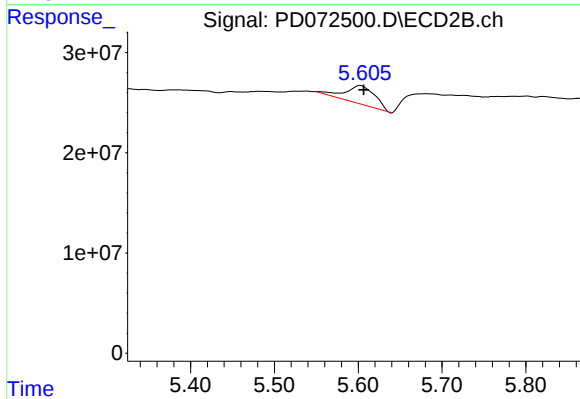

#8 Heptachlor epoxide


R.T.: 5.603 min
Delta R.T.: -0.004 min
Response: 45765332
Conc: 2.35 ng/ml

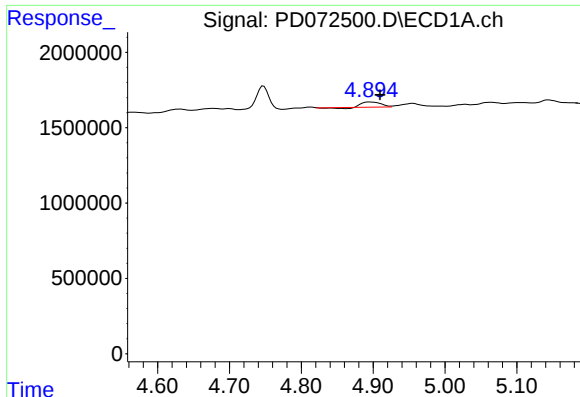

#10 trans-Chlordane


R.T.: 4.895 min
Delta R.T.: -0.014 min
Response: 532456
Conc: 0.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

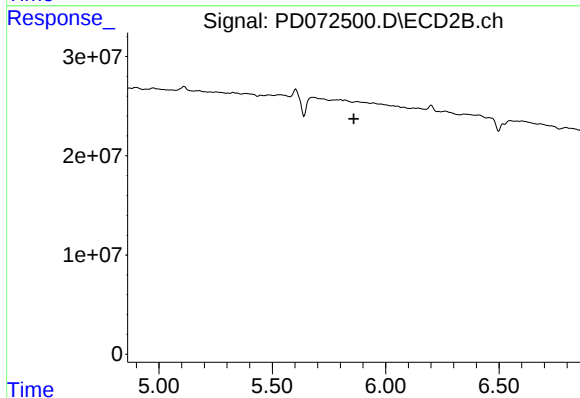


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

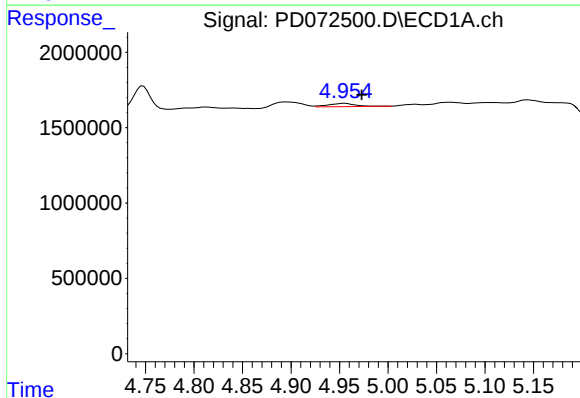


#11 cis-Chlordane

R.T.: 4.955 min
Delta R.T.: -0.018 min
Response: 418794
Conc: 0.14 ng/ml

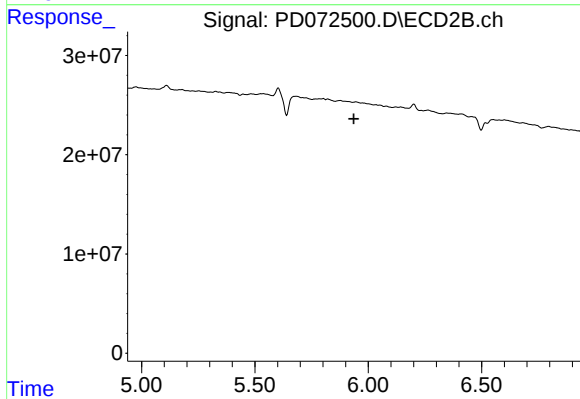

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.936 min
Response: 0
Conc: N.D.

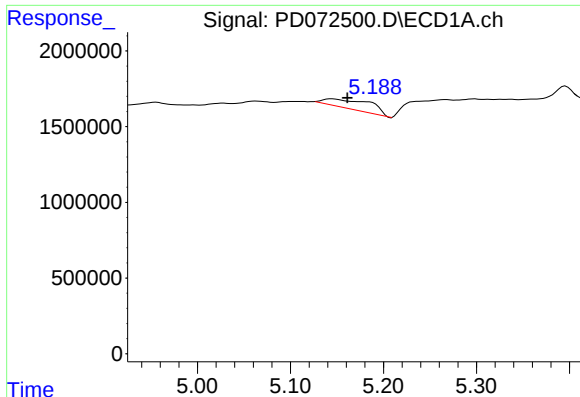

#12 4,4'-DDE


R.T.: 5.145 min
Delta R.T.: -0.017 min
Response: 2151518
Conc: 0.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

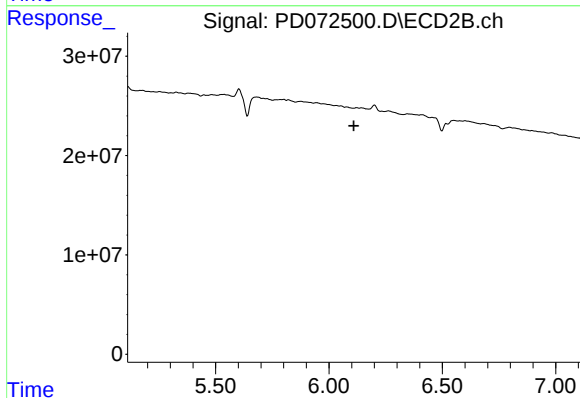


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

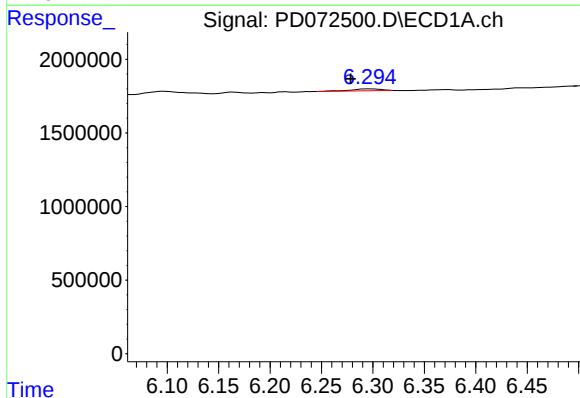


#19 Endosulfan Sulfate

R.T.: 6.296 min
Delta R.T.: 0.017 min
Response: 263640
Conc: 0.11 ng/ml

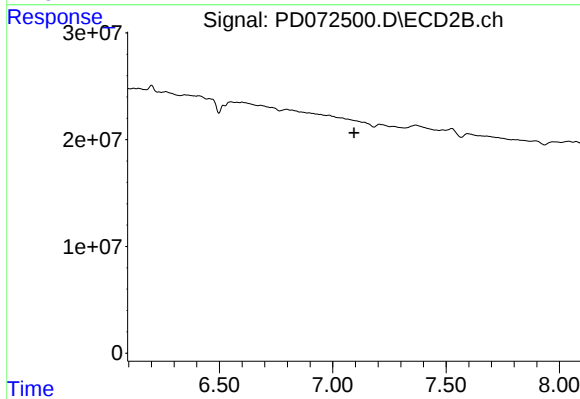

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.095 min
Response: 0
Conc: N.D.

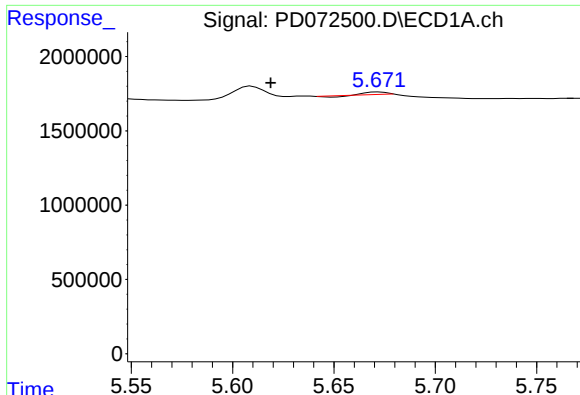

#23 Toxaphene-2


R.T.: 5.672 min
Delta R.T.: 0.053 min
Response: 82227
Conc: 6.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

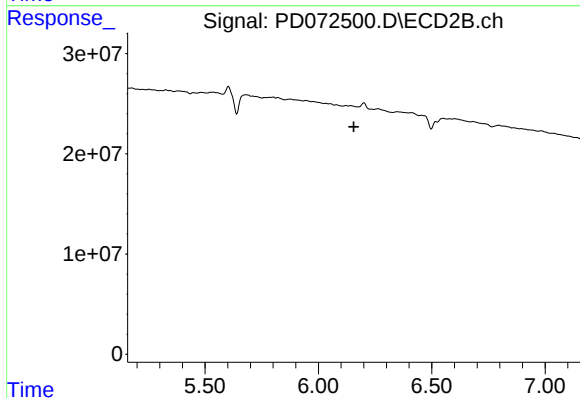


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.156 min
Response: 0
Conc: N.D.

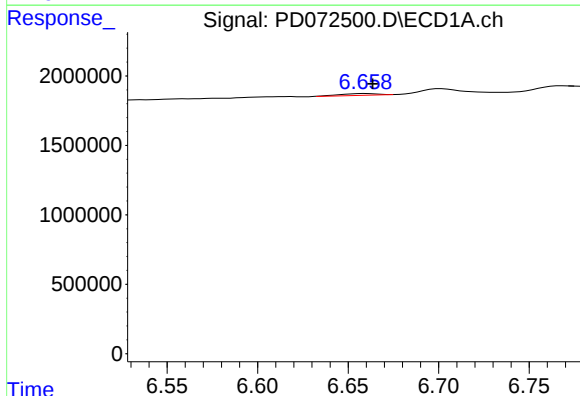


#25 Toxaphene-4

R.T.: 6.660 min
Delta R.T.: -0.004 min
Response: 178886
Conc: 2.37 ng/ml

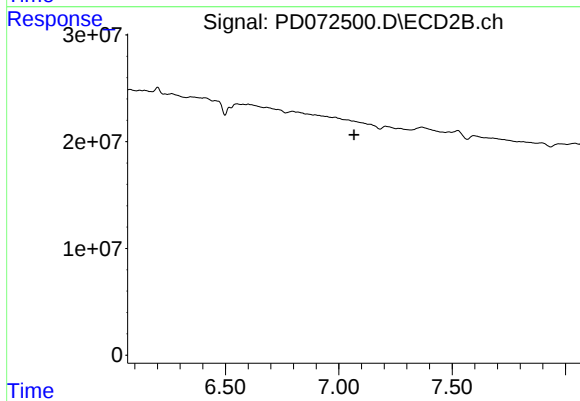

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T. : 7.068 min
Response: 0
Conc: N.D.

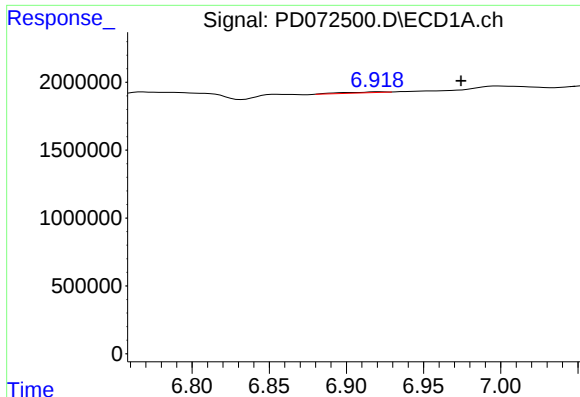

#26 Toxaphene-5


R.T.: 6.922 min
Delta R.T.: -0.053 min
Response: 122678
Conc: 2.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

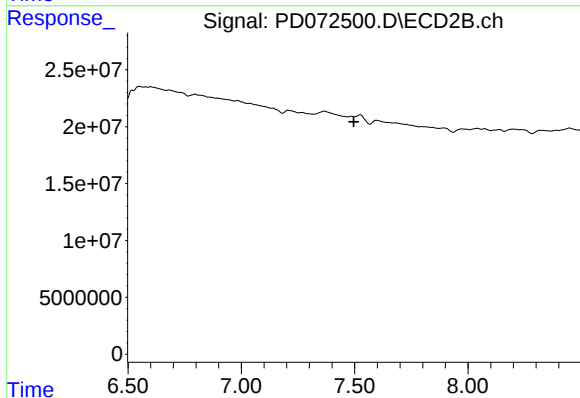


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.497 min
Response: 0
Conc: N.D.

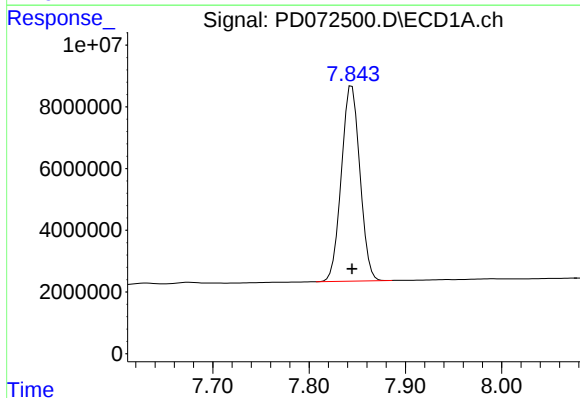

#27 Decachlorobiphenyl

R.T.: 7.844 min
Delta R.T.: 0.000 min
Response: 84388187
Conc: 42.16 ng/ml

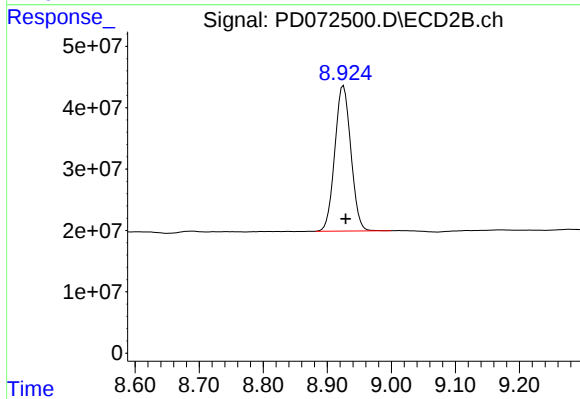

#27 Decachlorobiphenyl

R.T.: 8.925 min
Delta R.T.: -0.004 min
Response: 412974205
Conc: 45.88 ng/ml