

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD101922\  
 Data File : PD072504.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Oct 2022 12:03  
 Operator : AR\AJ  
 Sample : PIBLK374  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 20 05:02:53 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101722CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Oct 20 01:04:30 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 2.713  | 3.464 | 55449316 | 953.9E6  | 21.747 | 25.396 |
| 27)                         | SA Decachlor... | 7.852  | 8.927 | 85992823 | 426.7E6  | 42.961 | 47.405 |
| Target Compounds            |                 |        |       |          |          |        |        |
| 2)                          | A alpha-BHC     | 3.201  | 0.000 | 174905   | 0        | <MDL   | N.D. # |
| 8)                          | B Heptachlo...  | 0.000  | 5.602 | 0        | 57347691 | N.D.   | 2.947  |
| 9)                          | A Endosulfan I  | 4.966f | 0.000 | 506294   | 0        | 0.188  | N.D. # |
| 10)                         | B trans-Chl...  | 4.966f | 0.000 | 506294   | 0        | 0.163  | N.D. # |
| 11)                         | B cis-Chlor...  | 4.966  | 0.000 | 506294   | 0        | 0.168  | N.D. # |
| 15)                         | B Endosulfa...  | 5.838  | 0.000 | 223175   | 0        | <MDL   | N.D. # |
| 17)                         | MA 4,4'-DDT     | 5.972  | 0.000 | 72606    | 0        | <MDL   | N.D. # |
| 19)                         | B Endosulfa...  | 6.279  | 0.000 | 392519   | 0        | 0.163  | N.D. # |
| 24)                         | Toxaphene-3     | 5.838f | 0.000 | 223175   | 0        | 12.267 | N.D. # |
| -----                       |                 |        |       |          |          |        |        |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD101922\  
Data File : PD072504.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 19 Oct 2022 12:03  
Operator : AR\AJ  
Sample : PIBLK374  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 20 05:02:53 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD101722CLP.M  
Quant Title : GC Extractables  
QLast Update : Thu Oct 20 01:04:30 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

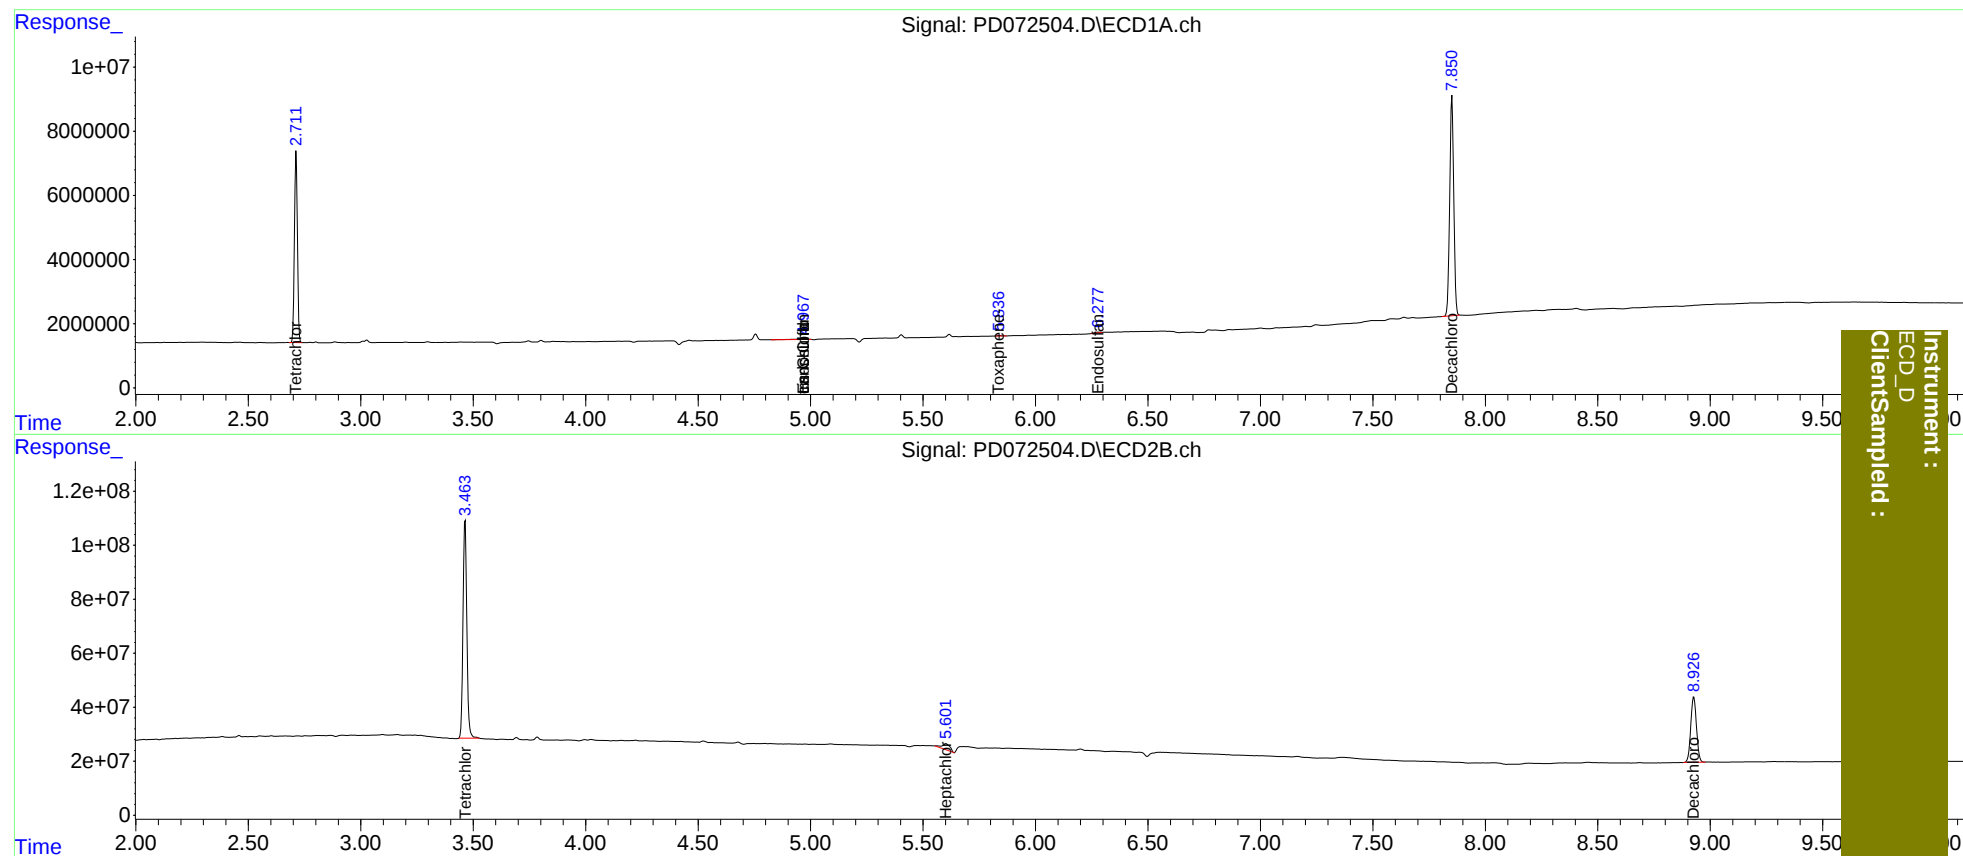


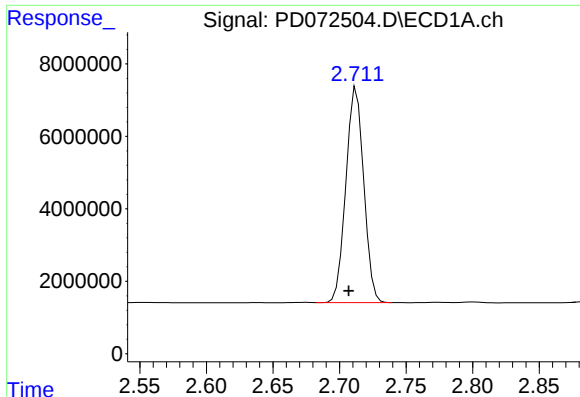

#1 Tetrachloro-m-xylene


R.T.: 2.713 min  
Delta R.T.: 0.006 min  
Response: 55449316  
Conc: 21.75 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :

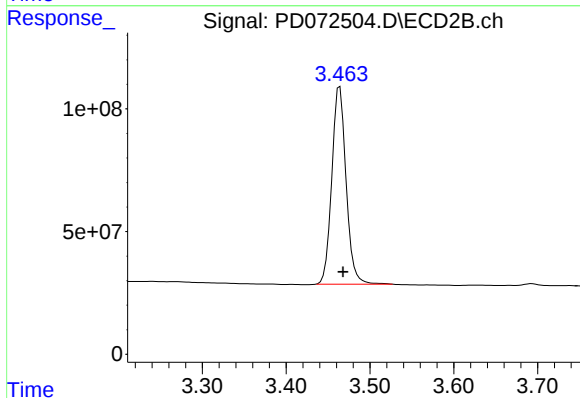


#1 Tetrachloro-m-xylene

R.T.: 3.464 min  
Delta R.T.: -0.004 min  
Response: 953871195  
Conc: 25.40 ng/ml

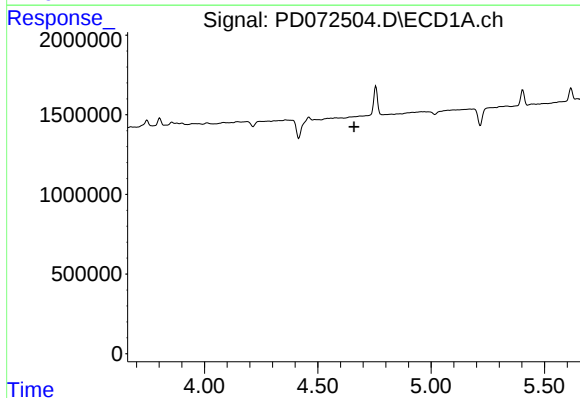


#8 Heptachlor epoxide

R.T.: 0.000 min  
Exp R.T. : 4.660 min  
Response: 0  
Conc: N.D.

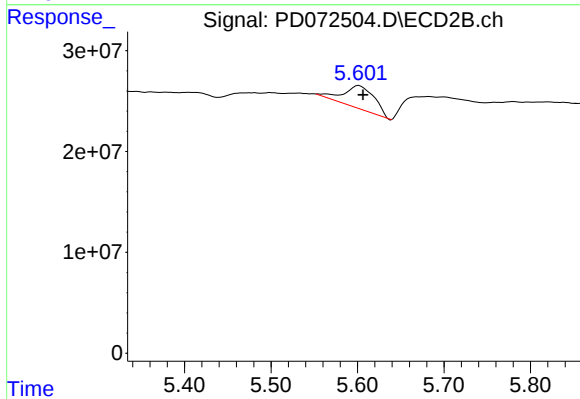

#8 Heptachlor epoxide


R.T.: 5.602 min  
Delta R.T.: -0.005 min  
Response: 57347691  
Conc: 2.95 ng/ml

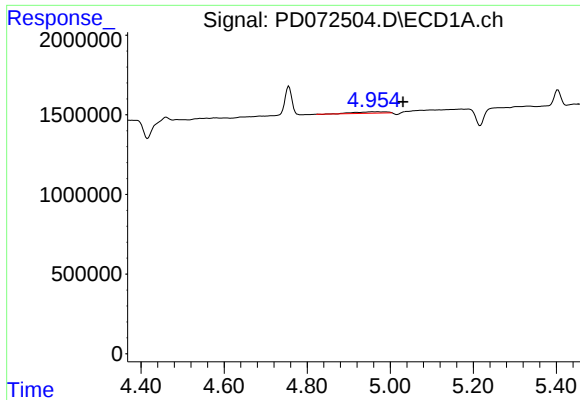

#9 Endosulfan I


R.T.: 4.966 min  
Delta R.T.: -0.065 min  
Response: 506294  
Conc: 0.19 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :

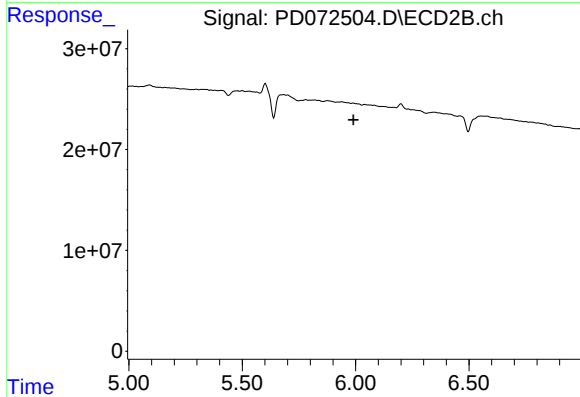


#9 Endosulfan I

R.T.: 0.000 min  
Exp R.T. : 5.991 min  
Response: 0  
Conc: N.D.

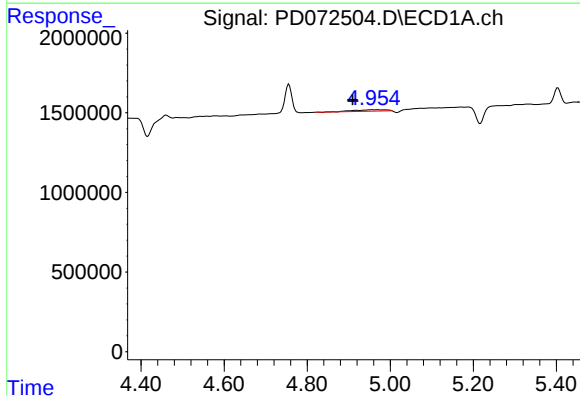


#10 trans-Chlordane

R.T.: 4.966 min  
Delta R.T.: 0.056 min  
Response: 506294  
Conc: 0.16 ng/ml

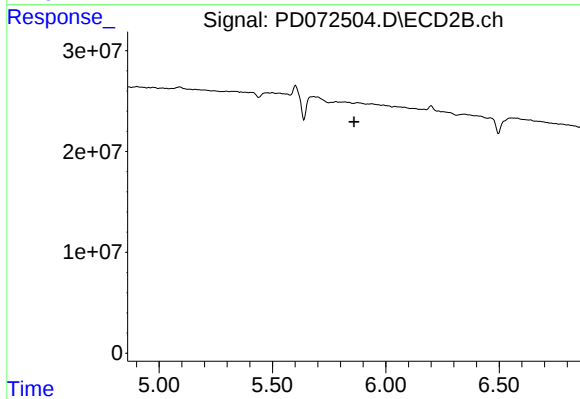

#10 trans-Chlordane


R.T.: 0.000 min  
Exp R.T. : 5.860 min  
Response: 0  
Conc: N.D.

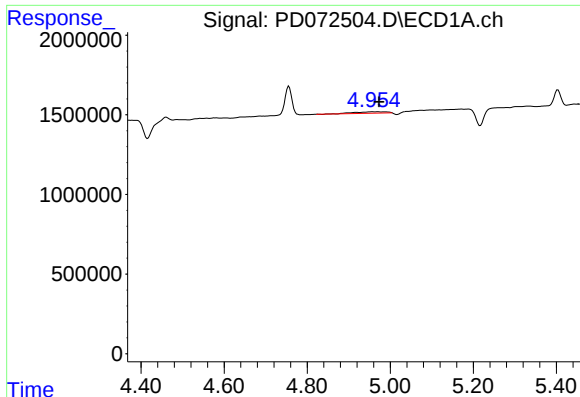

#11 cis-Chlordane


R.T.: 4.966 min  
Delta R.T.: -0.007 min  
Response: 506294  
Conc: 0.17 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :

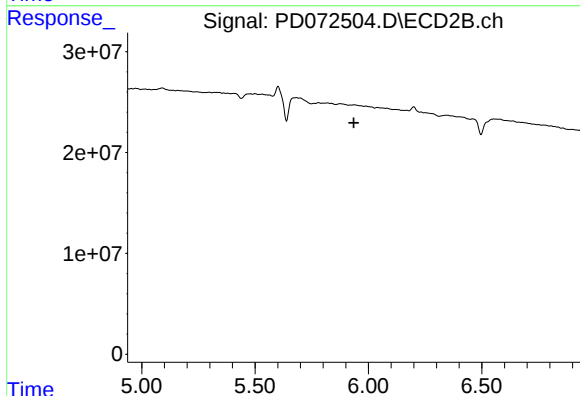


#11 cis-Chlordane

R.T.: 0.000 min  
Exp R.T. : 5.936 min  
Response: 0  
Conc: N.D.

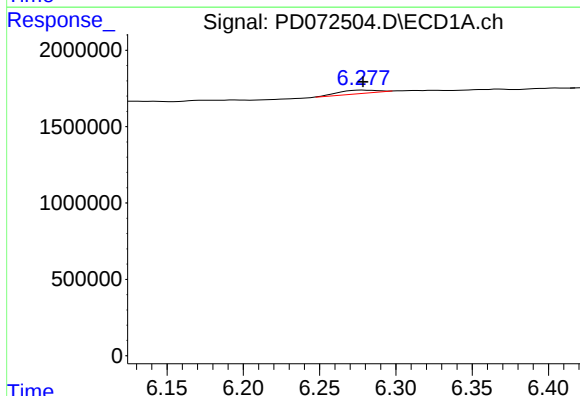


#19 Endosulfan Sulfate

R.T.: 6.279 min  
Delta R.T.: 0.001 min  
Response: 392519  
Conc: 0.16 ng/ml

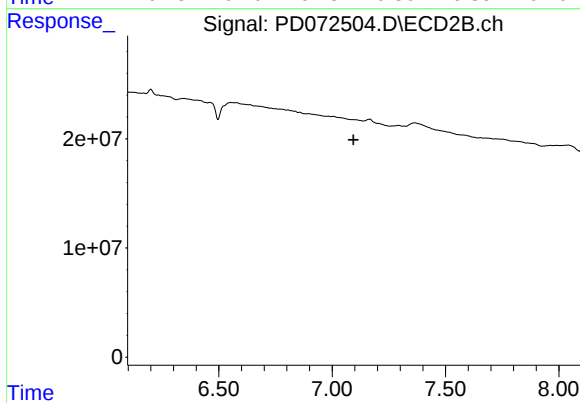

#19 Endosulfan Sulfate


R.T.: 0.000 min  
Exp R.T. : 7.095 min  
Response: 0  
Conc: N.D.

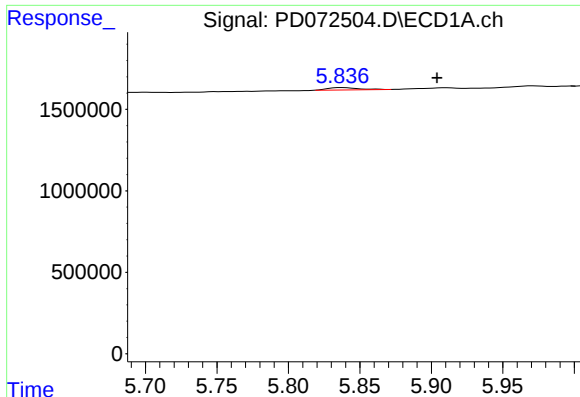

#24 Toxaphene-3


R.T.: 5.838 min  
Delta R.T.: -0.066 min  
Response: 223175  
Conc: 12.27 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :

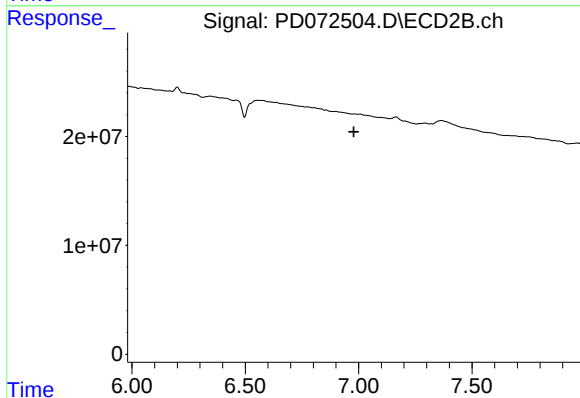


#24 Toxaphene-3

R.T.: 0.000 min  
Exp R.T. : 6.978 min  
Response: 0  
Conc: N.D.

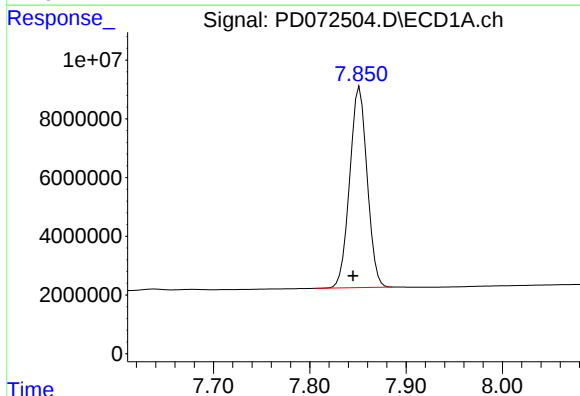

#27 Decachlorobiphenyl

R.T.: 7.852 min  
Delta R.T.: 0.007 min  
Response: 85992823  
Conc: 42.96 ng/ml

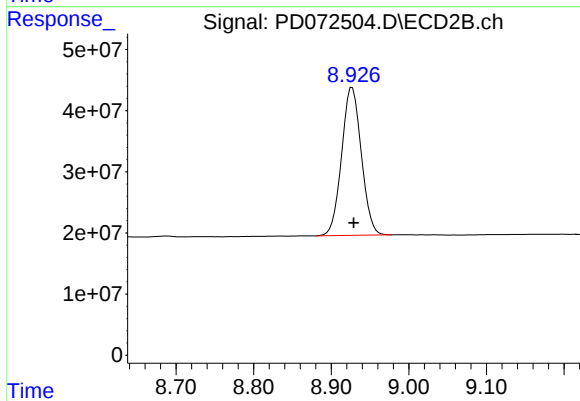

#27 Decachlorobiphenyl

R.T.: 8.927 min  
Delta R.T.: -0.002 min  
Response: 426749992  
Conc: 47.41 ng/ml