

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
 Data File : PD072503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2022 09:54
 Operator : AR\AJ
 Sample : PB148210BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS210

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 05:02:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.707	3.467	49214821	775.4E6	19.301	20.644
27)	SA Decachlor...	7.845	8.929	83498553	394.7E6	41.715	43.846
Target Compounds							
2)	A alpha-BHC	3.210	3.932	16598896	274.9E6	4.435m	5.585 #
3)	MA gamma-BHC...	3.542	4.266	15866555	232.2E6	4.820	5.570
4)	MA Heptachlor	3.874	4.833	15910672	166.3E6	4.603m	5.776 #
5)	MB Aldrin	4.154	5.172	15918531	140.7E6	4.699	5.846
6)	B beta-BHC	3.843	4.481	7611914	90401607	4.762m	5.431
7)	B delta-BHC	4.075	4.726	15535356	181.5E6	4.380	5.697 #
8)	B Heptachlo...	4.660	5.605	14807446	113.4E6	4.882	5.827
9)	A Endosulfan I	5.030	5.988	13592307	93898914	5.056	5.845m
10)	B trans-Chl...	4.910	5.858	14563265	101.5E6	4.685	5.423
11)	B cis-Chlor...	4.973	5.934	14535996	96462595	4.813	5.392
12)	B 4,4'-DDE	5.162	6.108	25793510	177.5E6	8.854	10.854
13)	MA Dieldrin	5.297	6.267	27799374	187.2E6	9.492	11.469
14)	MA Endrin	5.574	6.499	23708396	150.6E6	9.260	10.953
15)	B Endosulfa...	5.872	6.729	24155255	151.0E6	10.028	11.836
16)	A 4,4'-DDD	5.722	6.633	22022957	146.5E6	9.694	11.814
17)	MA 4,4'-DDT	5.971	6.941	19566937	132.3E6	8.852	10.997
18)	B Endrin al...	6.055	6.861	20311222	121.8E6	9.857	11.320
19)	B Endosulfa...	6.278	7.094	22900144	126.7E6	9.488	10.616
20)	A Methoxychlor	6.555	7.422	58914838	312.0E6	49.363	56.843
21)	B Endrin ke...	6.790	7.583	28175744	148.1E6	9.887	11.554

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
Data File : PD072503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2022 09:54
Operator : AR\AJ
Sample : PB148210BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 05:02:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

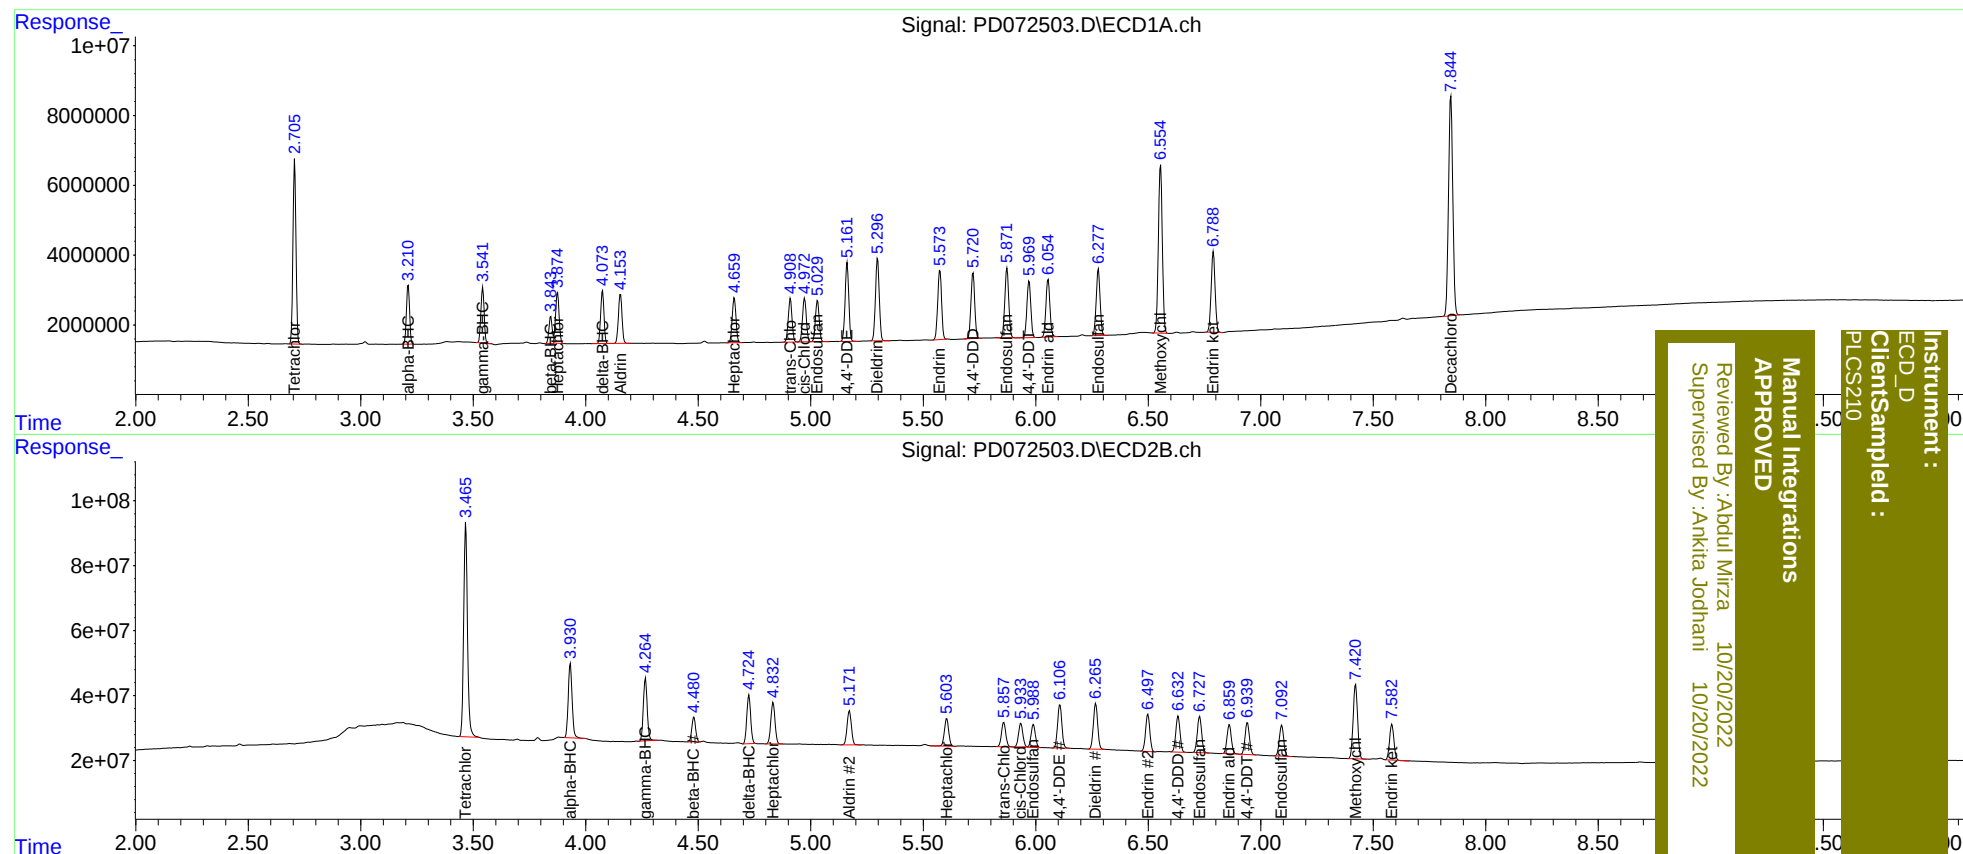

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022

Instrument :
ECD_D
Client Sampled :
PLCS210