

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
 Data File : PD072510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2022 13:53
 Operator : AR\AJ
 Sample : N5015-03MS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C1BE1MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 05:37:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.713	3.466	35402050	717.8E6	13.884	19.111 #
27)	SA Decachlor...	7.850	8.927	45007284	522.2E6	22.485	58.005 #
Target Compounds							
2)	A alpha-BHC	3.218	3.930	160.3E6	1963.4E6	42.822	39.892
3)	MA gamma-BHC...	3.550	4.264	166.6E6	1719.8E6	50.593	41.263
4)	MA Heptachlor	3.881	4.830	158.9E6	1260.0E6	45.980m	43.765m
5)	MB Aldrin	4.162	5.171	161.7E6	1125.7E6	47.737	46.787
6)	B beta-BHC	3.851	4.479	61497541	743.5E6	38.470m	44.660
7)	B delta-BHC	4.082	4.724	38002726	379.8E6	10.715	11.922
8)	B Heptachlo...	4.667	5.604	135.8E6	838.1E6	44.785	43.077
9)	A Endosulfan I	5.037	5.987	87349448	761.7E6	32.490	47.414m#
10)	B trans-Chl...	4.915	5.861	145.0E6	1083.7E6	46.646m	57.916m
11)	B cis-Chlor...	4.979	5.931	137.8E6	827.4E6	45.623	46.245m
12)	B 4,4'-DDE	5.168	6.106	281.6E6	1389.9E6	96.658	84.968
13)	MA Dieldrin	5.304	6.266	388.7E6	1485.6E6	132.726	91.019 #
14)	MA Endrin	5.580	6.498	252.1E6	1253.7E6	98.462	91.169
15)	B Endosulfa...	5.879	6.728	247.8E6	1246.2E6	102.871	97.679
16)	A 4,4'-DDD	5.726	6.630	204.6E6	1198.8E6	90.075m	96.662m
17)	MA 4,4'-DDT	5.976	6.940	212.8E6	1260.4E6	96.267	104.780
18)	B Endrin al...	6.061	6.859	175.0E6	935.1E6	84.920	86.922
19)	B Endosulfa...	6.284	7.092	167.4E6	883.1E6	69.351	73.963
20)	A Methoxychlor	6.559	7.420	525.5E6	2765.5E6	440.275m	503.799
21)	B Endrin ke...	6.794	7.582	234.9E6	1265.8E6	82.409	98.722

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
Data File : PD072510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2022 13:53
Operator : AR\AJ
Sample : N5015-03MS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 05:37:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

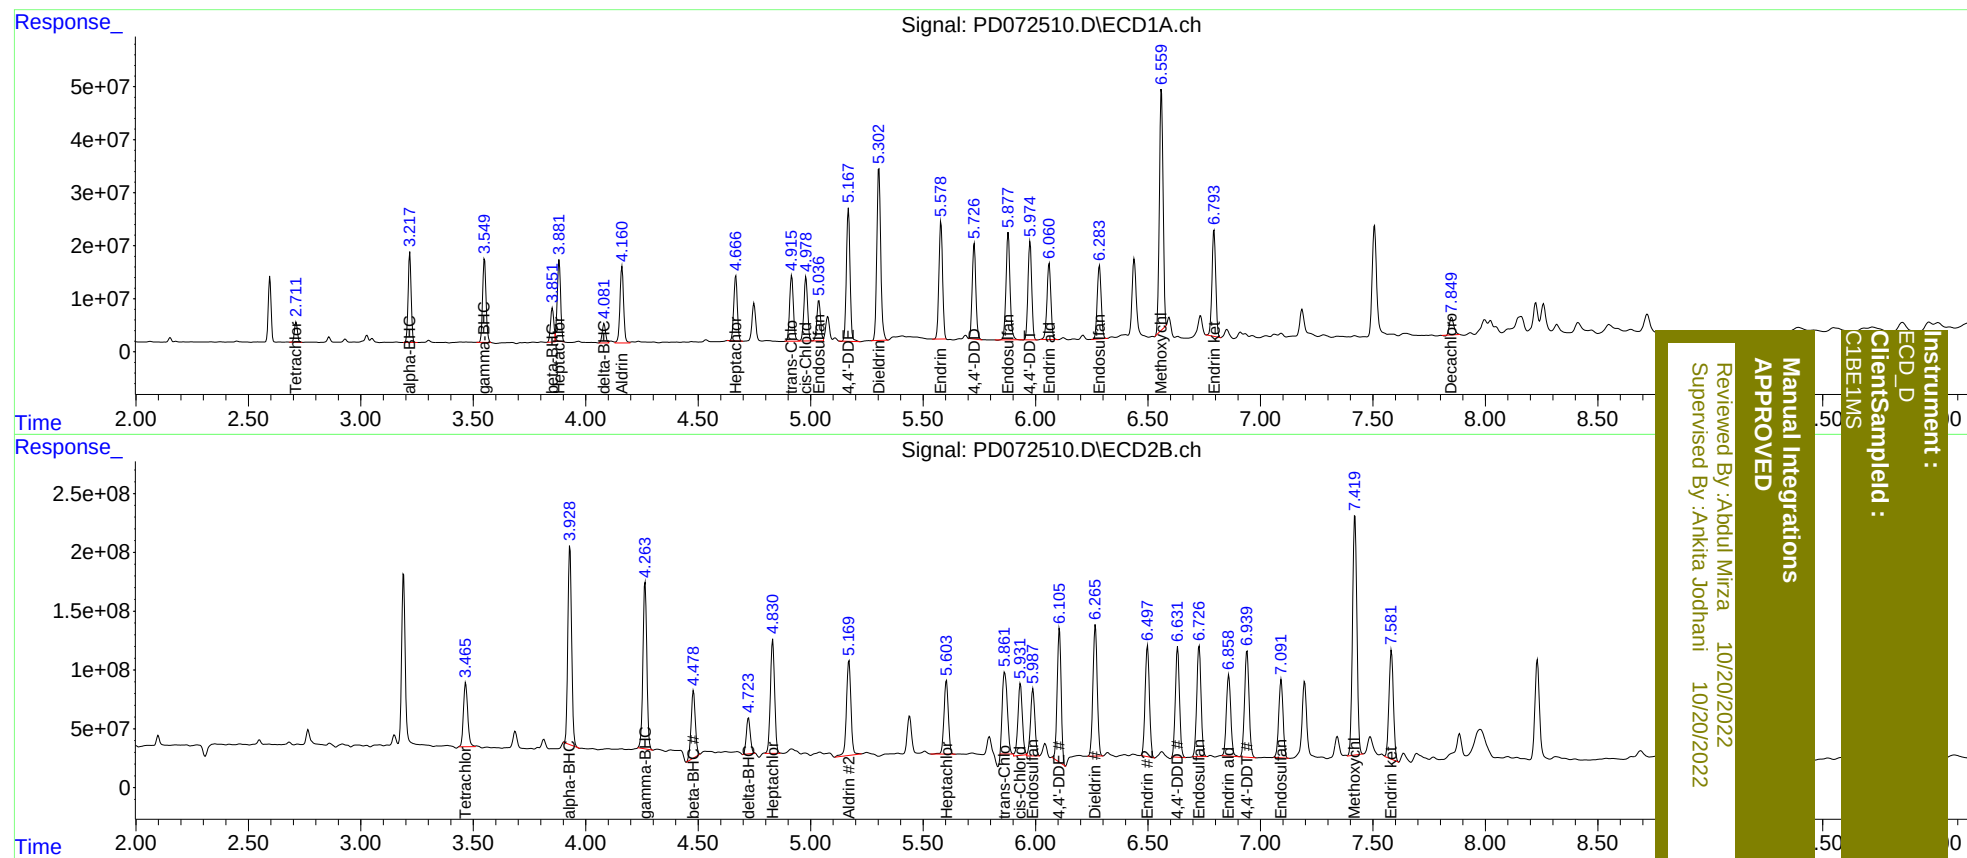

Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
CIBELMS