

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
 Data File : PD072511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2022 14:06
 Operator : AR\AJ
 Sample : N5015-04MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C1BE1MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 05:38:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.468	36324323	708.1E6	14.246	18.853 #
27)	SA Decachlor...	7.845	8.926	52546712	536.4E6	26.252	59.591 #
Target Compounds							
2)	A alpha-BHC	3.211	3.932	160.2E6	1913.3E6	42.791	38.875
3)	MA gamma-BHC...	3.543	4.266	166.0E6	1695.0E6	50.425	40.668
4)	MA Heptachlor	3.873	4.831	157.1E6	1222.3E6	45.442m	42.455m
5)	MB Aldrin	4.155	5.171	160.4E6	1098.8E6	47.336	45.669
6)	B beta-BHC	3.843	4.481	67794648	722.3E6	42.409m	43.391
7)	B delta-BHC	4.075	4.725	37805664	376.8E6	10.660	11.826
8)	B Heptachlo...	4.660	5.604	135.3E6	818.1E6	44.603	42.047
9)	A Endosulfan I	5.030	5.987	84443394	733.9E6	31.409	45.683m#
10)	B trans-Chl...	4.908	5.862	141.9E6	1052.6E6	45.640m	56.253m
11)	B cis-Chlor...	4.972	5.932	134.2E6	786.1E6	44.426	43.941m
12)	B 4,4'-DDE	5.161	6.106	280.3E6	1371.6E6	96.207	83.848
13)	MA Dieldrin	5.297	6.266	389.9E6	1446.2E6	133.137	88.607 #
14)	MA Endrin	5.573	6.498	250.0E6	1245.9E6	97.656	90.601
15)	B Endosulfa...	5.872	6.728	246.9E6	1217.1E6	102.483	95.402
16)	A 4,4'-DDD	5.719	6.630	202.4E6	1153.5E6	89.096m	93.011m
17)	MA 4,4'-DDT	5.969	6.940	208.8E6	1212.5E6	94.454	100.797
18)	B Endrin al...	6.054	6.859	171.1E6	922.1E6	83.021	85.716
19)	B Endosulfa...	6.277	7.092	166.5E6	857.7E6	68.963	71.838
20)	A Methoxychlor	6.553	7.420	503.5E6	2716.7E6	421.862	494.899
21)	B Endrin ke...	6.787	7.582	230.9E6	1232.6E6	81.031	96.131

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
Data File : PD072511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2022 14:06
Operator : AR\AJ
Sample : N5015-04MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 05:38:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

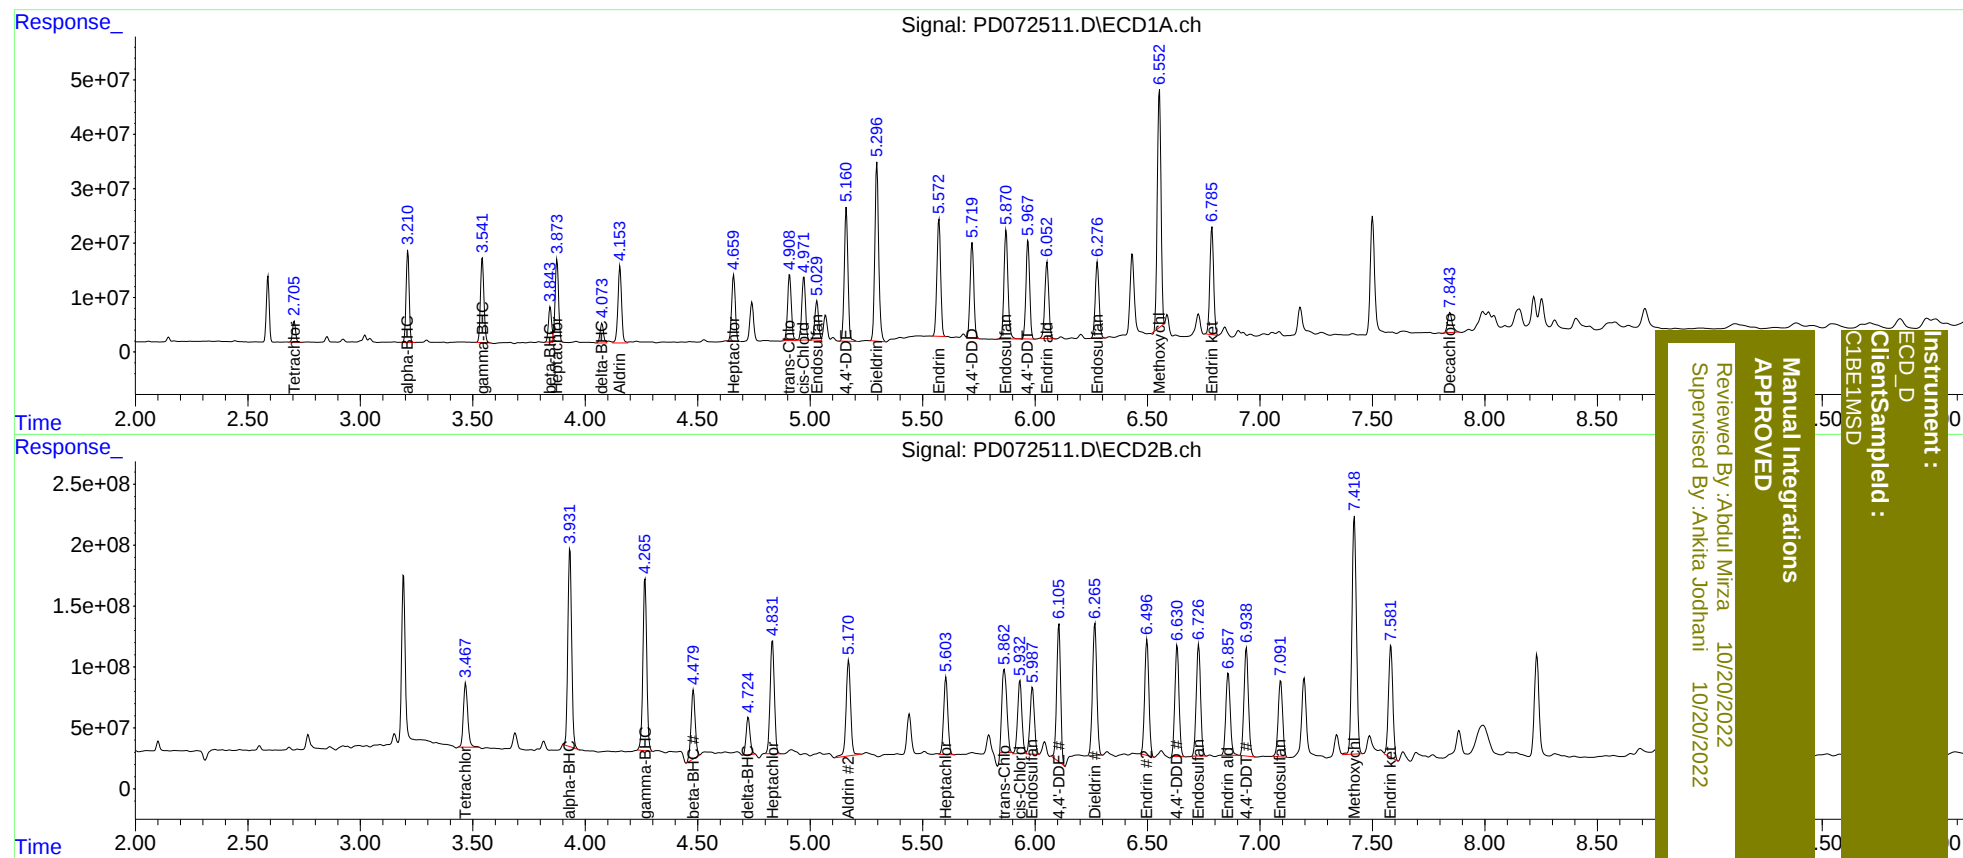

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022

Instrument :
ECD_D
ClientSampled :
CIBELMSD