

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
 Data File : PD072512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2022 14:20
 Operator : AR\AJ
 Sample : PB148370BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS370

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/20/2022
 Supervised By : Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 05:38:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 20 01:04:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.706	3.467	46800497	713.7E6	18.355	19.002
27)	SA Decachlor...	7.843	8.926	79829813	370.9E6	39.882	41.196
Target Compounds							
2)	A alpha-BHC	3.210	3.931	15714156	243.9E6	4.198	4.956
3)	MA gamma-BHC...	3.541	4.265	15064133	201.2E6	4.576	4.826
4)	MA Heptachlor	3.873	4.832	14485150	152.2E6	4.191m	5.285 #
5)	MB Aldrin	4.153	5.171	15007179	125.7E6	4.430	5.225
6)	B beta-BHC	3.842	4.481	6987394	78504092	4.371m	4.716
7)	B delta-BHC	4.074	4.725	14595849	160.7E6	4.115	5.044
8)	B Heptachlo...	4.660	5.605	13413647	103.2E6	4.422	5.305
9)	A Endosulfan I	5.029	5.988	11898009	98771673	4.426	6.148m#
10)	B trans-Chl...	4.908	5.858	13193753	85548077	4.244	4.572
11)	B cis-Chlor...	4.971	5.934	12753414	84276049	4.223	4.711
12)	B 4,4'-DDE	5.160	6.107	23880894	154.1E6	8.198	9.421
13)	MA Dieldrin	5.295	6.266	24498458	167.0E6	8.365	10.233
14)	MA Endrin	5.572	6.497	19923319	119.2E6	7.782	8.667m
15)	B Endosulfa...	5.870	6.728	21580040	130.8E6	8.959	10.254
16)	A 4,4'-DDD	5.719	6.632	21538153	131.3E6	9.481	10.588
17)	MA 4,4'-DDT	5.968	6.940	16677531	112.5E6	7.545	9.351
18)	B Endrin al...	6.053	6.860	18216032	127.8E6	8.840	11.881 #
19)	B Endosulfa...	6.276	7.092	19940748	109.3E6	8.262	9.151
20)	A Methoxychlor	6.552	7.420	51762043	263.0E6	43.370	47.919
21)	B Endrin ke...	6.786	7.580	26730599	120.7E6	9.380m	9.417m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD101922\
Data File : PD072512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2022 14:20
Operator : AR\AJ
Sample : PB148370BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 05:38:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD101722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Oct 20 01:04:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

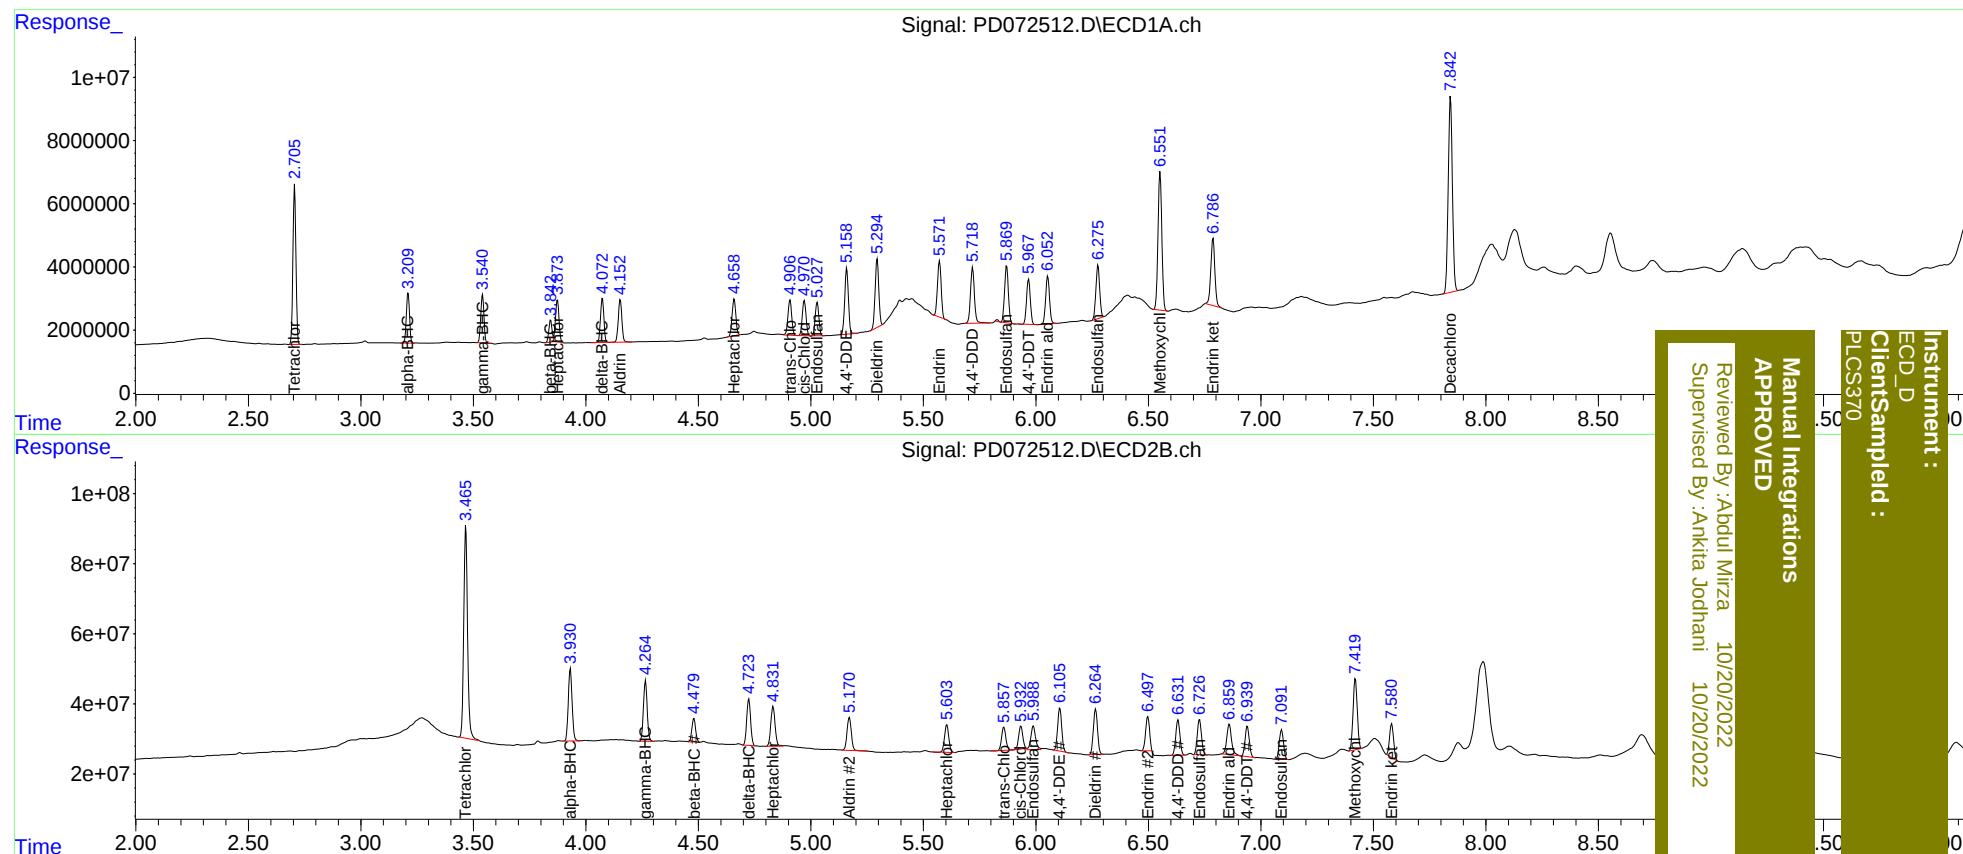

Reviewed By: Abdul Mirza 10/20/2022
Supervised By: Ankita Jodhani 10/20/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS370