

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110121\
 Data File : PD066648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2021 08:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 01:56:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	0.000	9.036	0	7013813	N.D.	1.302 #
Target Compounds							
7)	B delta-BHC	0.000	5.053f	0	2712668	N.D.	0.297 #
8)	B Heptachlo...	0.000	5.837	0	75169303	N.D.	10.371 #
9)	A Endosulfan I	0.000	6.214f	0	1721732	N.D.	0.218 #
13)	MA Dieldrin	0.000	6.477f	0	12296181	N.D.	1.482 #
14)	MA Endrin	5.992f	6.658	1476899	43539201	0.706	6.326 #
15)	B Endosulfa...	6.259	0.000	10267057	0	5.163	N.D. #
17)	MA 4,4'-DDT	0.000	7.085	0	528722	N.D.	0.073 #
21)	B Endrin ke...	7.088f	0.000	4401440	0	2.017	N.D. #
22)	Mirex	0.000	8.141	0	5605052	N.D.	0.948 #
27)	Chlordane-5	6.259	0.000	10267057	0	121.401	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110121\
Data File : PD066648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2021 08:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 01:56:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

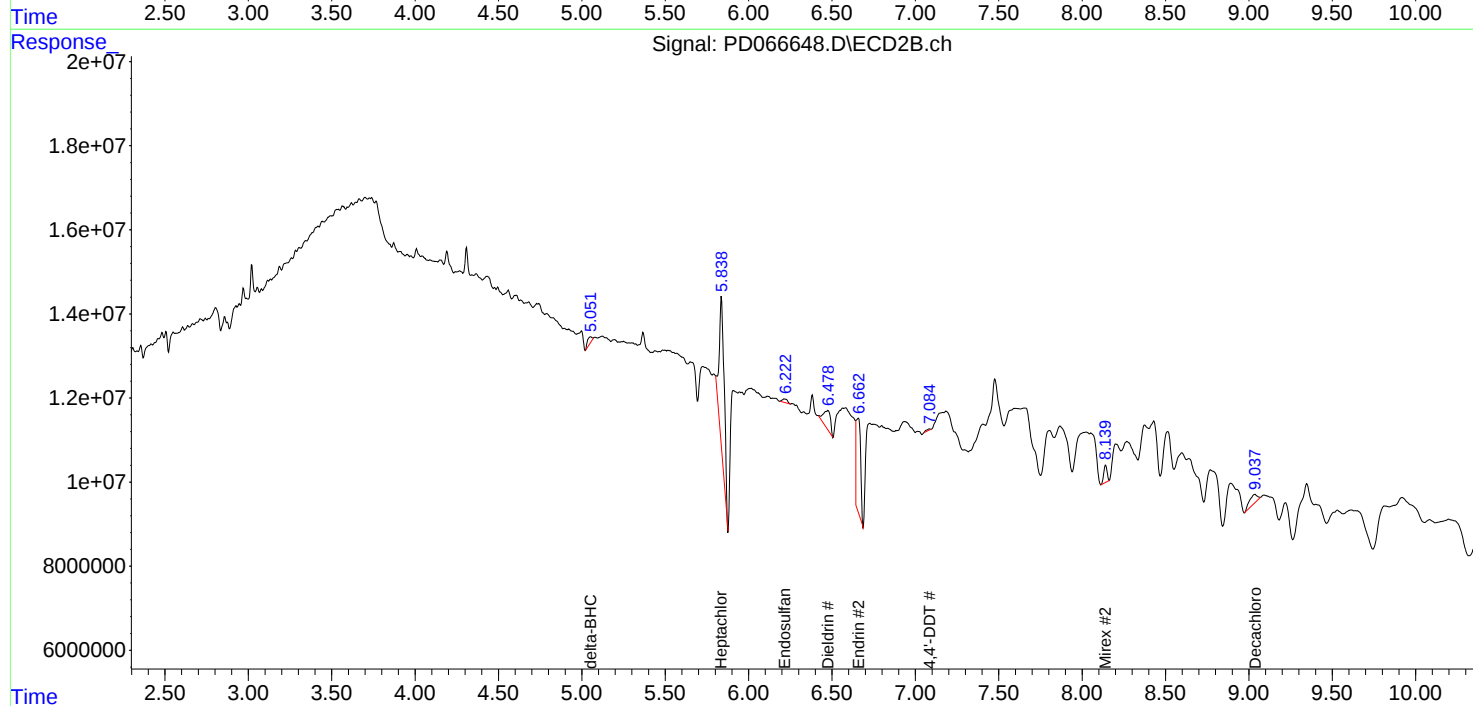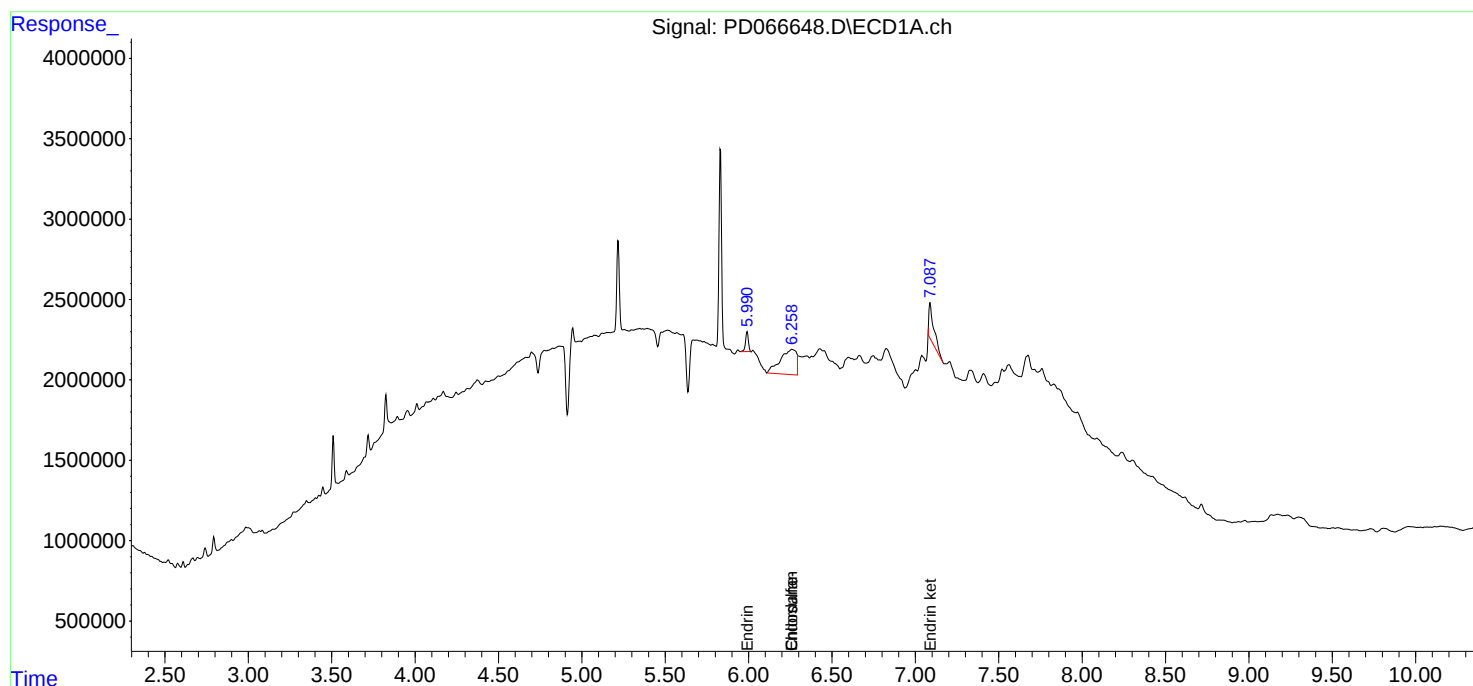


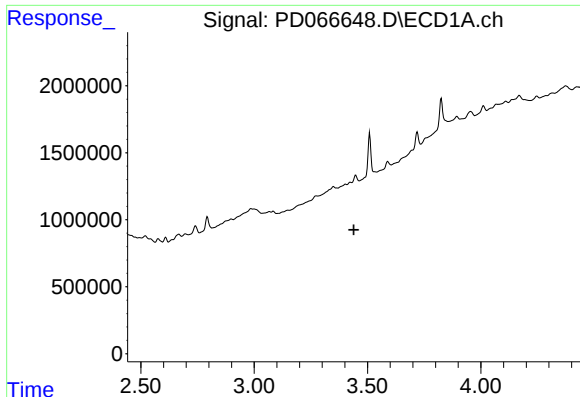

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

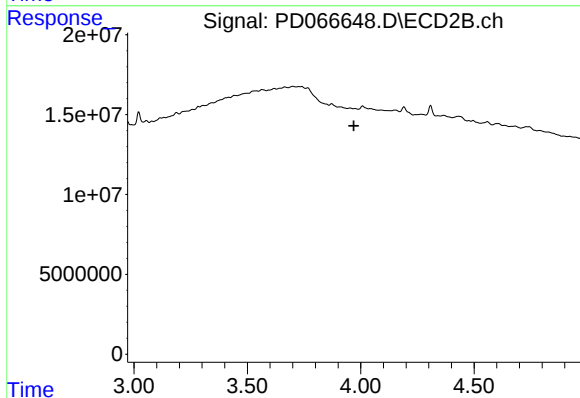


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

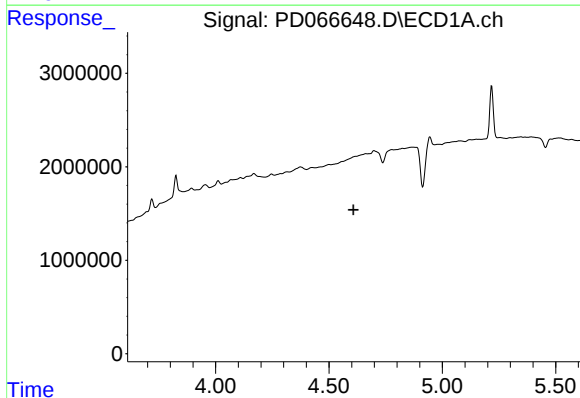


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

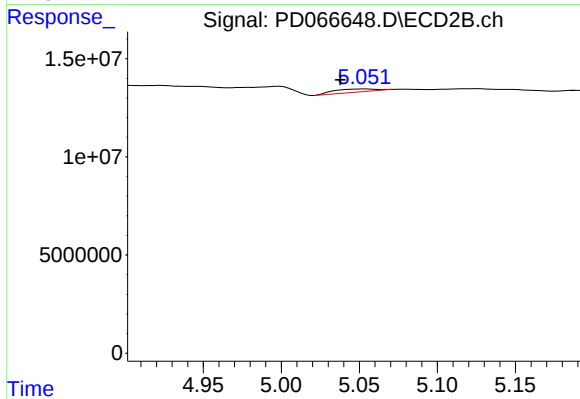

#7 delta-BHC


R.T.: 5.053 min
Delta R.T.: 0.015 min
Response: 2712668
Conc: 0.30 ng/ml

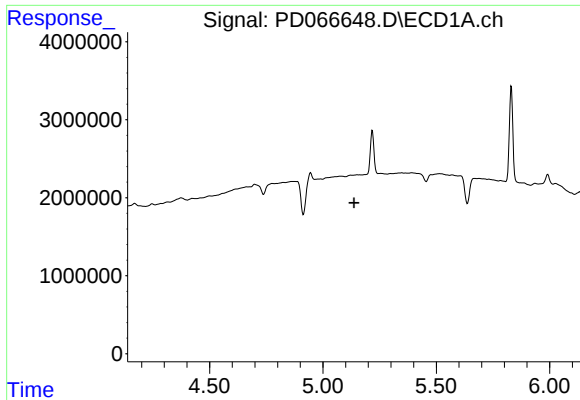

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

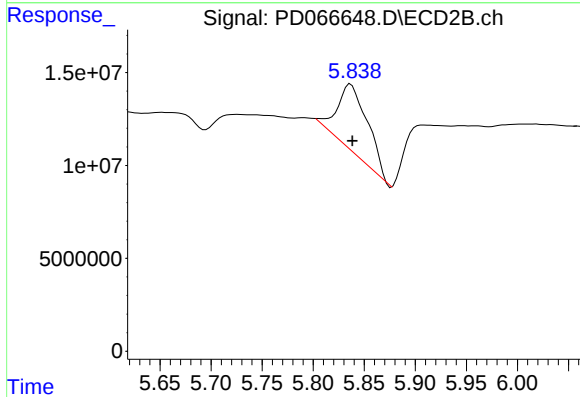


#8 Heptachlor epoxide

R.T.: 5.837 min
Delta R.T.: -0.002 min
Response: 75169303
Conc: 10.37 ng/ml

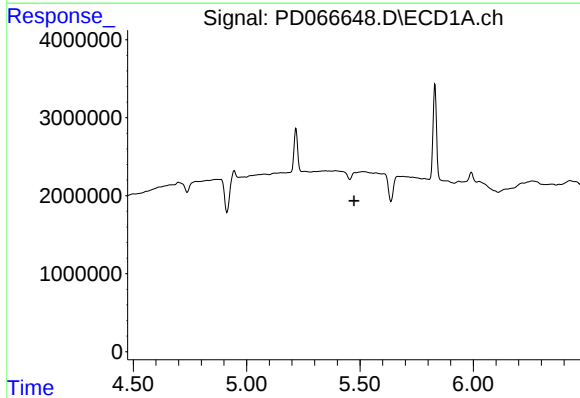


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.474 min
Response: 0
Conc: N.D.

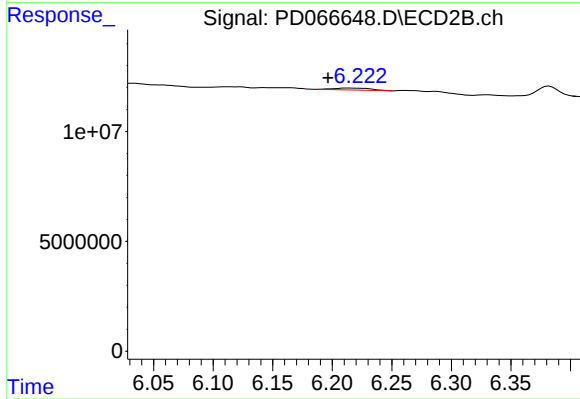

#9 Endosulfan I


R.T.: 6.214 min
Delta R.T.: 0.018 min
Response: 1721732
Conc: 0.22 ng/ml

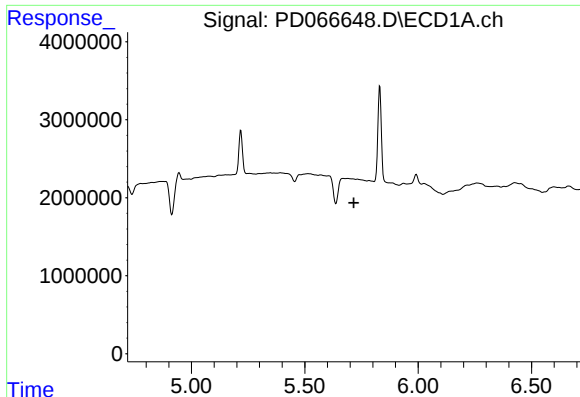

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.716 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

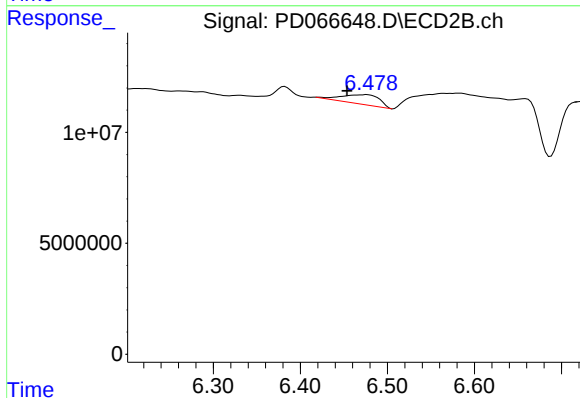


#13 Dieldrin

R.T.: 6.477 min
Delta R.T.: 0.023 min
Response: 12296181
Conc: 1.48 ng/ml

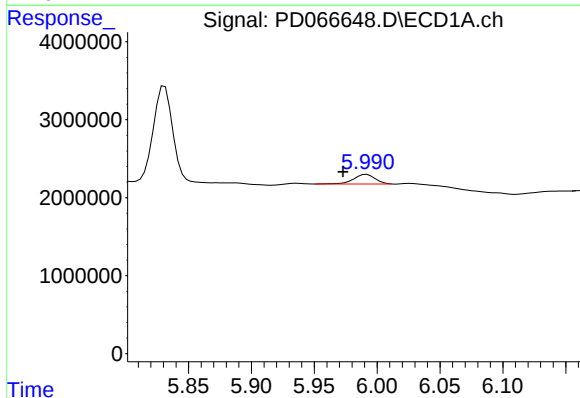


#14 Endrin

R.T.: 5.992 min
Delta R.T.: 0.019 min
Response: 1476899
Conc: 0.71 ng/ml

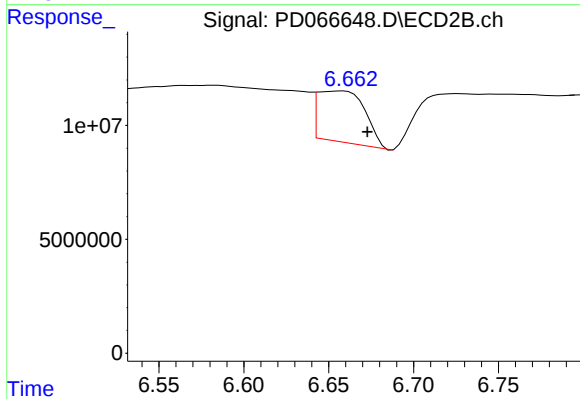

#14 Endrin


R.T.: 6.658 min
Delta R.T.: -0.014 min
Response: 43539201
Conc: 6.33 ng/ml

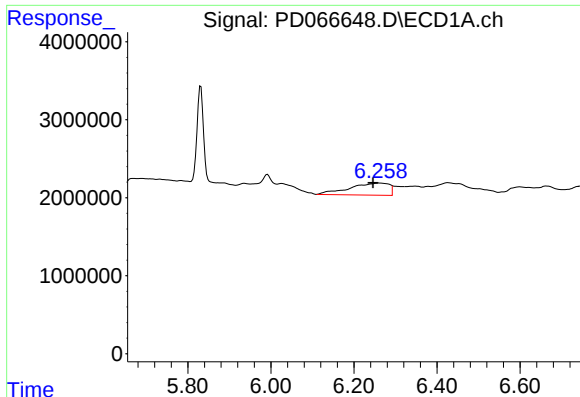

#15 Endosulfan II


R.T.: 6.259 min
Delta R.T.: 0.013 min
Response: 10267057
Conc: 5.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

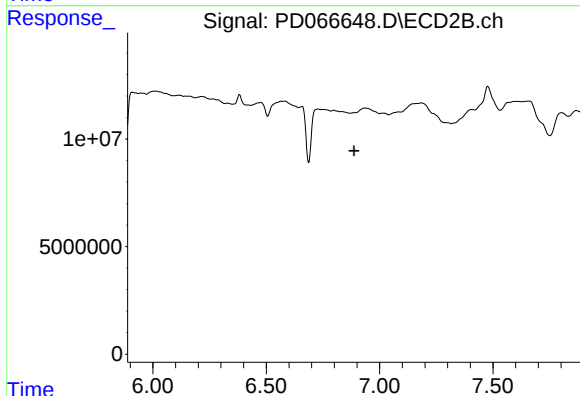


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.888 min
Response: 0
Conc: N.D.

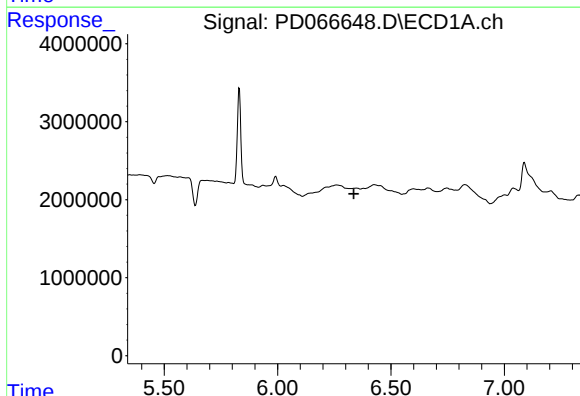


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.337 min
Response: 0
Conc: N.D.

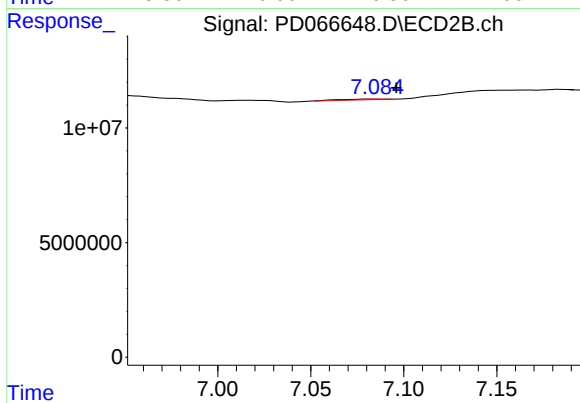

#17 4,4'-DDT


R.T.: 7.085 min
Delta R.T.: -0.011 min
Response: 528722
Conc: 0.07 ng/ml

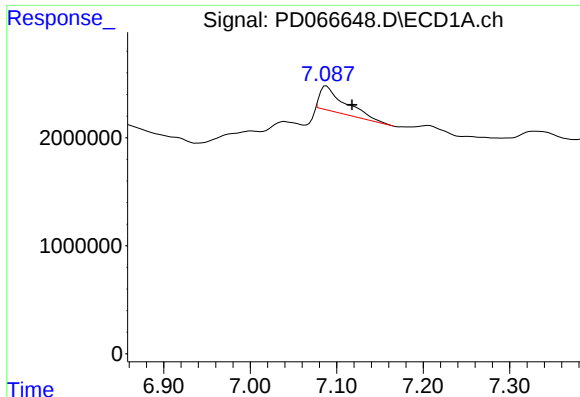

#21 Endrin ketone


R.T.: 7.088 min
Delta R.T.: -0.029 min
Response: 4401440
Conc: 2.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

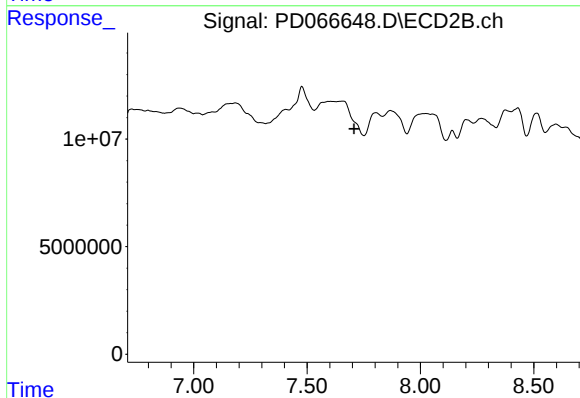


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.707 min
Response: 0
Conc: N.D.

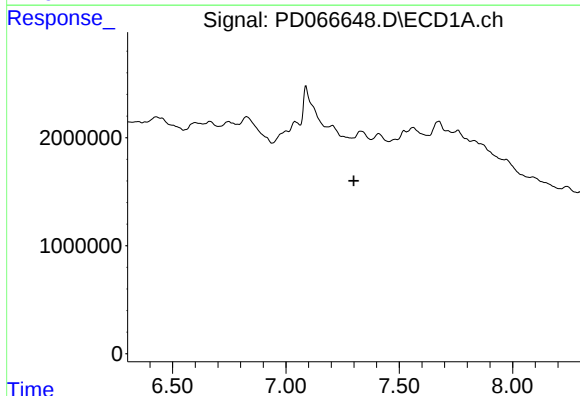


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.299 min
Response: 0
Conc: N.D.

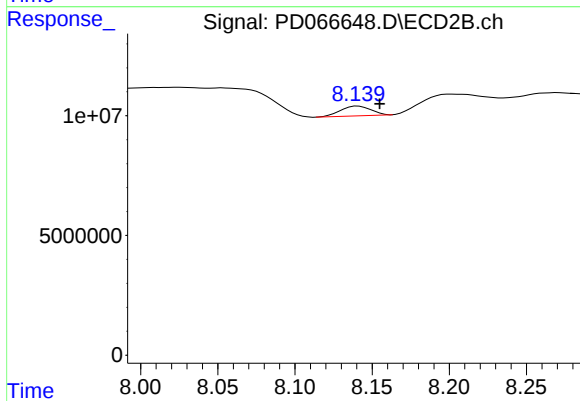

#22 Mirex


R.T.: 8.141 min
Delta R.T.: -0.014 min
Response: 5605052
Conc: 0.95 ng/ml

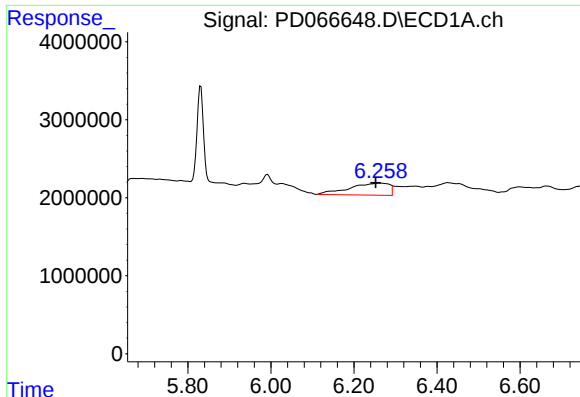

#27 Chlordane-5


R.T.: 6.259 min
Delta R.T.: 0.007 min
Response: 10267057
Conc: 121.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

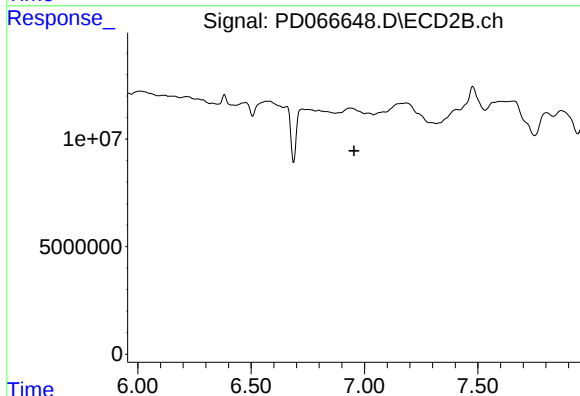


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.955 min
Response: 0
Conc: N.D.

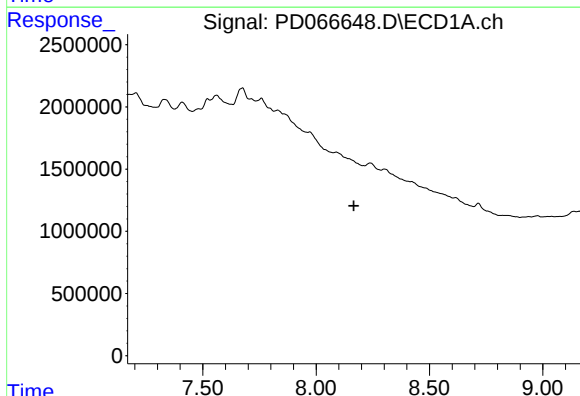

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.166 min
Response: 0
Conc: N.D.

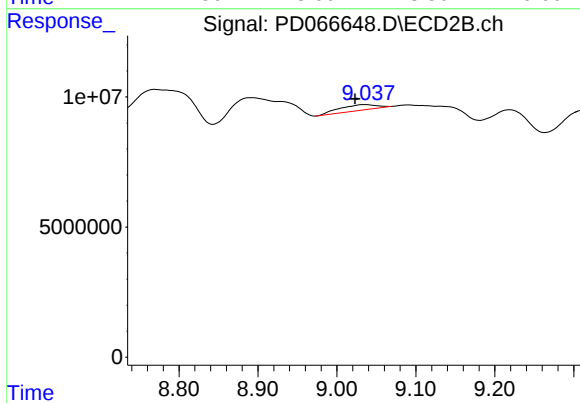

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: 0.013 min
Response: 7013813
Conc: 1.30 ng/ml