

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110121\
 Data File : PD066658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2021 12:29
 Operator : AR\AJ
 Sample : PB139886BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 02:08:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.968	37257984	171.6E6	19.968	21.211
28)	SA Decachlor...	8.165	9.022	22481828	115.1E6	19.458	21.377
Target Compounds							
6)	B beta-BHC	0.000	4.845f	0	1354020	N.D.	0.291 #
8)	B Heptachlo...	0.000	5.867f	0	1773989	N.D.	0.245 #
15)	B Endosulfa...	6.263f	0.000	1700565	0	0.855	N.D. #
22)	Mirex	0.000	8.182f	0	3187984	N.D.	0.539 #
27)	Chlordane-5	6.263	0.000	1700565	0	20.108	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110121\
Data File : PD066658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2021 12:29
Operator : AR\AJ
Sample : PB139886BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 02:08:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

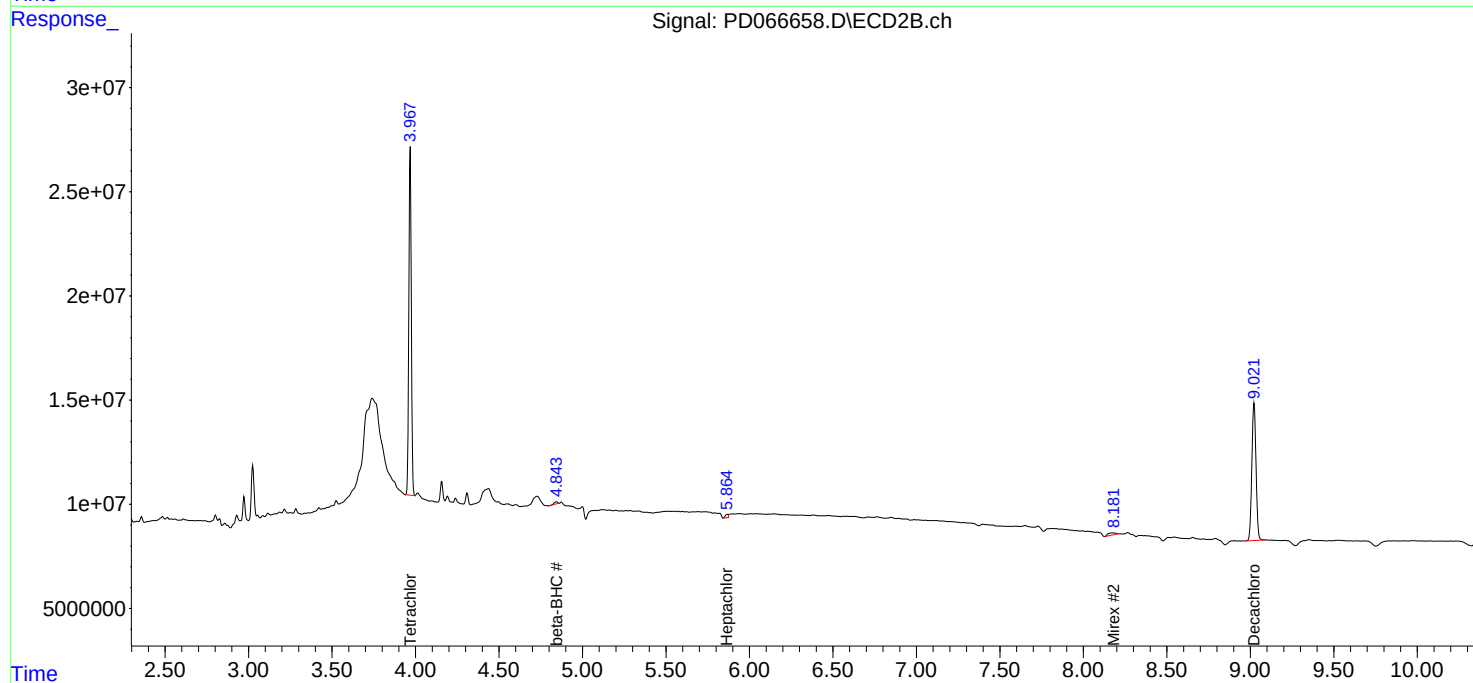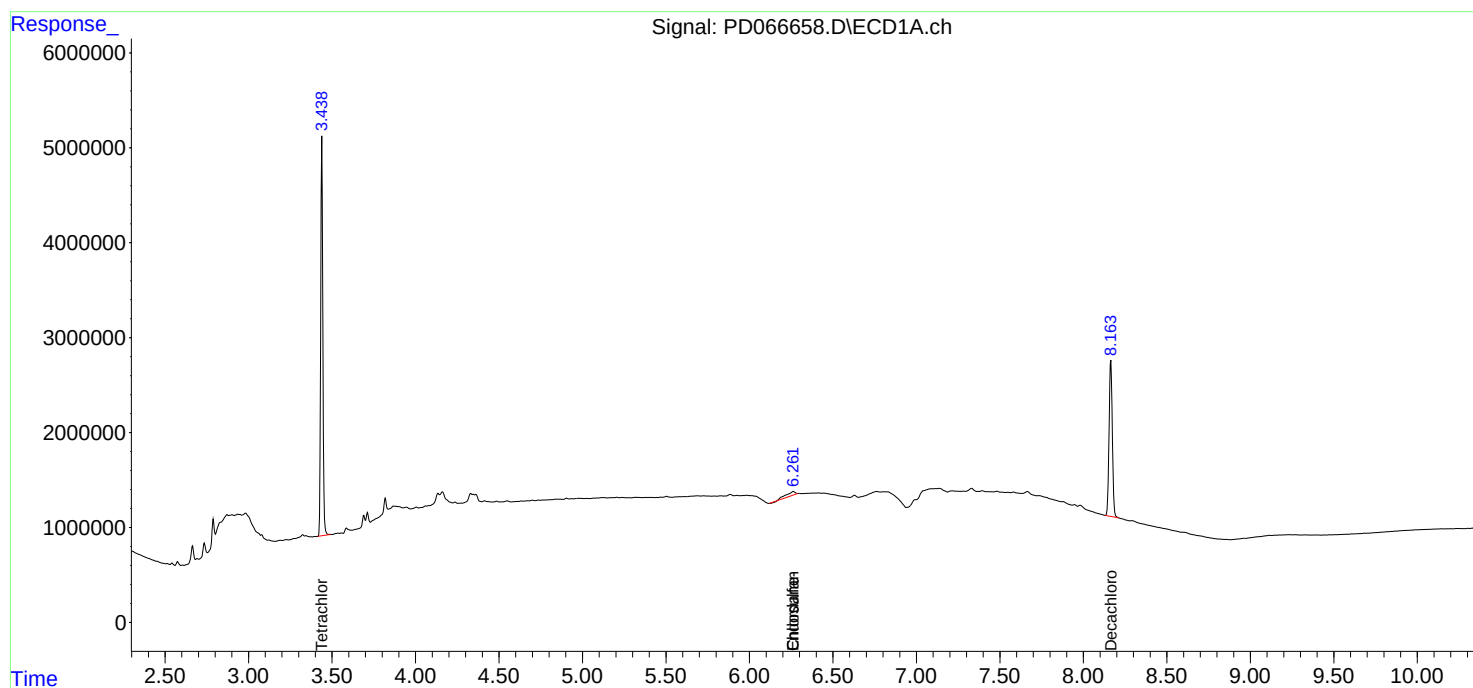


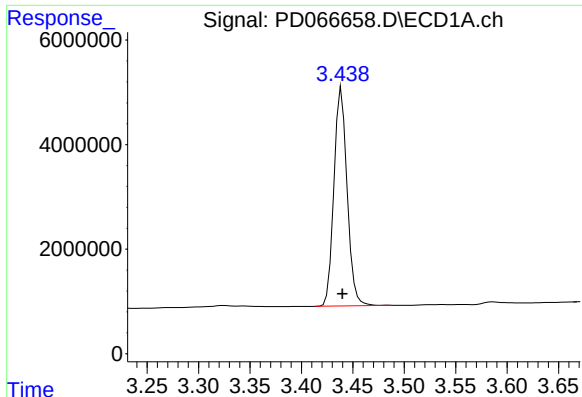

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 37257984
Conc: 19.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

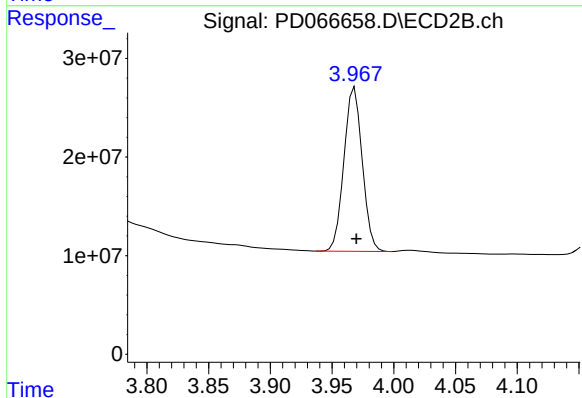


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 171646580
Conc: 21.21 ng/ml

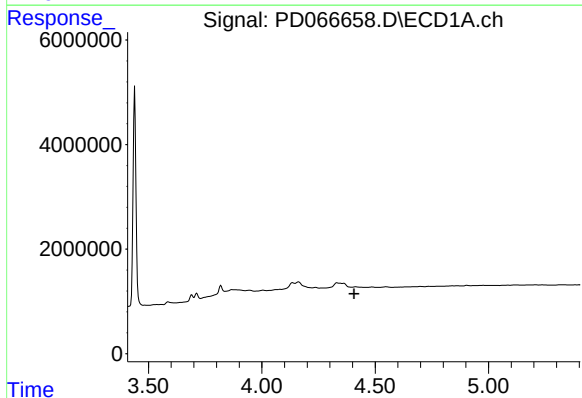


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.406 min
Response: 0
Conc: N.D.

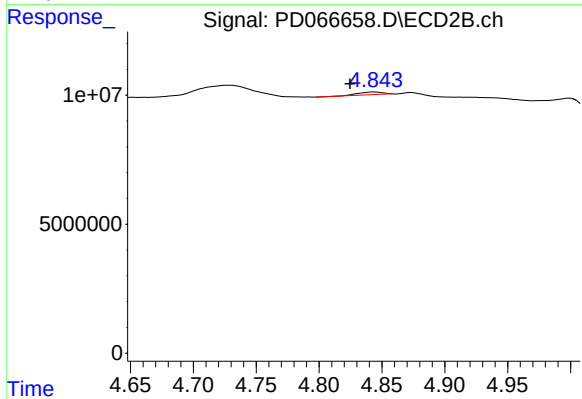

#6 beta-BHC


R.T.: 4.845 min
Delta R.T.: 0.020 min
Response: 1354020
Conc: 0.29 ng/ml

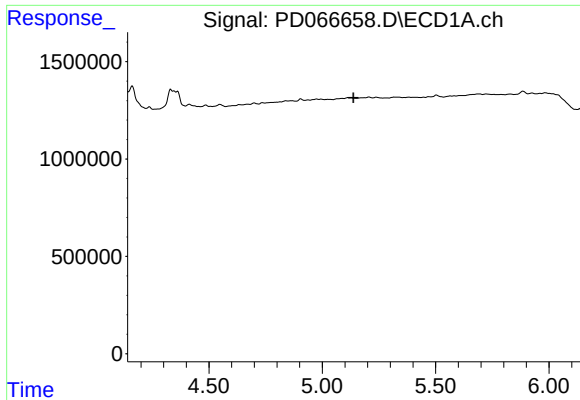

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

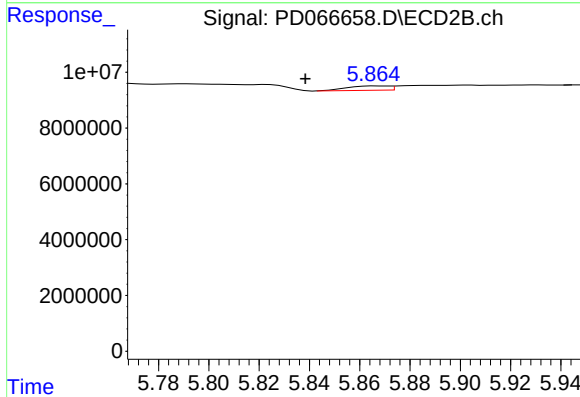


#8 Heptachlor epoxide

R.T.: 5.867 min
Delta R.T.: 0.029 min
Response: 1773989
Conc: 0.24 ng/ml

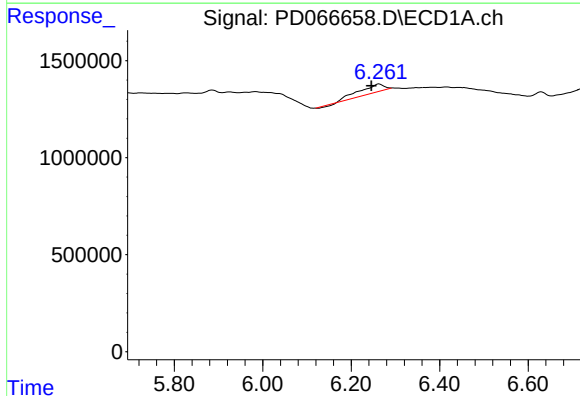


#15 Endosulfan II

R.T.: 6.263 min
Delta R.T.: 0.017 min
Response: 1700565
Conc: 0.86 ng/ml

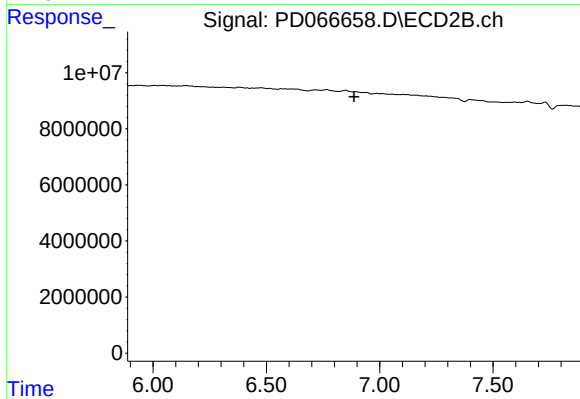

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.888 min
Response: 0
Conc: N.D.

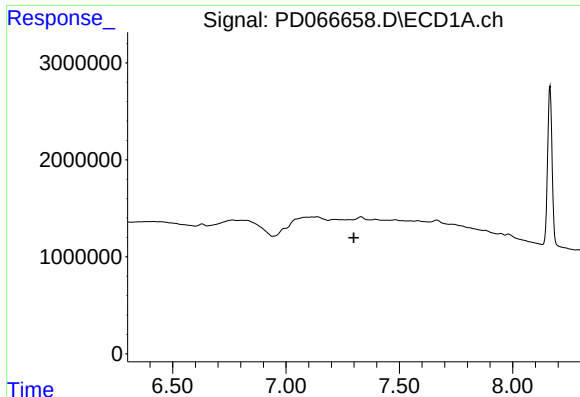

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.299 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

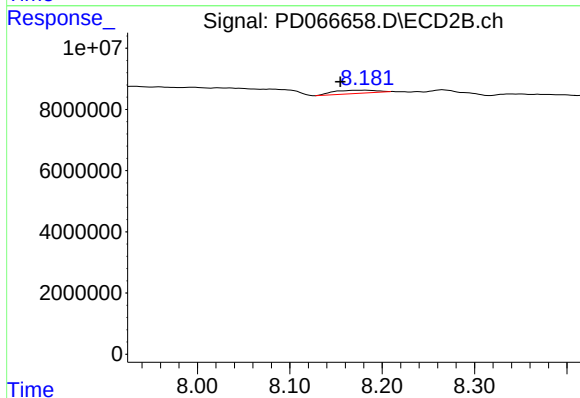


#22 Mirex

R.T.: 8.182 min
Delta R.T.: 0.028 min
Response: 3187984
Conc: 0.54 ng/ml

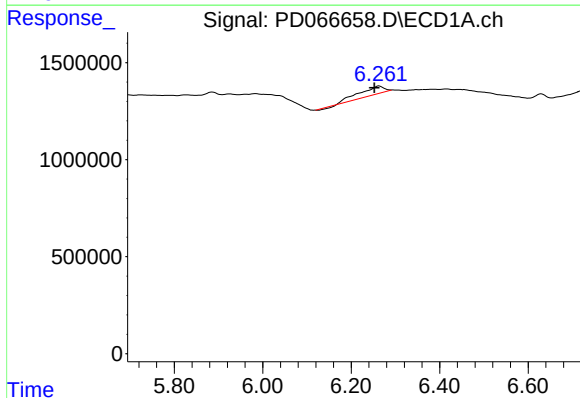


#27 Chlordane-5

R.T.: 6.263 min
Delta R.T.: 0.010 min
Response: 1700565
Conc: 20.11 ng/ml

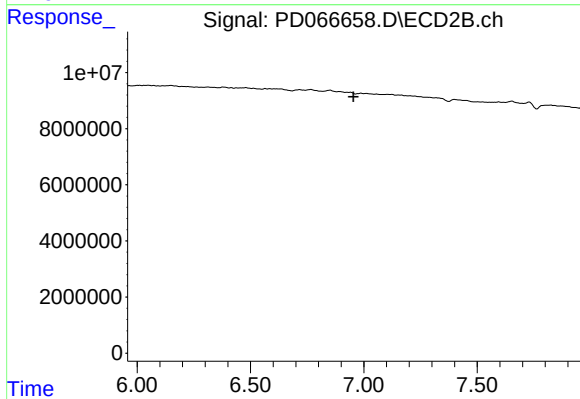

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.955 min
Response: 0
Conc: N.D.

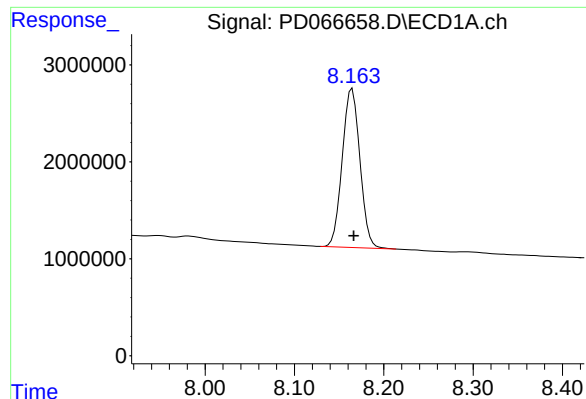

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.002 min
Response: 22481828
Conc: 19.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

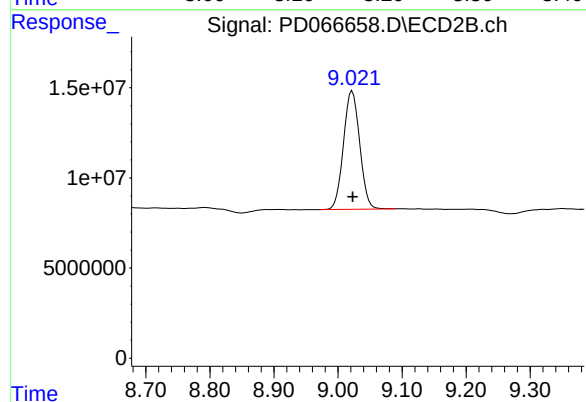

#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.000 min
Response: 115147493
Conc: 21.38 ng/ml