

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110121\
 Data File : PD066662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2021 13:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 02:09:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	3.968	39501301	180.2E6	21.171	22.263
28)	SA Decachlor...	8.173	9.027	24467078	124.8E6	21.176	23.170
Target Compounds							
4)	MA Heptachlor	4.422f	5.132f	1919890	1402256	0.647	0.143 #
6)	B beta-BHC	4.422f	0.000	1919890	0	1.537	N.D. #
7)	B delta-BHC	0.000	5.060f	0	3348223	N.D.	0.366 #
8)	B Heptachlo...	0.000	5.862f	0	232144	N.D.	0.032 #
15)	B Endosulfa...	0.000	6.885	0	2062538	N.D.	0.292 #
17)	MA 4,4'-DDT	0.000	7.069f	0	1341566	N.D.	0.185 #
21)	B Endrin ke...	0.000	7.729f	0	2021368	N.D.	0.240 #
27)	Chlordane-5	0.000	6.932f	0	99022	N.D.	0.363 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110121\
Data File : PD066662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2021 13:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 02:09:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

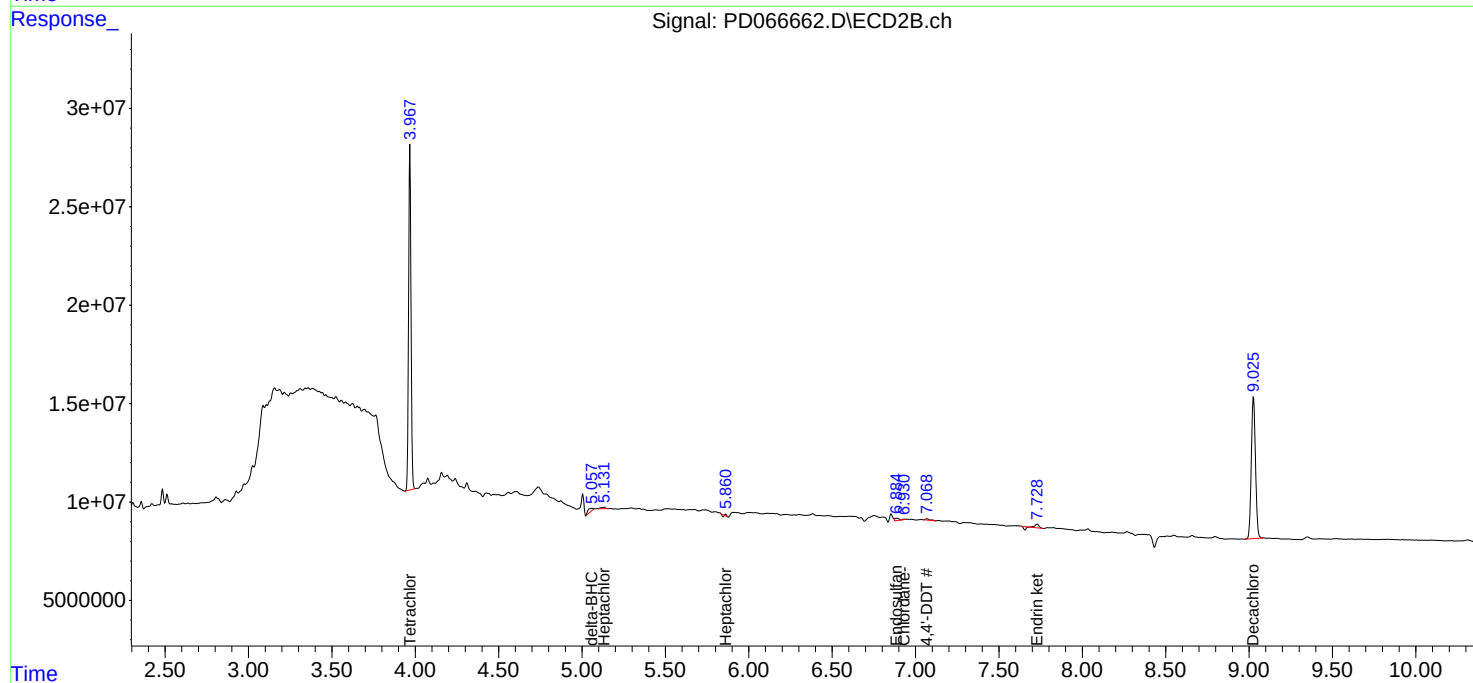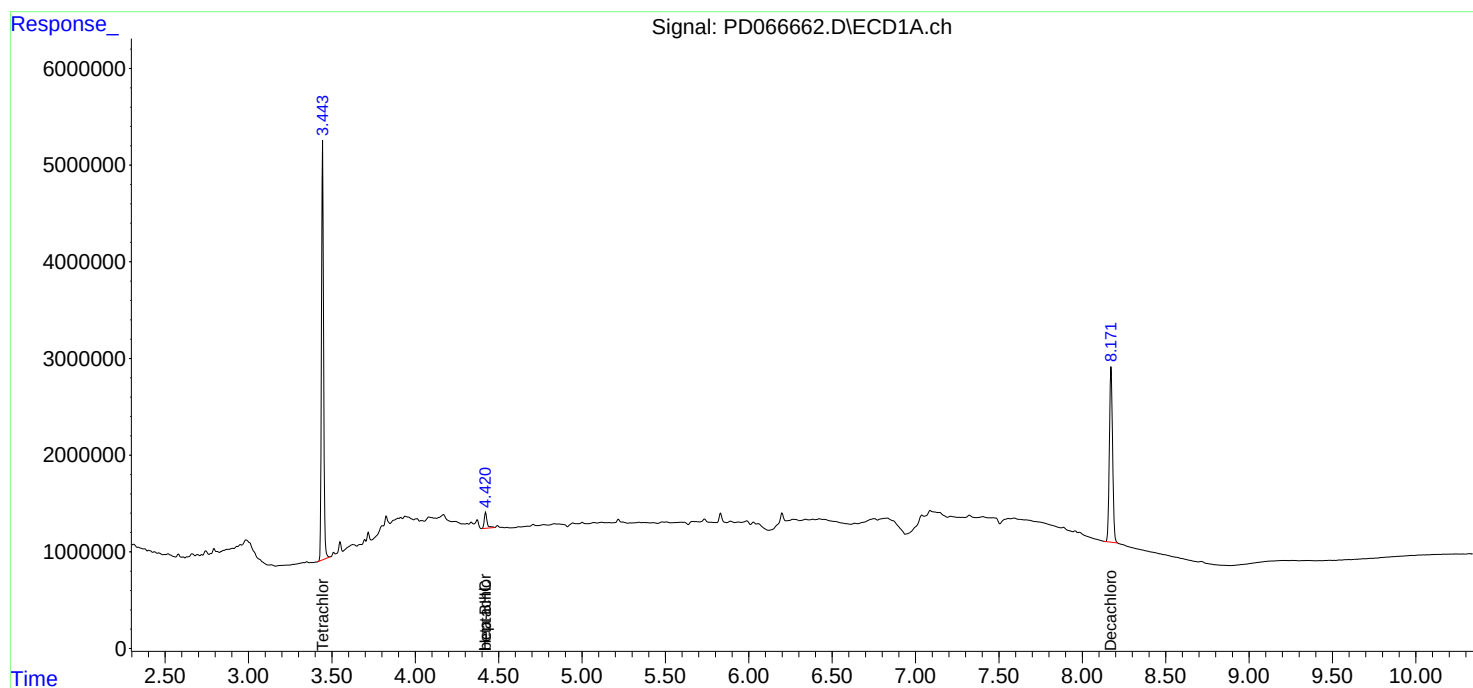


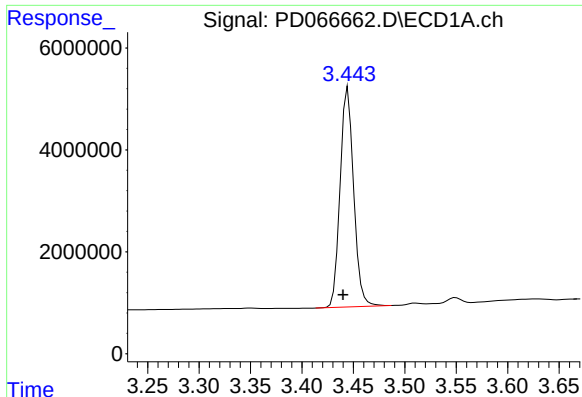

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.005 min
Response: 39501301
Conc: 21.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

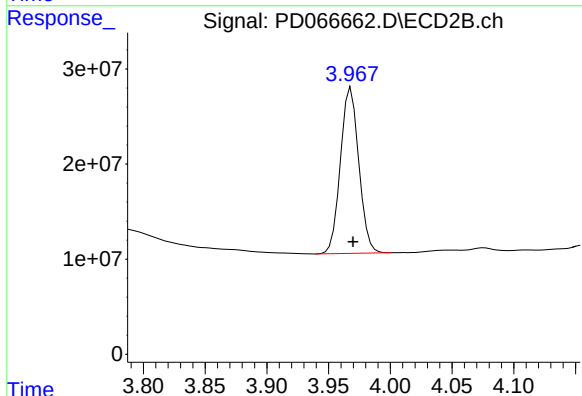


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: -0.002 min
Response: 180157447
Conc: 22.26 ng/ml

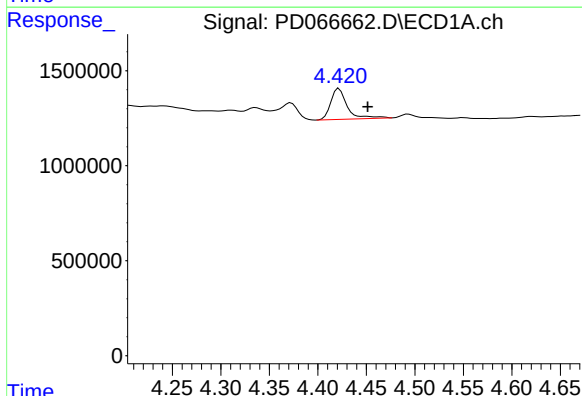


#4 Heptachlor

R.T.: 4.422 min
Delta R.T.: -0.030 min
Response: 1919890
Conc: 0.65 ng/ml

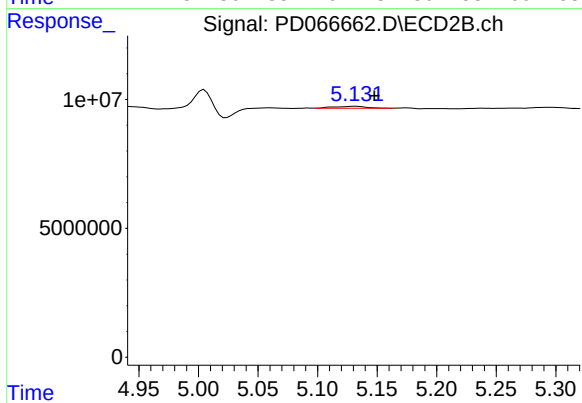

#4 Heptachlor


R.T.: 5.132 min
Delta R.T.: -0.015 min
Response: 1402256
Conc: 0.14 ng/ml

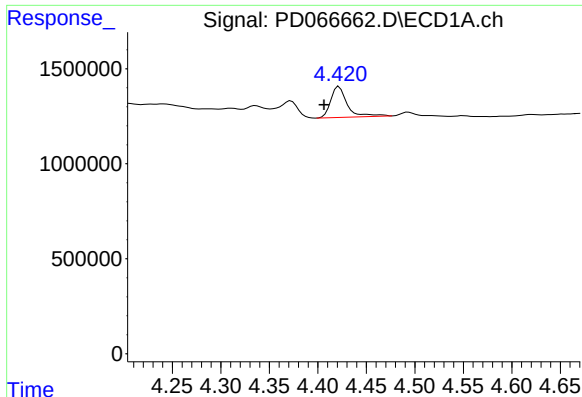

#6 beta-BHC


R.T.: 4.422 min
Delta R.T.: 0.015 min
Response: 1919890
Conc: 1.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

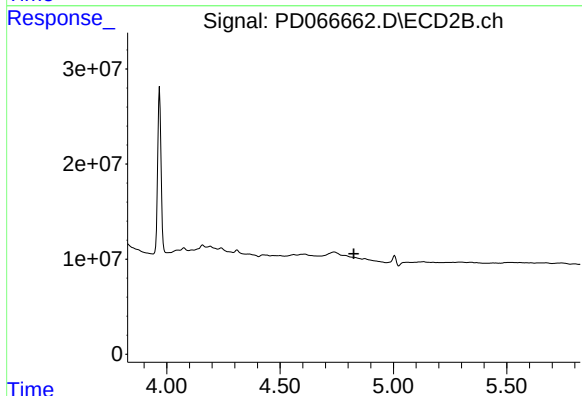


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.825 min
Response: 0
Conc: N.D.

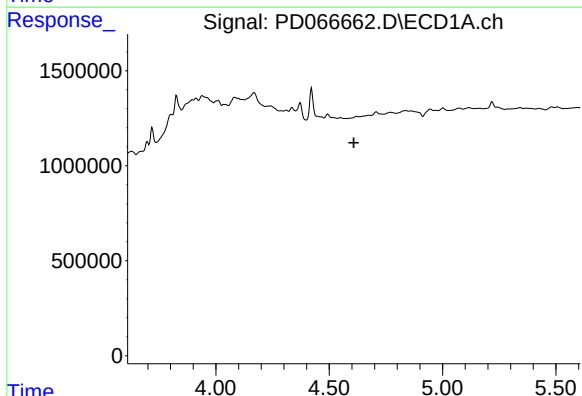


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

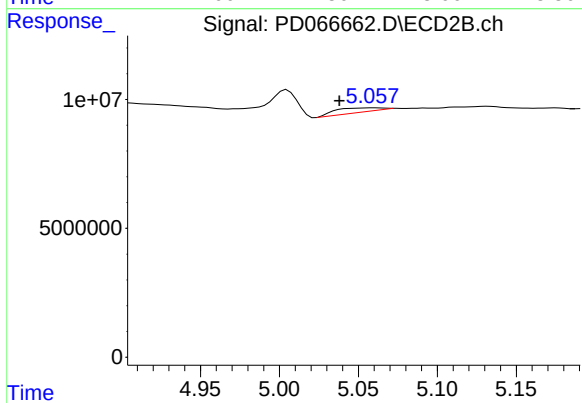

#7 delta-BHC


R.T.: 5.060 min
Delta R.T.: 0.022 min
Response: 3348223
Conc: 0.37 ng/ml

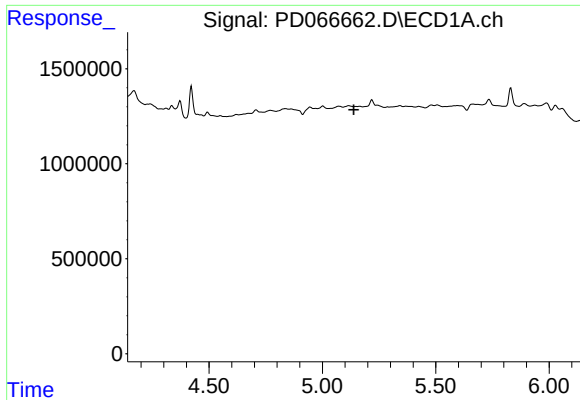

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

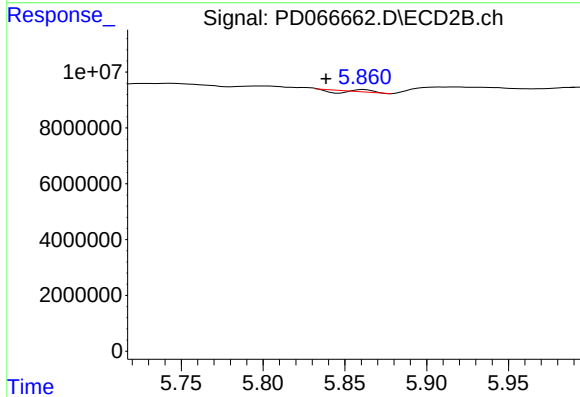


#8 Heptachlor epoxide

R.T.: 5.862 min
Delta R.T.: 0.023 min
Response: 232144
Conc: 0.03 ng/ml

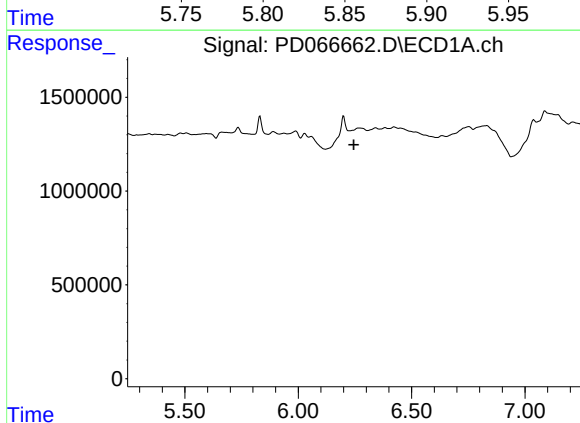


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

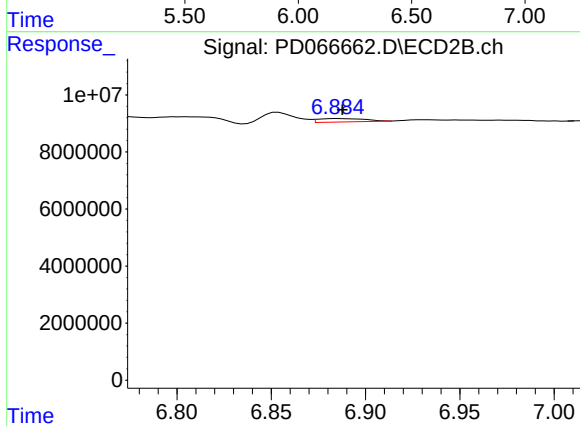

#15 Endosulfan II


R.T.: 6.885 min
Delta R.T.: -0.002 min
Response: 2062538
Conc: 0.29 ng/ml

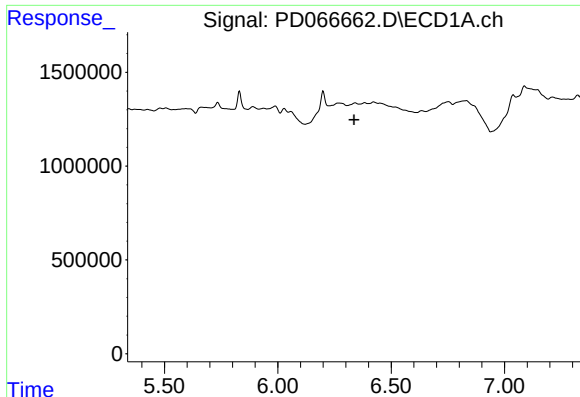

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

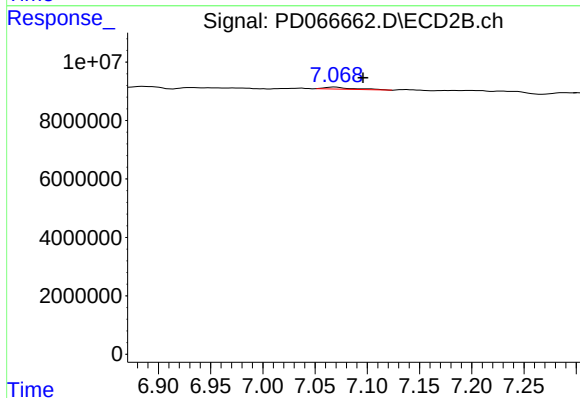


#17 4,4'-DDT

R.T.: 7.069 min
Delta R.T.: -0.027 min
Response: 1341566
Conc: 0.18 ng/ml

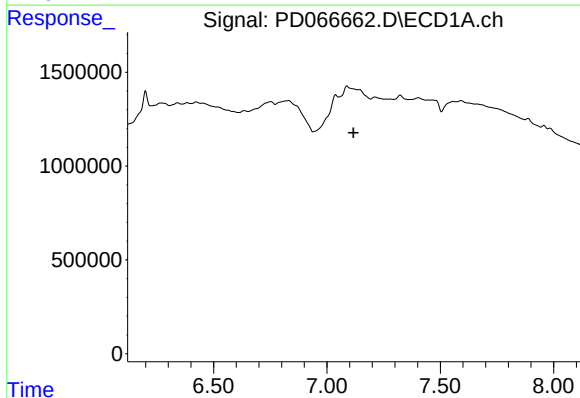


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.118 min
Response: 0
Conc: N.D.

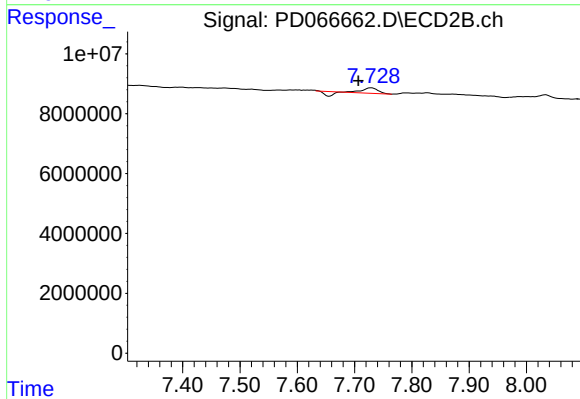

#21 Endrin ketone


R.T.: 7.729 min
Delta R.T.: 0.022 min
Response: 2021368
Conc: 0.24 ng/ml

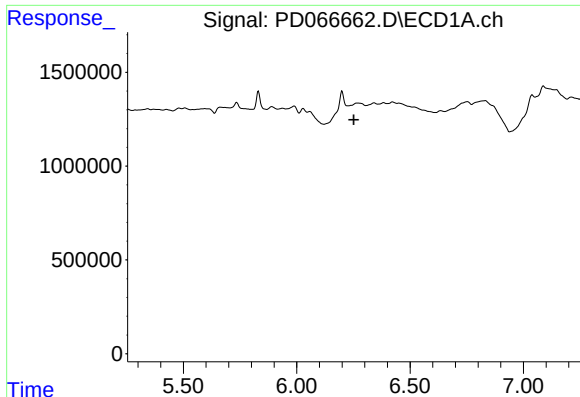

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.252 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

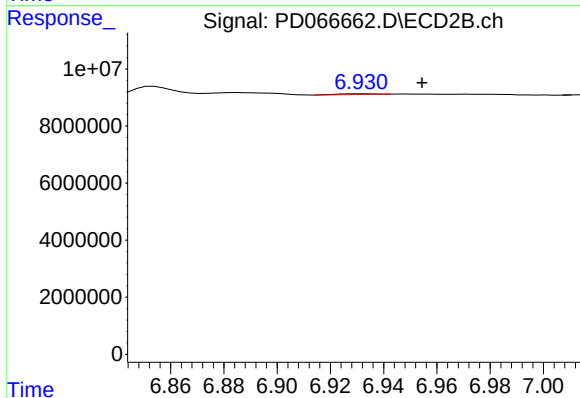


#27 Chlordane-5

R.T.: 6.932 min
Delta R.T.: -0.023 min
Response: 99022
Conc: 0.36 ng/ml

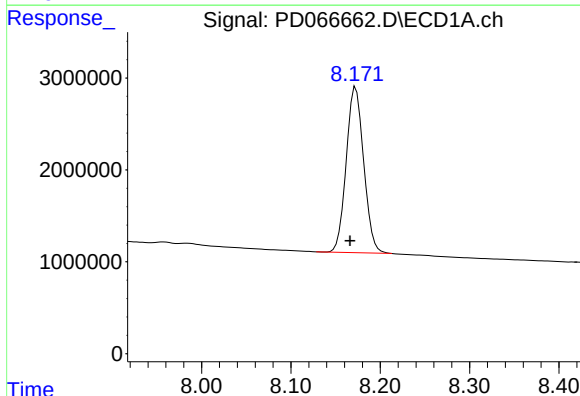

#28 Decachlorobiphenyl

R.T.: 8.173 min
Delta R.T.: 0.006 min
Response: 24467078
Conc: 21.18 ng/ml

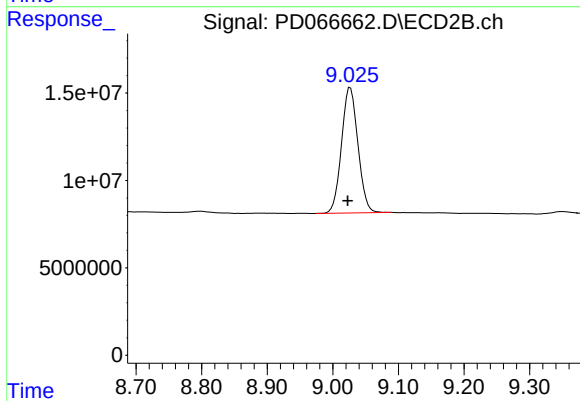

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: 0.004 min
Response: 124801237
Conc: 23.17 ng/ml