

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110121\
 Data File : PD066665.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2021 15:42
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

mohammad
 11/2/2021 1:48:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 06:08:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 03:24:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.445	3.968	87854739	374.5E6	48.540	47.846
7) SA Decachlor...	8.175	9.027	50464859	254.0E6	44.833	48.493
Target Compounds						
2) Toxaphene-1	5.684	6.354	8247814	21123425	502.513m	472.494
3) Toxaphene-2	5.846	7.054	8346600	34971064	452.277	502.407
4) Toxaphene-3	6.288	7.215	17845564	64875696	467.313	503.998
5) Toxaphene-4	6.531	7.355	18576458	36134899	475.699	489.946
6) Toxaphene-5	7.017	7.634	19401226	51044892	495.267	492.561

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110121\
Data File : PD066665.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2021 15:42
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 06:08:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 03:24:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

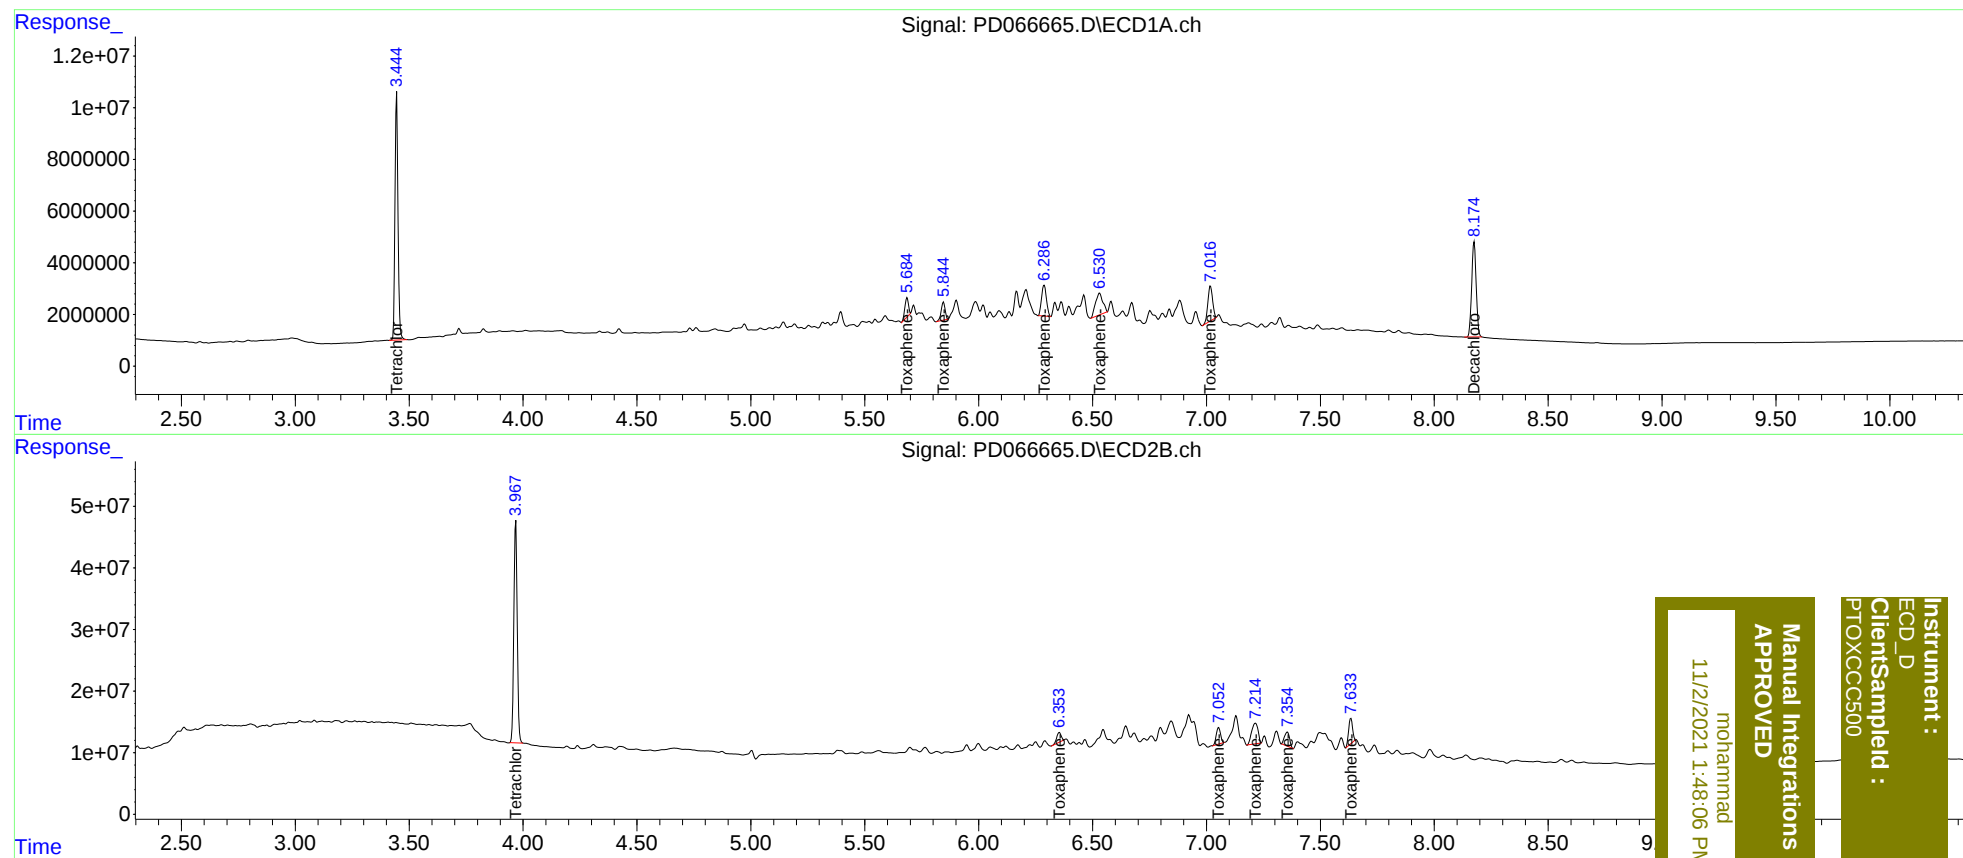

Manual Integrations
APPROVED

11/2/2021 1:48:06 PM
mohammad

Instrument :
ECD_D
ClientSampled :
PTOXCCC500