

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110422\
 Data File : PD072836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Nov 2022 01:26
 Operator : AR\AJ
 Sample : PIBLK395
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK462

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 11:26:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 16:50:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.701	3.462	49103740	896.8E6	21.121	22.379
27)	SA Decachlor...	7.831	8.912	79191560	414.8E6	40.344	44.113

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110422\
Data File : PD072836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Nov 2022 01:26
Operator : AR\AJ
Sample : PIBLK395
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 11:26:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102622CLP.M
Quant Title : GC Extractables
Qlast Update : Wed Oct 26 16:50:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


Response_

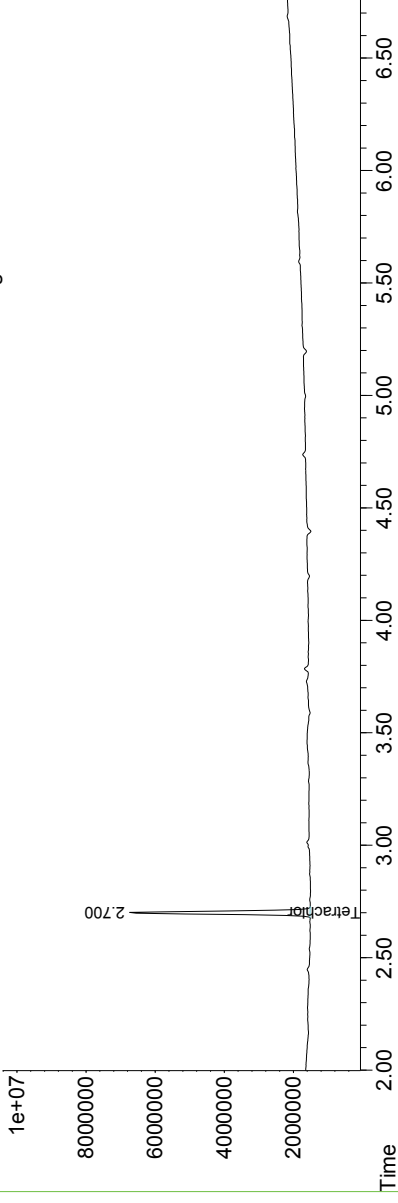

Signal: PD072836.D\ECD1A.ch

This chromatogram displays the detector response over time for signal PD072836.D\ECD1A.ch. The y-axis represents 'Response_' ranging from 0 to 1e+07. The x-axis represents 'Time' in minutes, ranging from 2.00 to 9.50. Two distinct peaks are labeled: one at 2.700 minutes and another at 7.830 minutes. The peak at 7.830 minutes is significantly larger than the one at 2.700 minutes.

Response_

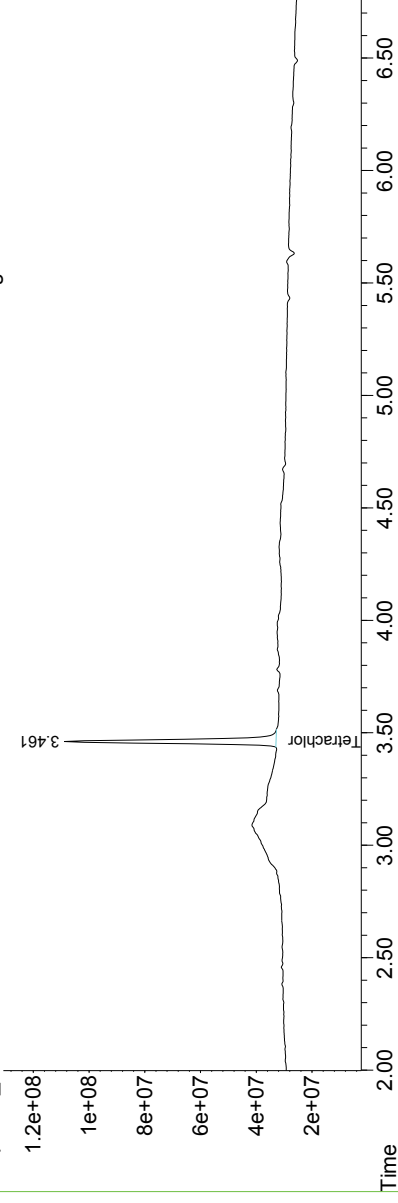

Signal: PD072836.D\ECD2B.ch

This chromatogram displays the detector response over time for signal PD072836.D\ECD2B.ch. The y-axis represents 'Response_' ranging from 0 to 1.2e+08. The x-axis represents 'Time' in minutes, ranging from 2.00 to 9.50. Two distinct peaks are labeled: one at 3.461 minutes and another at 8.911 minutes. The peak at 3.461 minutes is significantly larger than the one at 8.911 minutes.

Instrument :
ECD_D
ClientSampleId :
PIBLK462