

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110624\
 Data File : PD086396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 08:36
 Operator : AR\AJ
 Sample : P4622-12MSD
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6N6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/07/2024
 Supervised By :Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 22:08:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.887	24595970	176.2E6	18.682	18.995
27)	SA Decachlor...	9.092	8.095	32405722	177.1E6	18.076	18.732
Target Compounds							
2)	A alpha-BHC	4.009	3.401	151.1E6	766.3E6	60.693m	53.335
3)	MA gamma-BHC...	4.340	3.738	146.6E6	713.2E6	58.933m	52.874
4)	MA Heptachlor	4.943	4.093	142.6E6	708.3E6	57.676	51.845m
5)	MB Aldrin	5.286	4.381	139.1E6	697.0E6	57.378	51.379
6)	B beta-BHC	4.526	4.032	56141378	302.0E6	50.552	48.167m
7)	B delta-BHC	4.775	4.271	150.0E6	719.3E6	57.937	51.266
8)	B Heptachlo...	5.705	4.885	121.6E6	621.1E6	53.224	49.532m
9)	A Endosulfan I	6.088	5.261	111.0E6	574.0E6	54.781	49.997
10)	B trans-Chl...	5.960	5.139	117.3E6	658.2E6	53.153	50.035m
11)	B cis-Chlor...	6.041	5.205	120.8E6	629.2E6	54.613	49.538
12)	B 4,4'-DDE	6.210	5.391	238.9E6	1215.6E6	111.846	99.139
13)	MA Dieldrin	6.362	5.526	265.7E6	1255.5E6	116.498	101.761m
14)	MA Endrin	6.588	5.804	220.8E6	1137.2E6	117.459	101.191
15)	B Endosulfa...	6.799	6.095	215.8E6	1057.5E6	107.655	95.853
16)	A 4,4'-DDD	6.718	5.945	191.0E6	991.2E6	117.841	100.980
17)	MA 4,4'-DDT	7.033	6.199	194.1E6	1036.3E6	116.408m	100.982m
18)	B Endrin al...	6.928	6.274	145.0E6	720.5E6	97.207	86.800
19)	B Endosulfa...	7.162	6.499	201.9E6	1016.6E6	109.521	96.440
20)	A Methoxychlor	7.506	6.773	507.8E6	2130.2E6	539.608	448.143
21)	B Endrin ke...	7.643	7.007	225.0E6	1063.2E6	109.163	92.912

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110624\
Data File : PD086396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 08:36
Operator : AR\AJ
Sample : P4622-12MSD
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 22:08:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

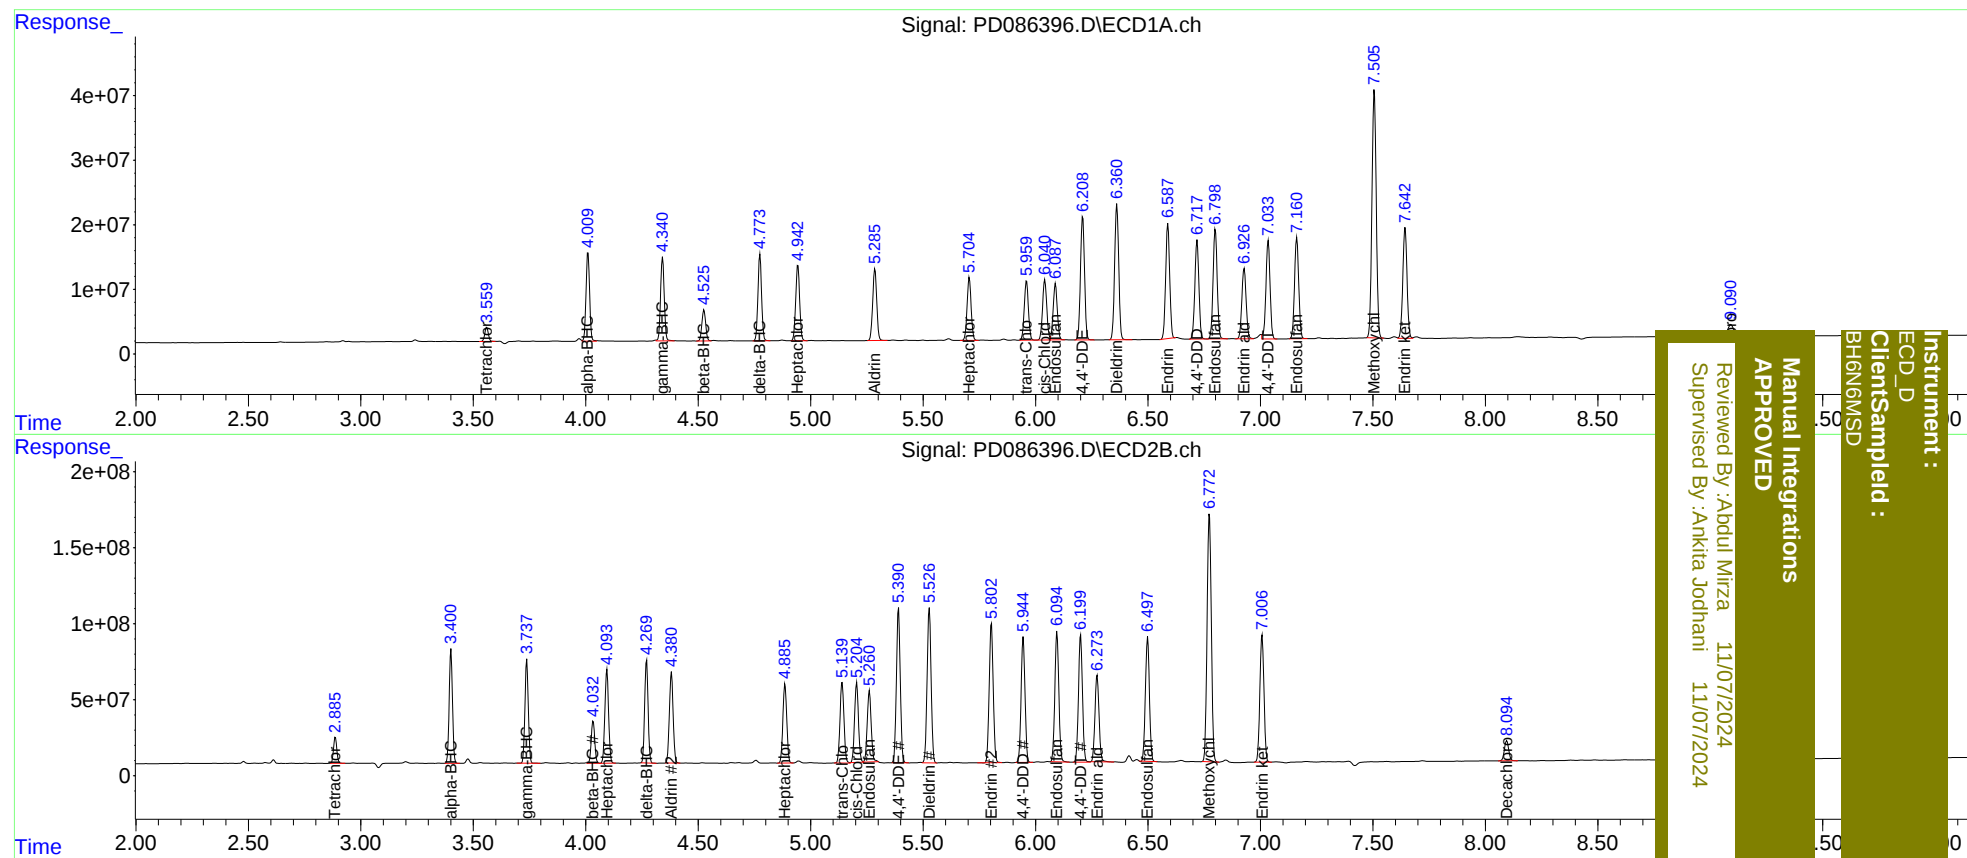

Instrument :
ECD_D
Client Sampled :
BH6N6MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 11/07/2024
Supervised By: Ankita Jodhani 11/07/2024