

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110624\
 Data File : PD086395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Nov 2024 08:21
 Operator : AR\AJ
 Sample : P4622-11MS
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH6N6MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/07/2024
 Supervised By : Ankita Jodhani 11/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 22:08:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 25 14:36:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.887	24696115	173.4E6	18.758	18.697
2)	SA Decachlor...	9.091	8.094	32805721	178.7E6	18.299	18.899
Target Compounds							
2)	A alpha-BHC	4.009	3.402	150.5E6	764.3E6	60.449m	53.195
3)	MA gamma-BHC...	4.342	3.739	144.0E6	709.7E6	57.872	52.621
4)	MA Heptachlor	4.943	4.093	142.5E6	710.3E6	57.628	51.992m
5)	MB Aldrin	5.285	4.382	140.2E6	698.8E6	57.858	51.509
6)	B beta-BHC	4.525	4.034	56150906	294.5E6	50.561	46.964
7)	B delta-BHC	4.774	4.270	150.3E6	724.2E6	58.073	51.614m
8)	B Heptachlo...	5.705	4.886	124.0E6	619.0E6	54.268	49.363
9)	A Endosulfan I	6.088	5.261	114.7E6	575.7E6	56.641	50.140
10)	B trans-Chl...	5.960	5.139	121.9E6	659.2E6	55.248	50.111m
11)	B cis-Chlor...	6.041	5.205	124.8E6	630.3E6	56.429	49.628
12)	B 4,4'-DDE	6.209	5.391	240.2E6	1199.7E6	112.469	97.844
13)	MA Dieldrin	6.361	5.528	267.3E6	1248.5E6	117.177	101.194
14)	MA Endrin	6.587	5.803	229.0E6	1134.2E6	121.805m	100.928m
15)	B Endosulfa...	6.799	6.096	216.3E6	1067.9E6	107.891	96.792
16)	A 4,4'-DDD	6.718	5.945	190.4E6	981.9E6	117.505	100.030
17)	MA 4,4'-DDT	7.032	6.199	194.1E6	1049.4E6	116.399m	102.262m
18)	B Endrin al...	6.928	6.274	147.0E6	727.7E6	98.561	87.669
19)	B Endosulfa...	7.162	6.498	197.0E6	1046.6E6	106.893	99.284
20)	A Methoxychlor	7.505	6.773	511.7E6	2210.8E6	543.670	465.112
21)	B Endrin ke...	7.642	7.007	226.8E6	1091.5E6	110.064	95.390

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110624\
Data File : PD086395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Nov 2024 08:21
Operator : AR\AJ
Sample : P4622-11MS
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 22:08:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102524CLP.M
Quant Title : GC Extractables
QLast Update : Fri Oct 25 14:36:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

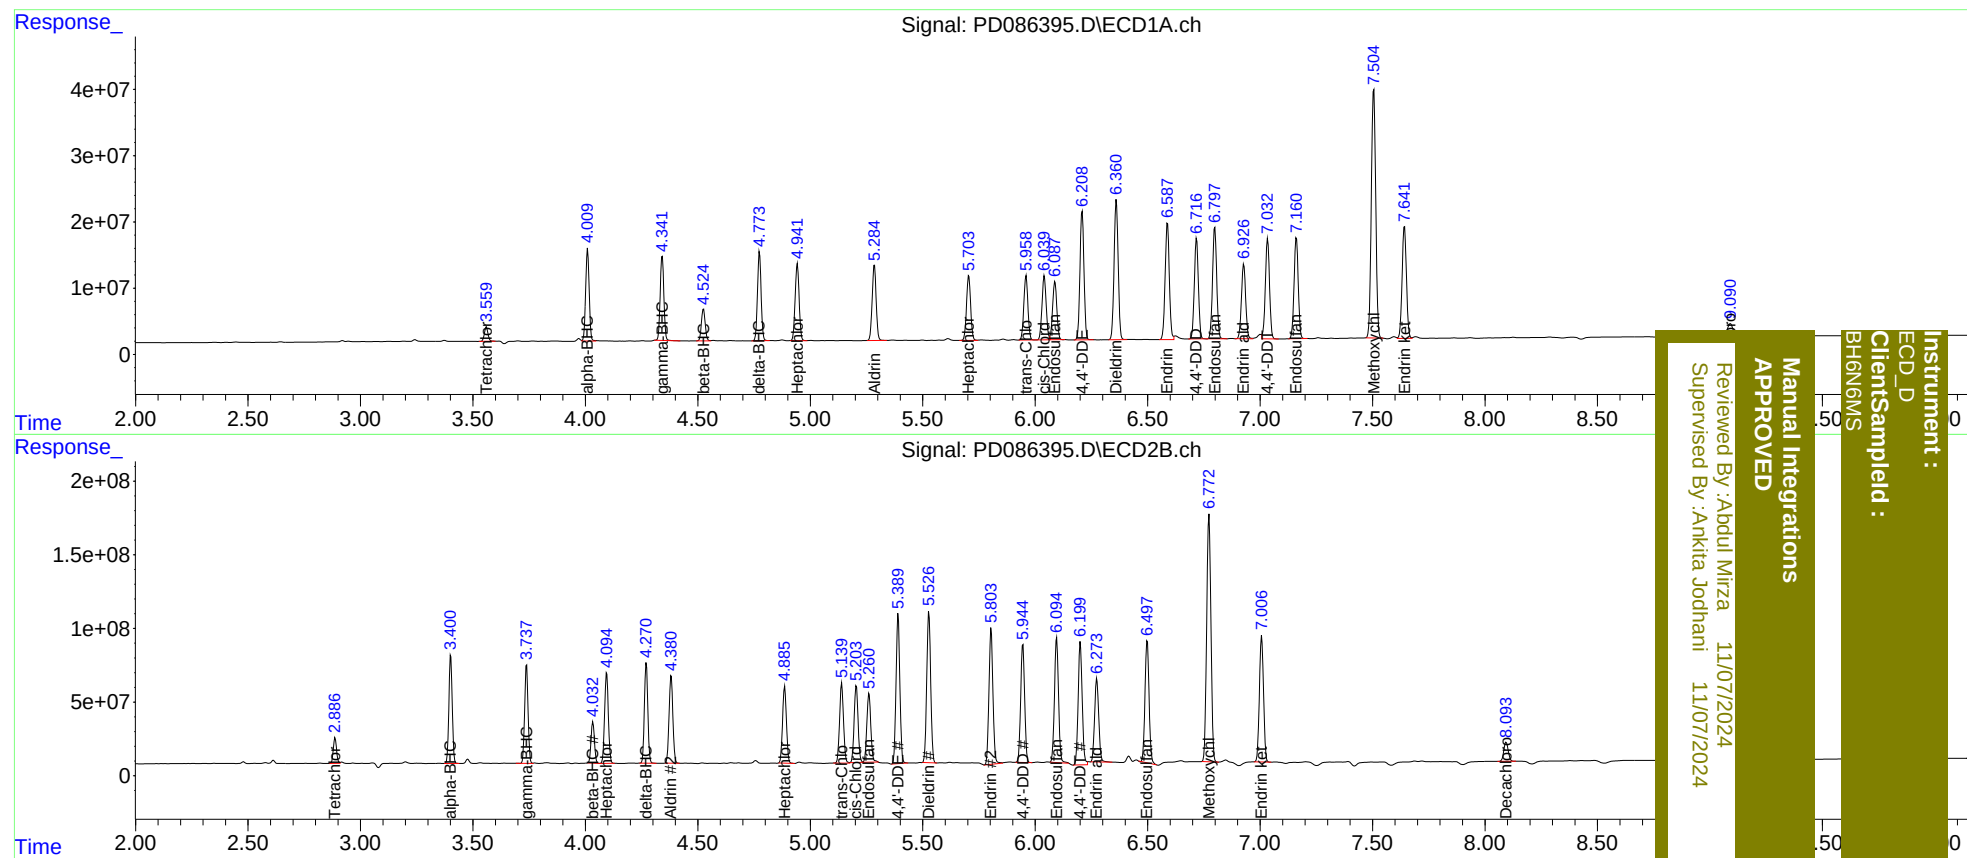

Instrument :
ECD_D
ClientSampled :
BH6N6MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 11/07/2024
Supervised By: Ankita Jodhani 11/07/2024