

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110918\
 Data File : PD050279.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2018 13:27
 Operator : AJ\SJ
 Sample : J5840-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 23:17:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 06 03:52:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.234	4.060	13912586	614.6E6	21.495	21.375
27)	SA Decachlor...	9.017	9.168	23542366	657.8E6	35.236	34.363
Target Compounds							
2)	A alpha-BHC	4.672	0.000	313287	0	0.341	N.D. #
3)	MA gamma-BHC...	4.977	4.742	3064588	890294	3.434	<MDL #
4)	MA Heptachlor	0.000	5.266	0	1546216	N.D.	<MDL
6)	B beta-BHC	0.000	4.954f	0	94762948	N.D.	5.279
7)	B delta-BHC	0.000	5.175f	0	5750114	N.D.	0.151
8)	B Heptachlo...	0.000	5.938	0	2198224	N.D.	<MDL
9)	A Endosulfan I	6.276f	0.000	1353236	0	1.802	N.D. #
10)	B trans-Chl...	6.276f	6.193	1353236	-9435976	1.664	N.D. #
11)	B cis-Chlor...	6.276	6.193f	1353236	-9435976	1.747	N.D. #
13)	MA Dieldrin	0.000	6.564	0	6767042	N.D.	0.219
15)	B Endosulfa...	0.000	6.991	0	8613041	N.D.	0.355


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110918\
Data File : PD050279.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2018 13:27
Operator : AJ\SJ
Sample : J5840-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 23:17:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 06 03:52:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

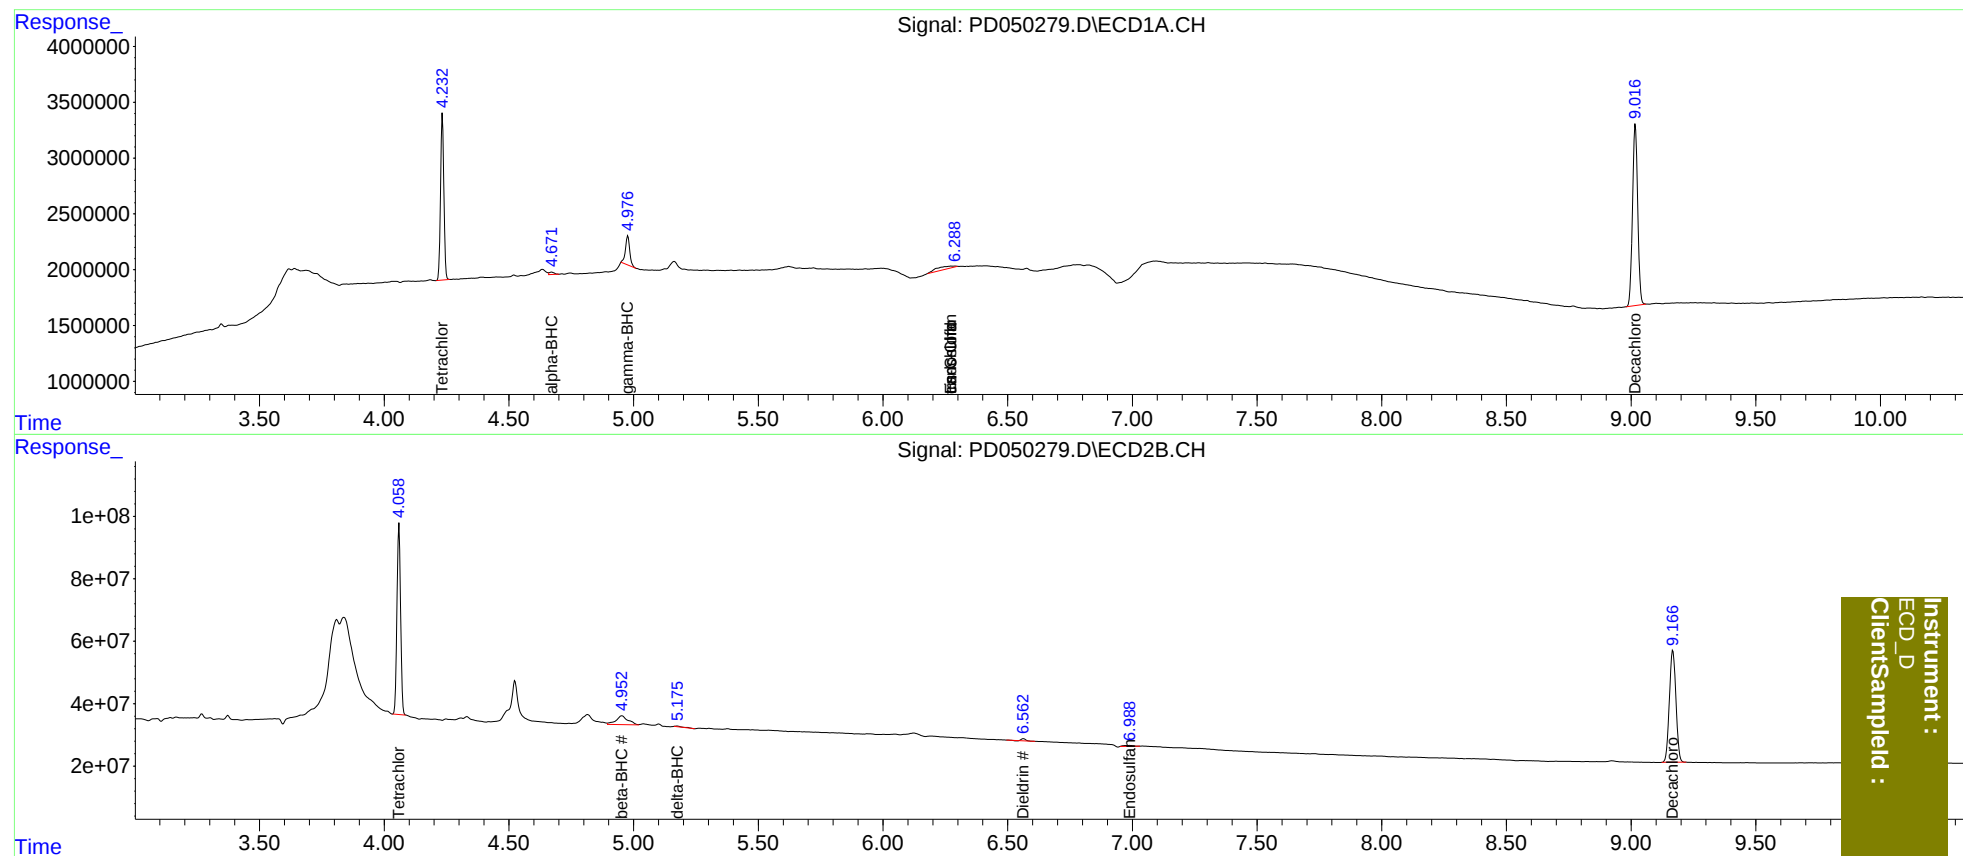


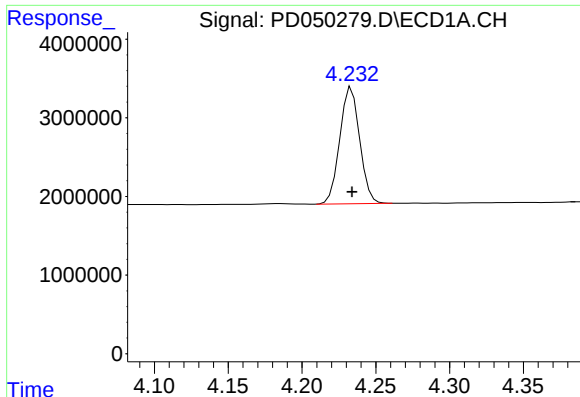

#1 Tetrachloro-m-xylene


R.T.: 4.234 min
Delta R.T.: 0.000 min
Response: 13912586
Conc: 21.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

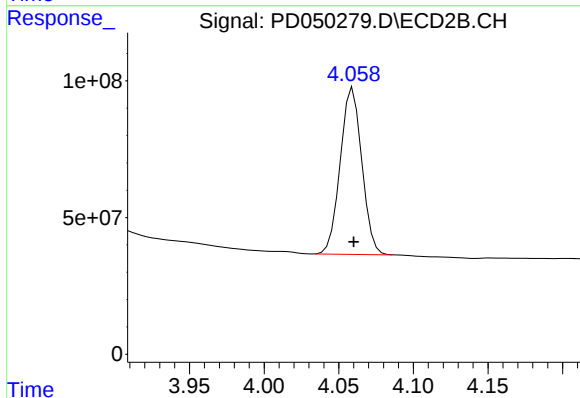


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.000 min
Response: 614598665
Conc: 21.38 ng/ml

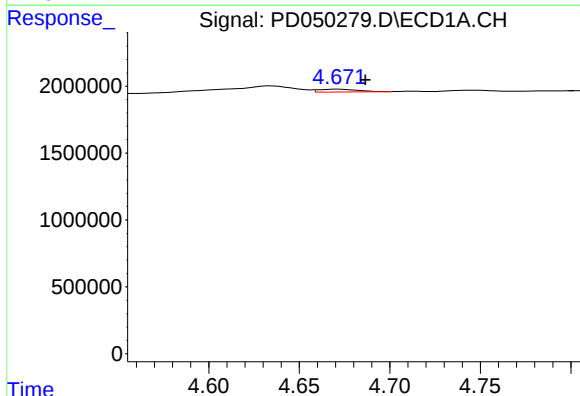


#2 alpha-BHC

R.T.: 4.672 min
Delta R.T.: -0.015 min
Response: 313287
Conc: 0.34 ng/ml

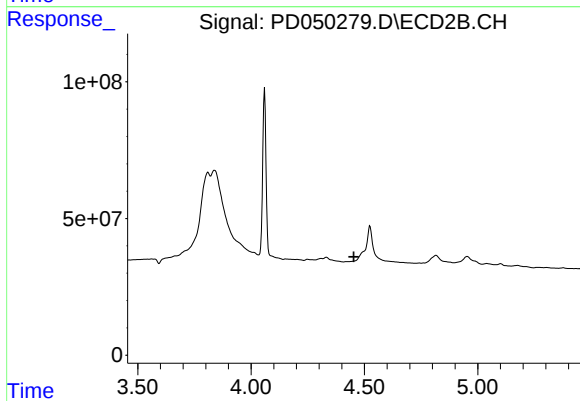

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.453 min
Response: 0
Conc: N.D.

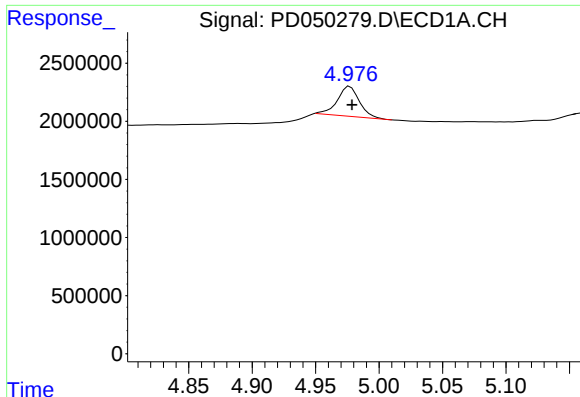

#3 gamma-BHC (Lindane)


R.T.: 4.977 min
Delta R.T.: -0.002 min
Response: 3064588
Conc: 3.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

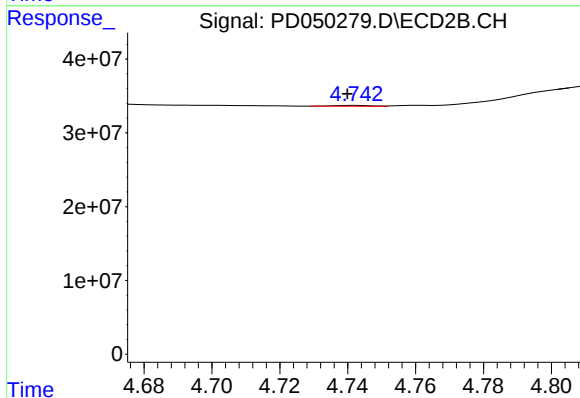


#3 gamma-BHC (Lindane)

R.T.: 4.742 min
Delta R.T.: 0.003 min
Response: 890294
Conc: N.D.

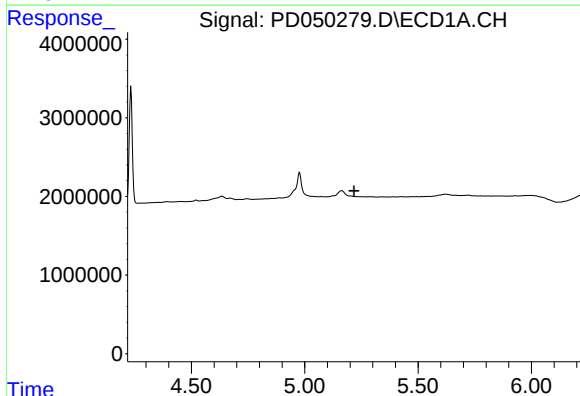


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 5.218 min
Response: 0
Conc: N.D.

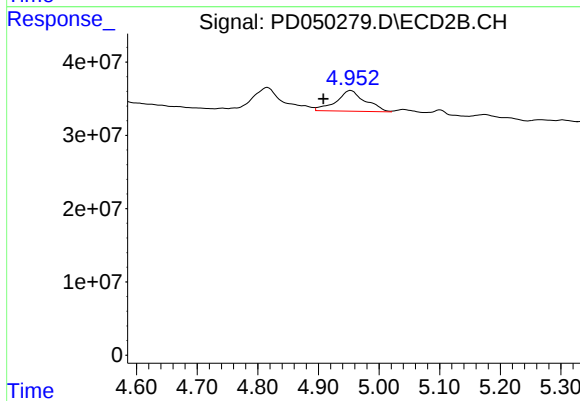

#6 beta-BHC


R.T.: 4.954 min
Delta R.T.: 0.045 min
Response: 94762948
Conc: 5.28 ng/ml

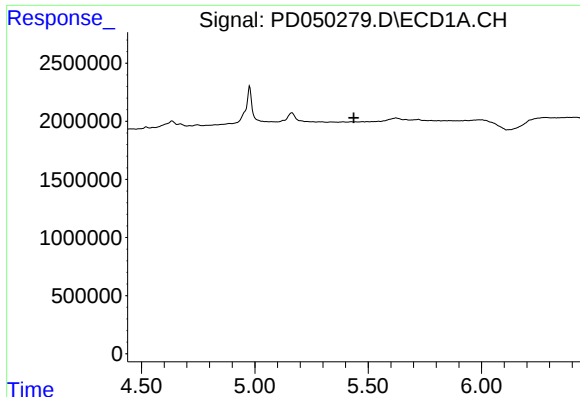

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 5.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

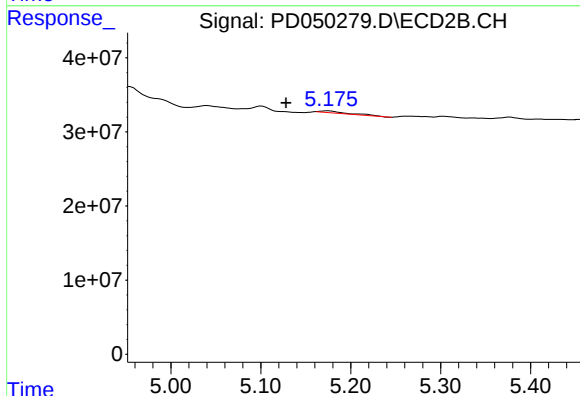


#7 delta-BHC

R.T.: 5.175 min
Delta R.T.: 0.047 min
Response: 5750114
Conc: 0.15 ng/ml

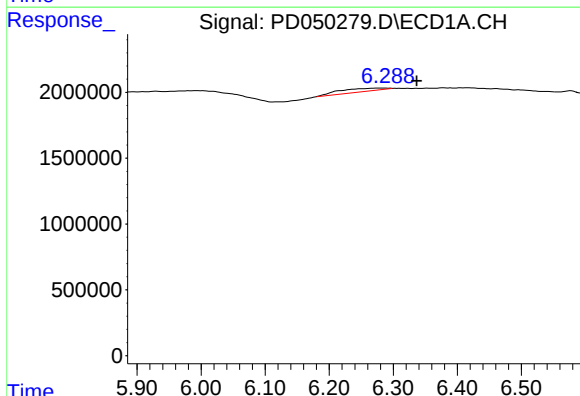


#9 Endosulfan I

R.T.: 6.276 min
Delta R.T.: -0.060 min
Response: 1353236
Conc: 1.80 ng/ml

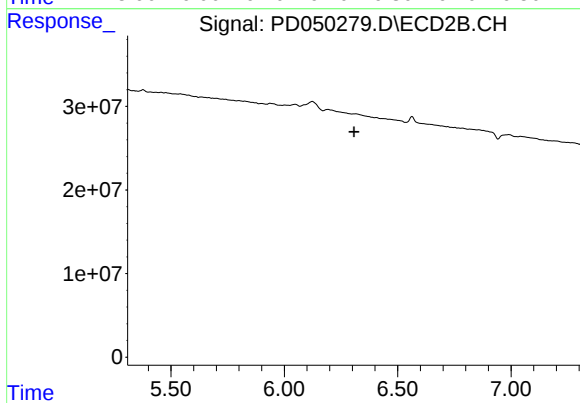

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.308 min
Response: 0
Conc: N.D.

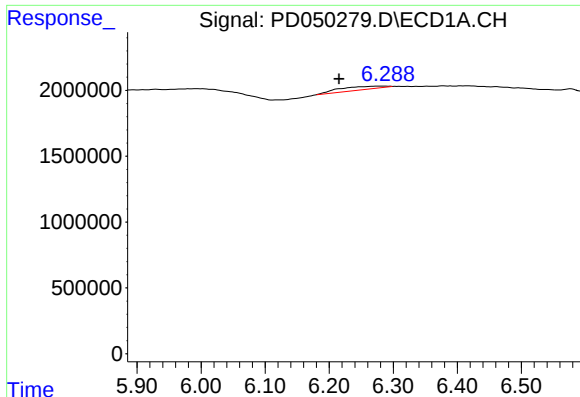

#10 trans-Chlordane


R.T.: 6.276 min
Delta R.T.: 0.061 min
Response: 1353236
Conc: 1.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

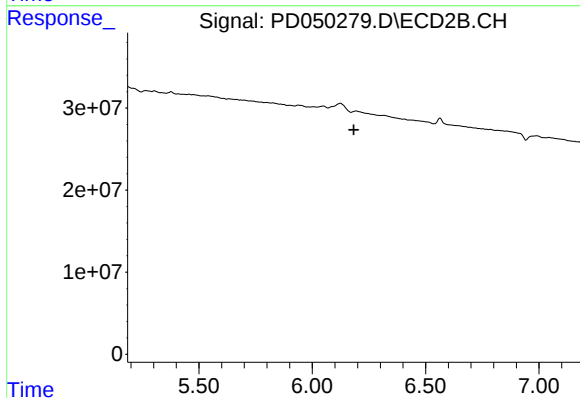


#10 trans-Chlordane

R.T.: 6.193 min
Delta R.T.: 0.011 min
Response: -9435976
Conc: N.D.

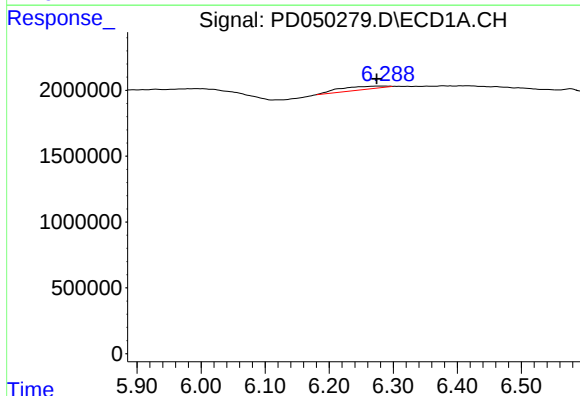


#11 cis-Chlordane

R.T.: 6.276 min
Delta R.T.: 0.002 min
Response: 1353236
Conc: 1.75 ng/ml

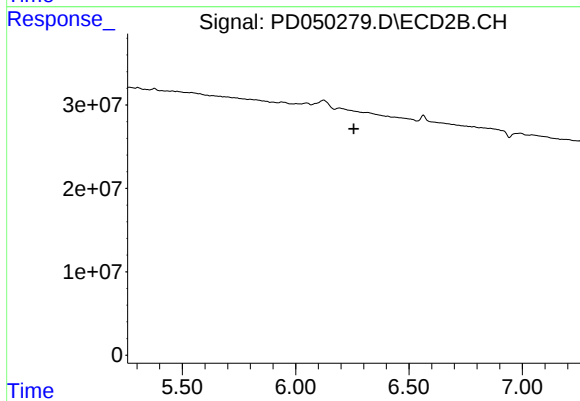

#11 cis-Chlordane


R.T.: 6.193 min
Delta R.T.: -0.063 min
Response: -9435976
Conc: N.D.

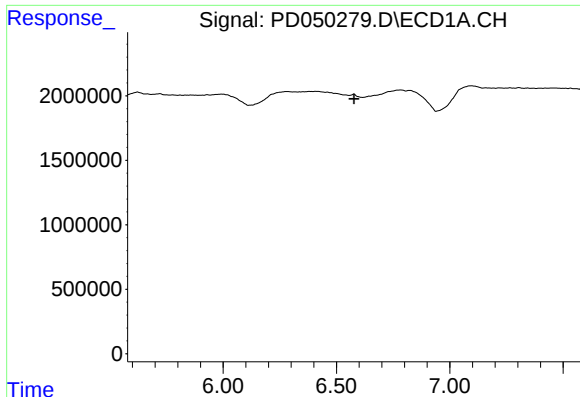

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.578 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

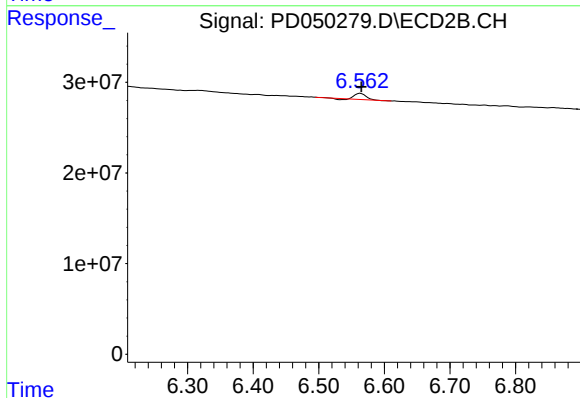


#13 Dieldrin

R.T.: 6.564 min
Delta R.T.: -0.002 min
Response: 6767042
Conc: 0.22 ng/ml

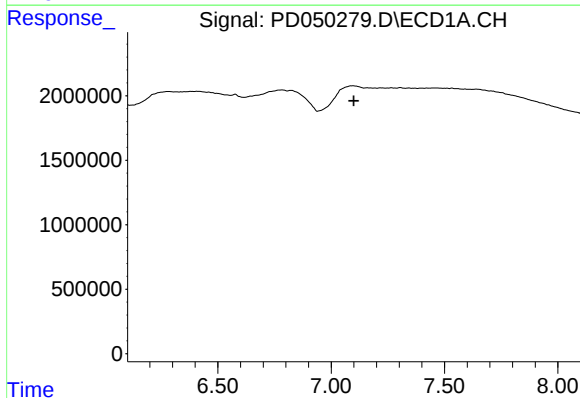


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 7.100 min
Response: 0
Conc: N.D.

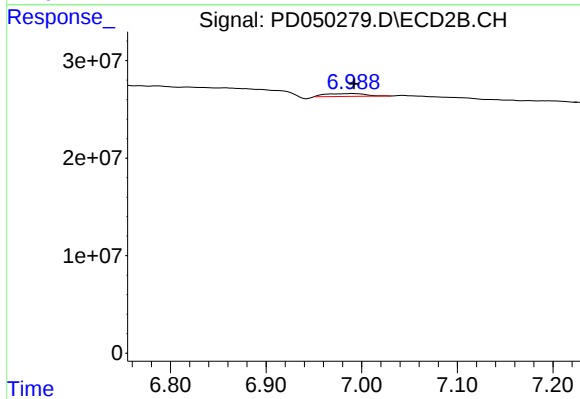

#15 Endosulfan II


R.T.: 6.991 min
Delta R.T.: -0.001 min
Response: 8613041
Conc: 0.35 ng/ml

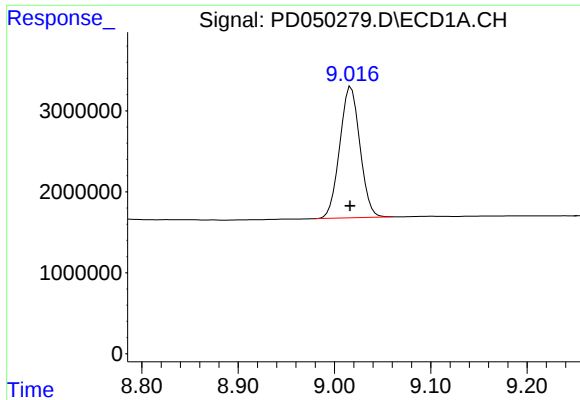

#27 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.001 min
Response: 23542366
Conc: 35.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

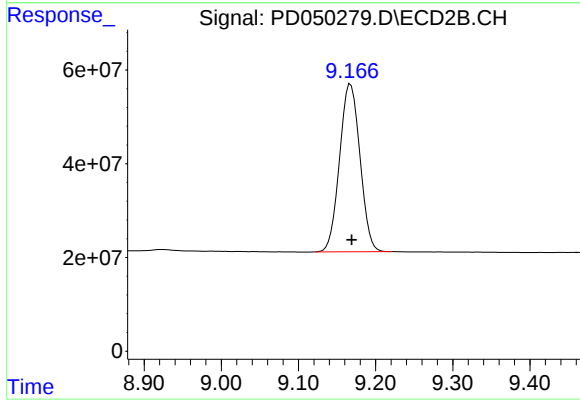

#27 Decachlorobiphenyl

R.T.: 9.168 min
Delta R.T.: -0.001 min
Response: 657760099
Conc: 34.36 ng/ml