

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110918\
 Data File : PD050280.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2018 13:41
 Operator : AJ\SJ
 Sample : J5840-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 23:17:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 06 03:52:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	4.060	13809635	498.3E6	21.336	17.330
27)	SA Decachlor...	9.017	9.169	14972809	429.9E6	22.410	22.457
Target Compounds							
2)	A alpha-BHC	4.673	0.000	300286	0	0.326	N.D. #
3)	MA gamma-BHC...	4.973	0.000	1041720	0	1.167	N.D. #
6)	B beta-BHC	0.000	4.953f	0	87036500	N.D.	4.849
8)	B Heptachlo...	6.008	5.976	236825	7924933	0.313	0.247
9)	A Endosulfan I	0.000	6.251f	0	2596149	N.D.	<MDL
10)	B trans-Chl...	6.266f	6.197	1452407	-9040653	1.786	N.D. #
11)	B cis-Chlor...	6.266	6.251	1452407	2596149	1.875	<MDL #
20)	A Methoxychlor	0.000	7.595f	0	1810779	N.D.	0.181

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110918\
Data File : PD050280.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2018 13:41
Operator : AJ\SJ
Sample : J5840-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 23:17:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 06 03:52:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

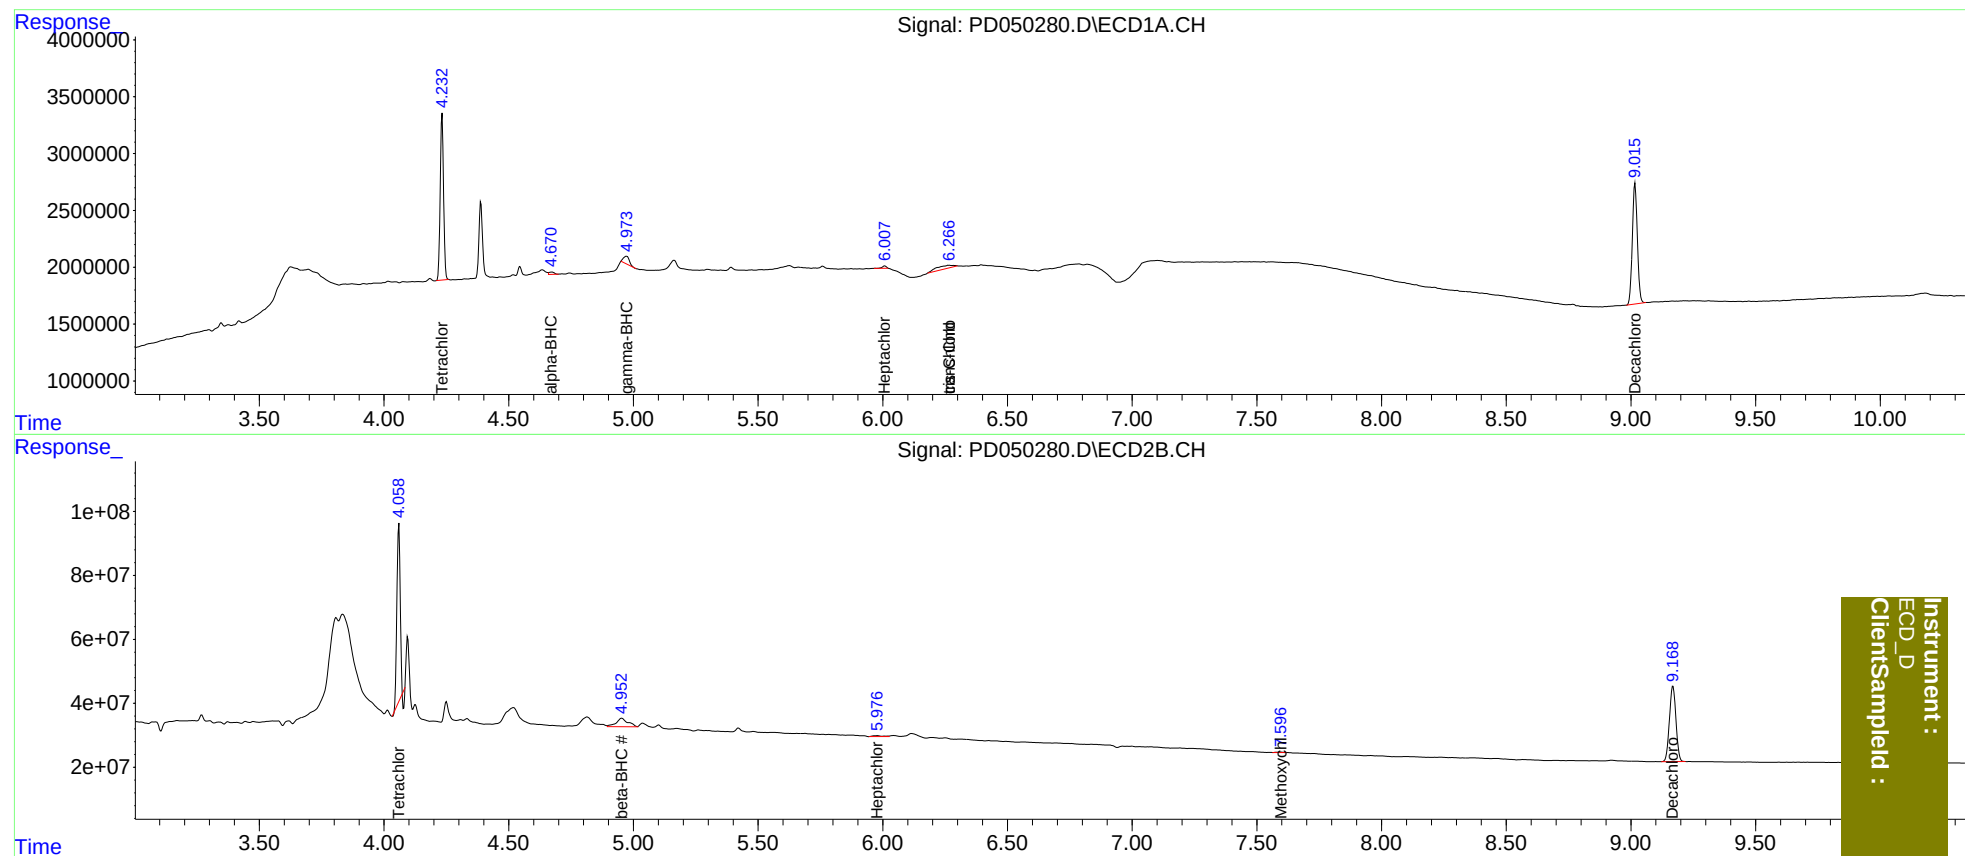


Instrument :
ECD_D
ClientSampled :

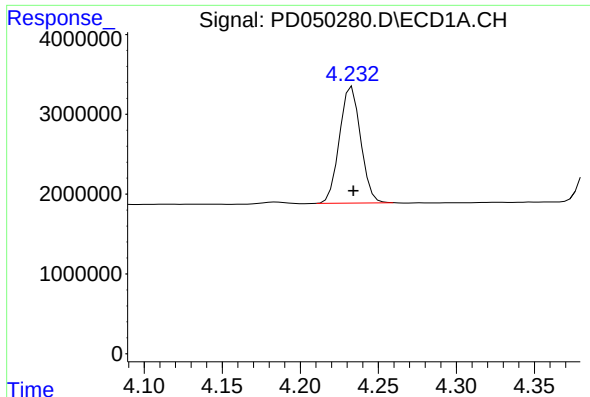

#1 Tetrachloro-m-xylene


R.T.: 4.233 min
Delta R.T.: 0.000 min
Response: 13809635
Conc: 21.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

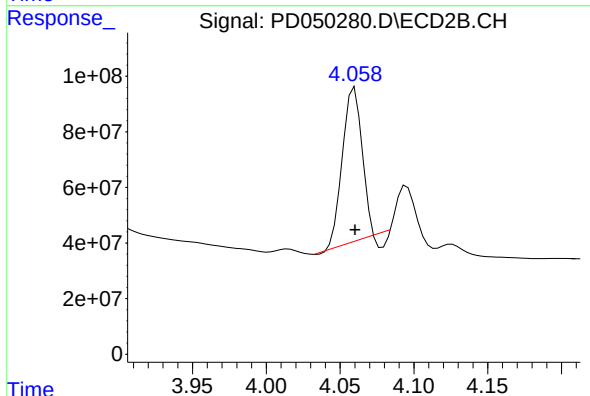


#1 Tetrachloro-m-xylene

R.T.: 4.060 min
Delta R.T.: 0.000 min
Response: 498284281
Conc: 17.33 ng/ml

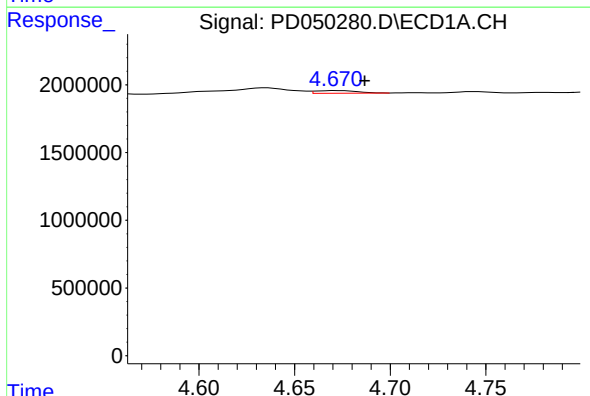


#2 alpha-BHC

R.T.: 4.673 min
Delta R.T.: -0.014 min
Response: 300286
Conc: 0.33 ng/ml

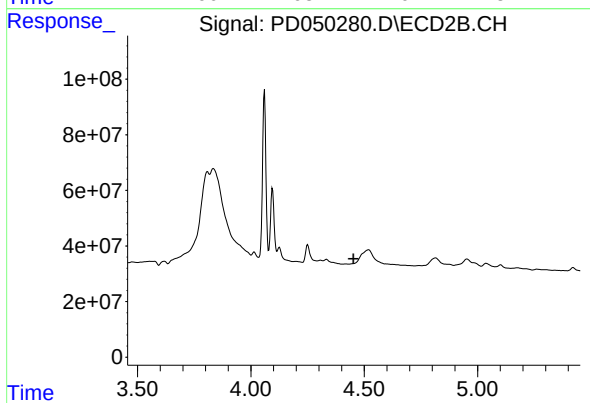

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.453 min
Response: 0
Conc: N.D.

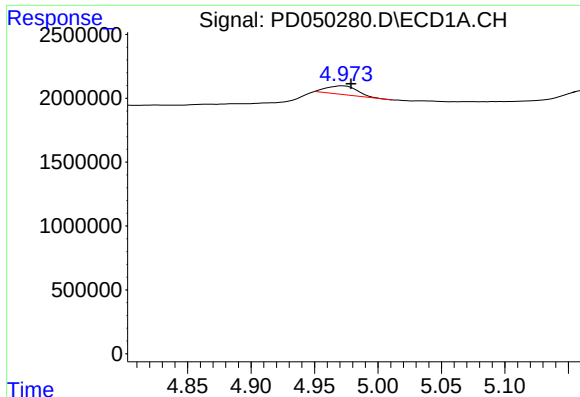

#3 gamma-BHC (Lindane)


R.T.: 4.973 min
Delta R.T.: -0.006 min
Response: 1041720
Conc: 1.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

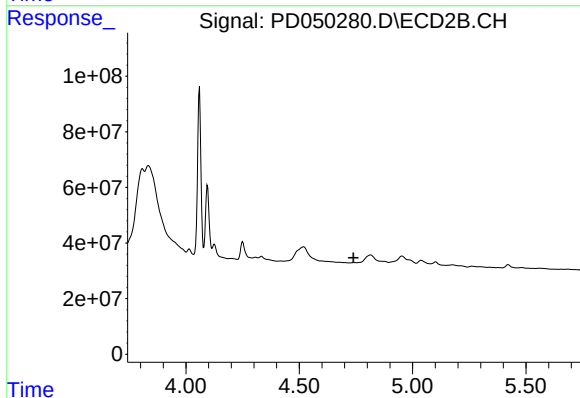


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.740 min
Response: 0
Conc: N.D.

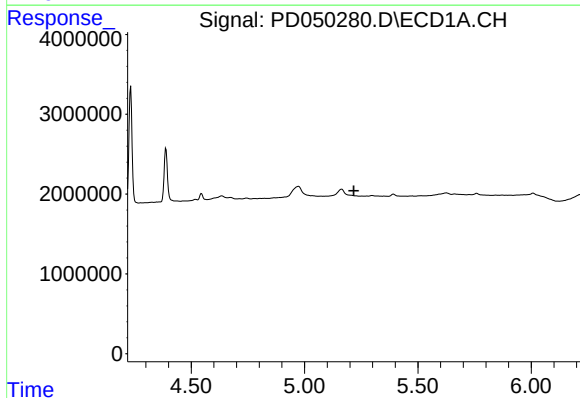


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 5.218 min
Response: 0
Conc: N.D.

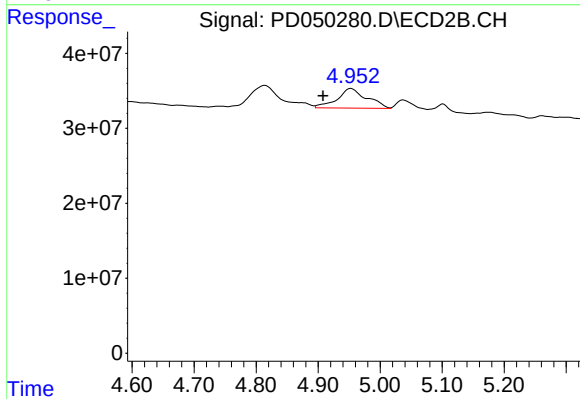

#6 beta-BHC


R.T.: 4.953 min
Delta R.T.: 0.045 min
Response: 87036500
Conc: 4.85 ng/ml

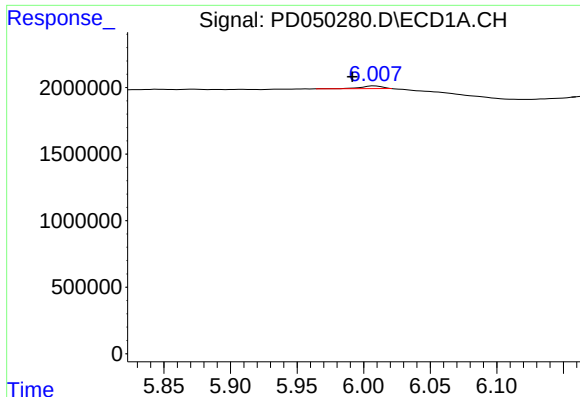

#8 Heptachlor epoxide


R.T.: 6.008 min
Delta R.T.: 0.017 min
Response: 236825
Conc: 0.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

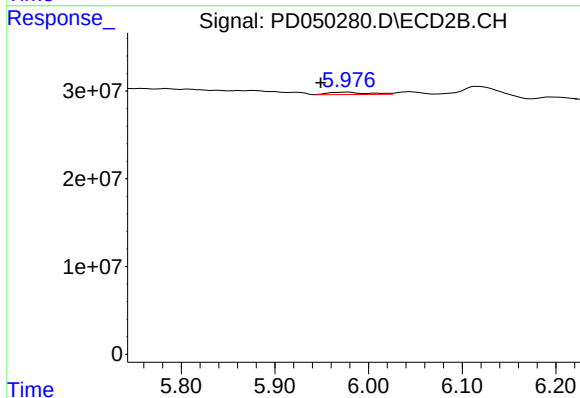


#8 Heptachlor epoxide

R.T.: 5.976 min
Delta R.T.: 0.027 min
Response: 7924933
Conc: 0.25 ng/ml

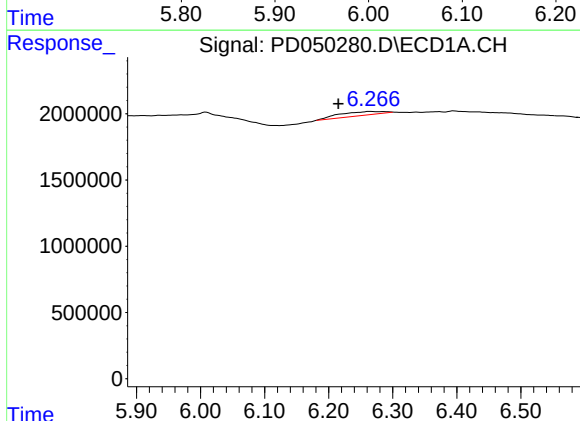


#10 trans-Chlordane

R.T.: 6.266 min
Delta R.T.: 0.051 min
Response: 1452407
Conc: 1.79 ng/ml

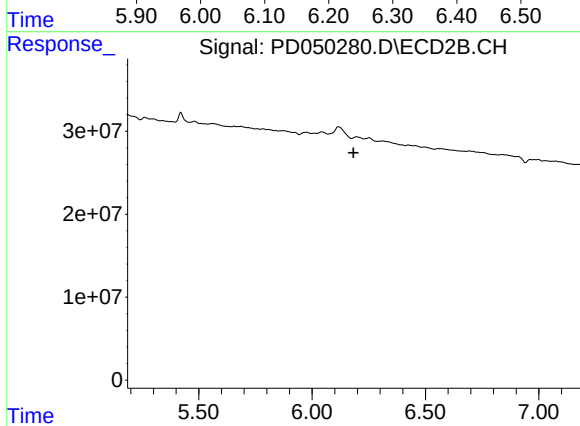

#10 trans-Chlordane


R.T.: 6.197 min
Delta R.T.: 0.014 min
Response: -9040653
Conc: N.D.

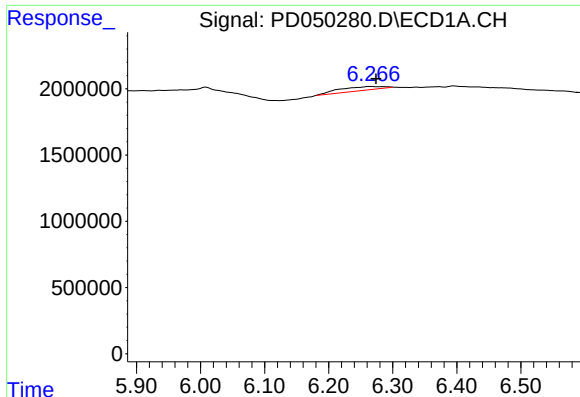

#11 cis-Chlordane


R.T.: 6.266 min
Delta R.T.: -0.008 min
Response: 1452407
Conc: 1.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

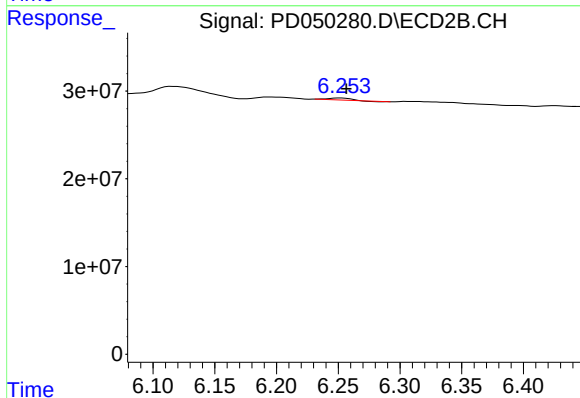


#11 cis-Chlordane

R.T.: 6.251 min
Delta R.T.: -0.005 min
Response: 2596149
Conc: N.D.

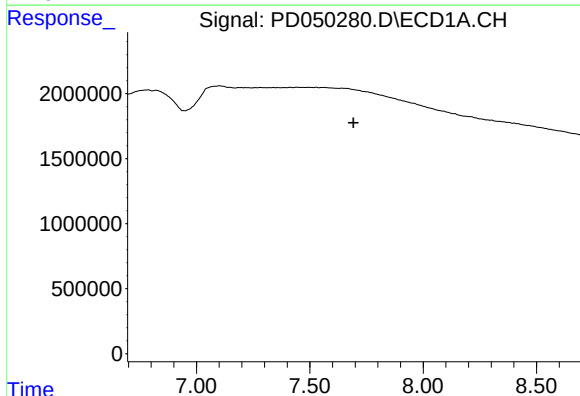


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.693 min
Response: 0
Conc: N.D.

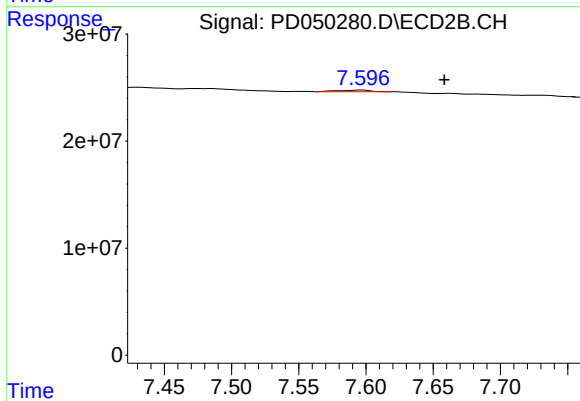

#20 Methoxychlor


R.T.: 7.595 min
Delta R.T.: -0.063 min
Response: 1810779
Conc: 0.18 ng/ml

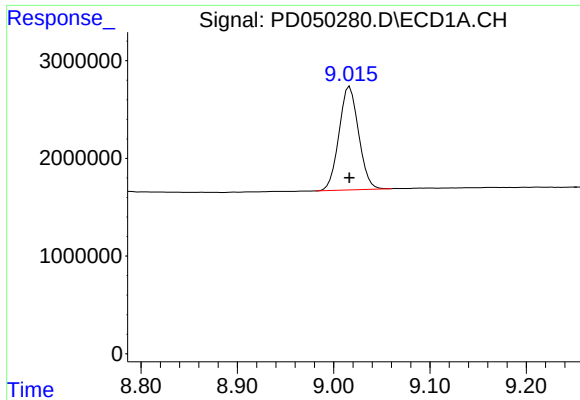

#27 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.000 min
Response: 14972809
Conc: 22.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

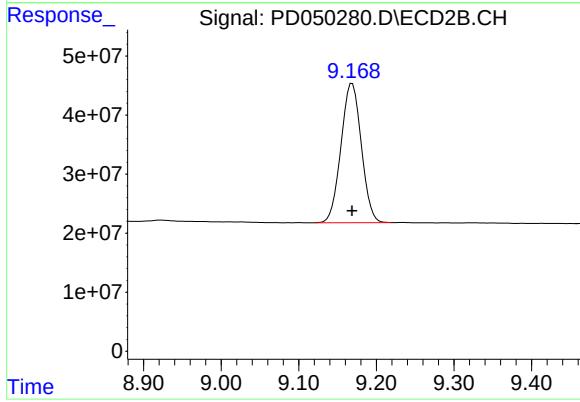

#27 Decachlorobiphenyl

R.T.: 9.169 min
Delta R.T.: 0.000 min
Response: 429866906
Conc: 22.46 ng/ml