

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110918\
 Data File : PD050290.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2018 16:01
 Operator : AJ\SJ
 Sample : J5840-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AG7

Manual Integrations
 APPROVED

Sohil
 11/13/2018 12:08:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 23:18:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 06 03:52:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	4.233	4.060	14141657	598.5E6	21.849	20.814
2) SA Decachlor...	9.017	9.170	25540723	689.2E6	38.227	36.006
Target Compounds						
8) B Heptachlo...	5.991	5.948	371361	17422607	0.491	0.542
13) MA Dieldrin	6.577	6.564	8082816	334.7E6	9.580	10.810m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD110918\
Data File : PD050290.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2018 16:01
Operator : AJ\SJ
Sample : J5840-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 23:18:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110618CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 06 03:52:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

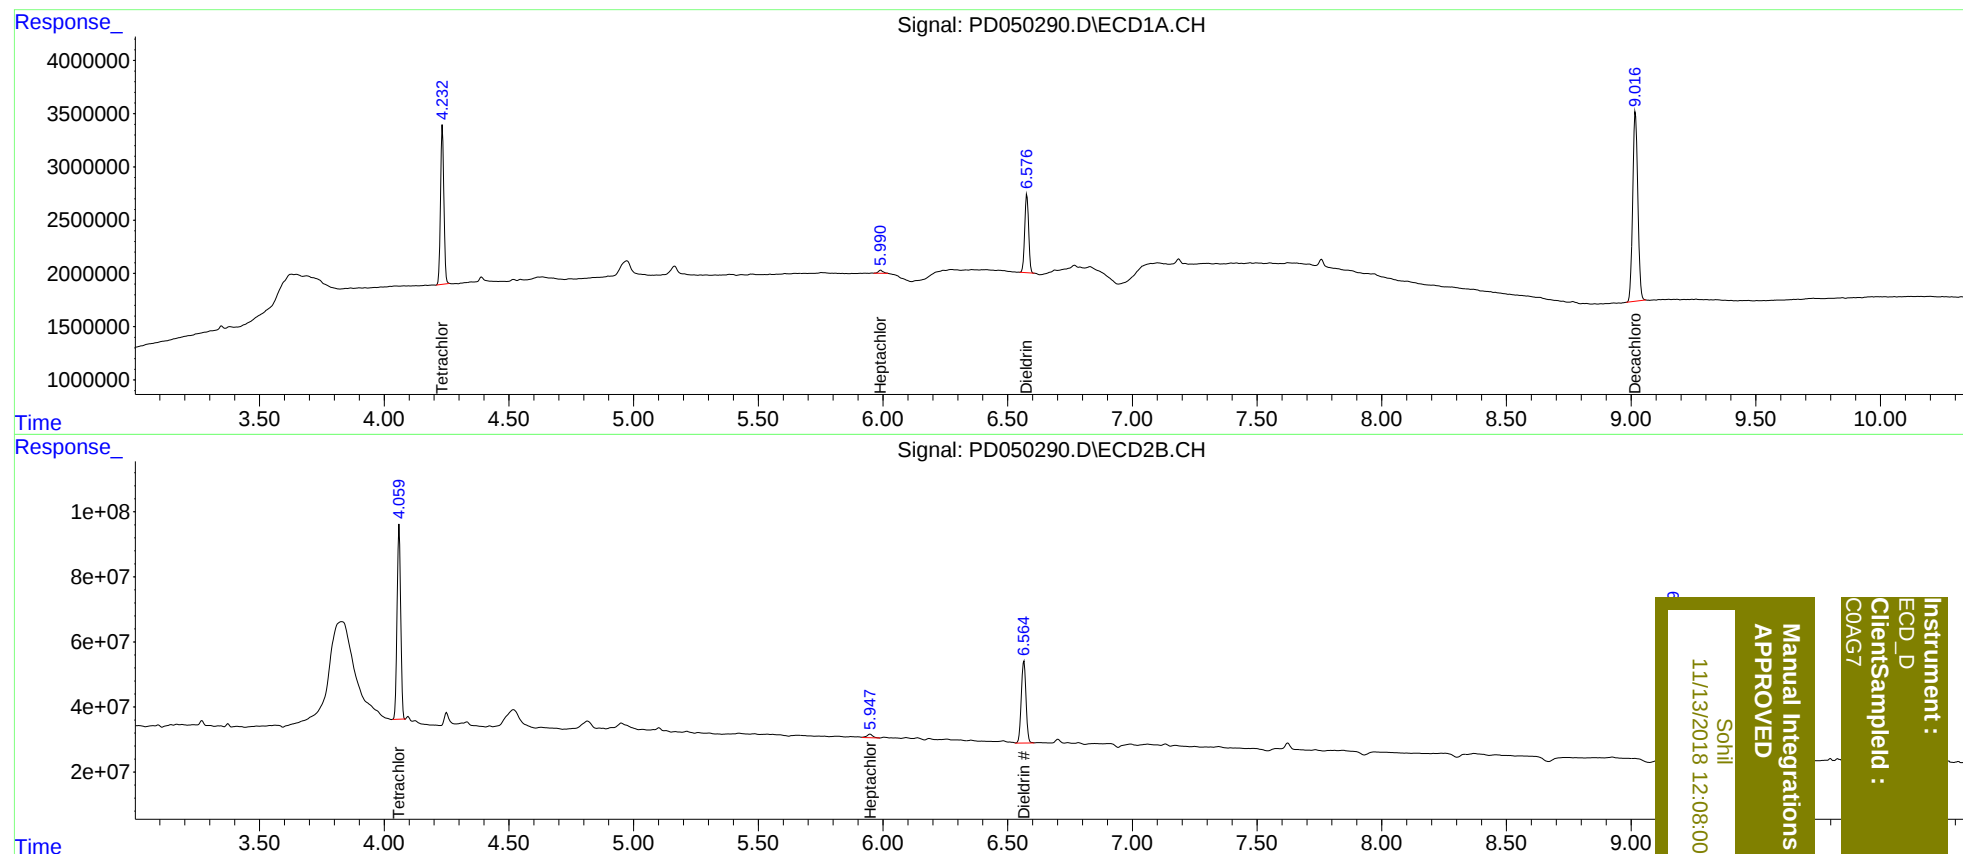

Manual Integrations
APPROVED

Sohil
11/13/2018 12:08:00 PM

Instrument :
ECD_D
ClientSampled :
COAG7