

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112221\
 Data File : PD067059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2021 15:45
 Operator : AR\AJ
 Sample : M4770-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CC-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 04:55:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 28 02:17:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.967	34002500	178.8E6	18.224	22.097
28)	SA Decachlor...	8.163	9.028	20209593	107.8E6	17.491	20.022
Target Compounds							
2)	A alpha-BHC	0.000	4.341f	0	1298252	N.D.	0.118 #
3)	MA gamma-BHC...	4.160	4.628f	3924632	1864876	1.300	0.187 #
6)	B beta-BHC	0.000	4.842f	0	1592365	N.D.	0.342 #
15)	B Endosulfa...	6.255	6.900	1768314	2437969	0.889	0.345 #
27)	Chlordane-5	6.255	0.000	1768314	0	20.909	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112221\
Data File : PD067059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2021 15:45
Operator : AR\AJ
Sample : M4770-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
CC-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 04:55:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD102821.M
Quant Title : GC Extractables
QLast Update : Thu Oct 28 02:17:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

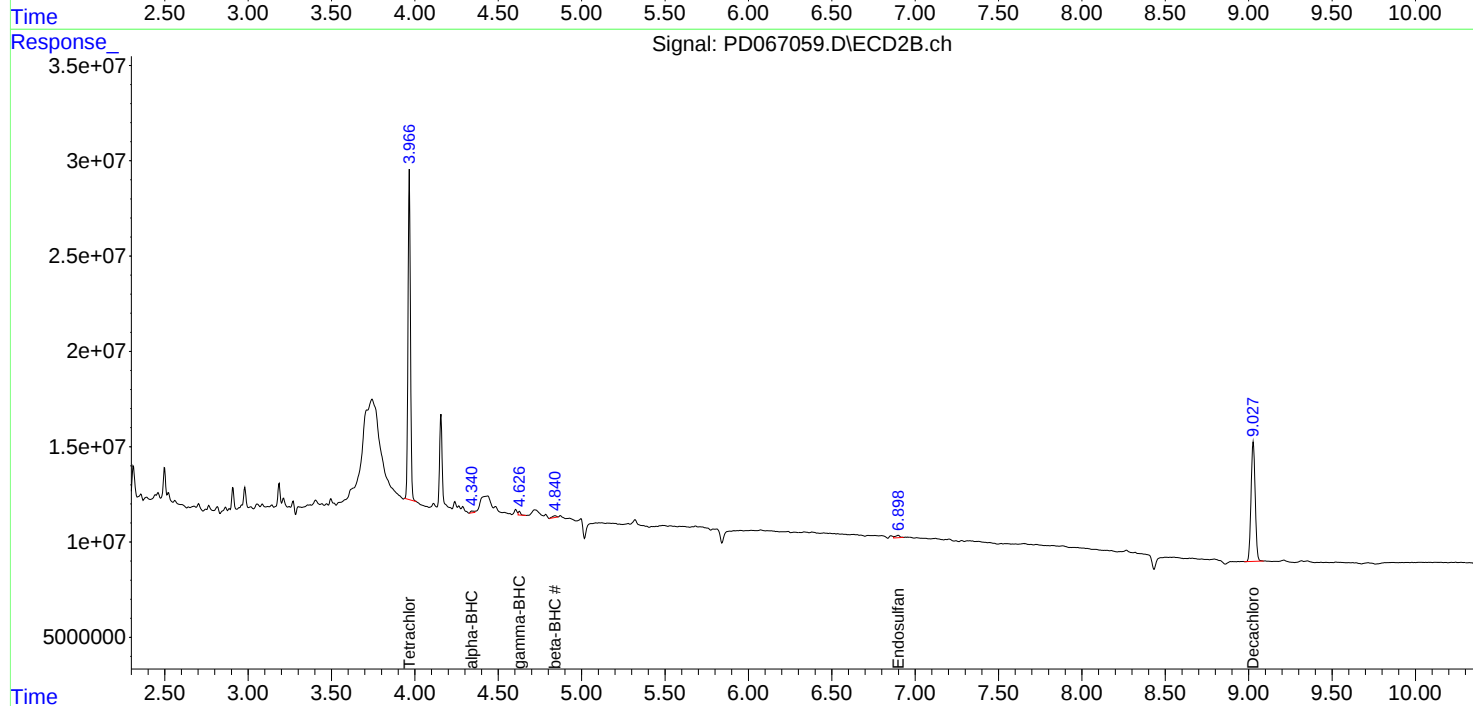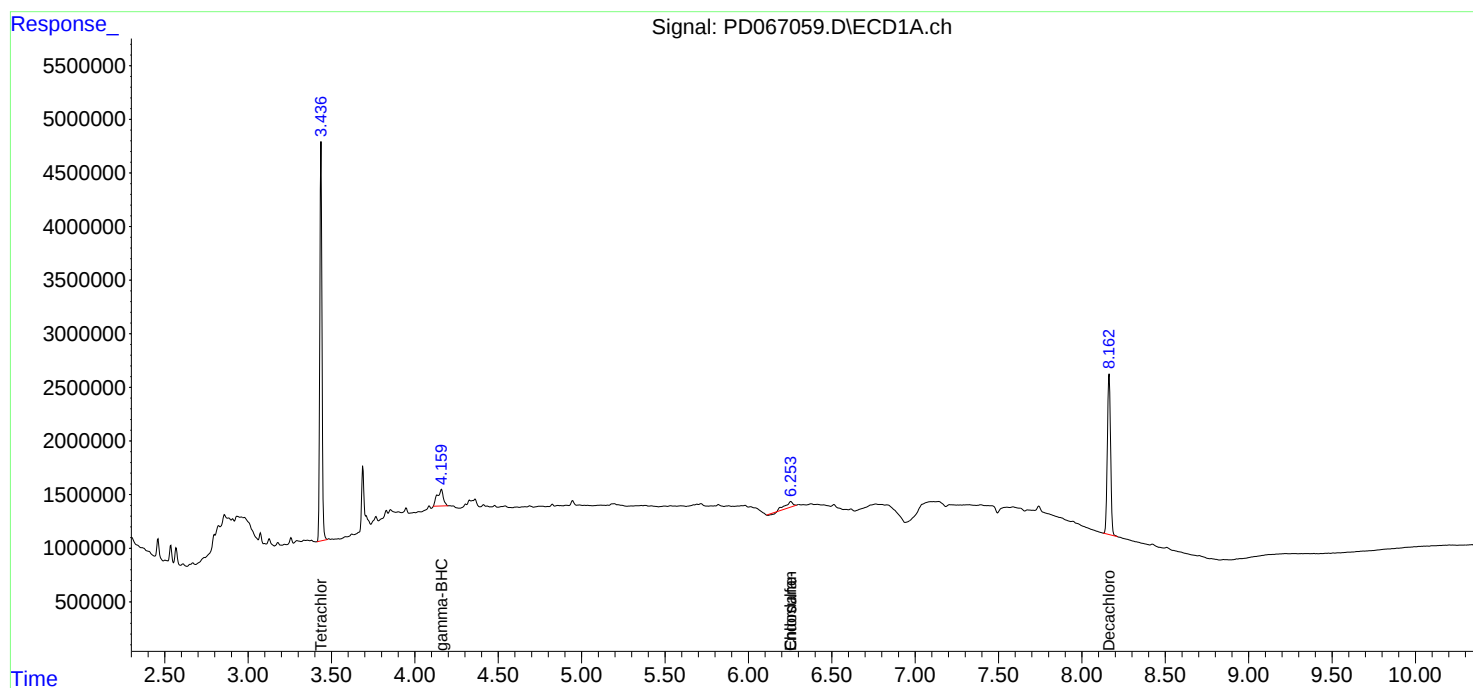


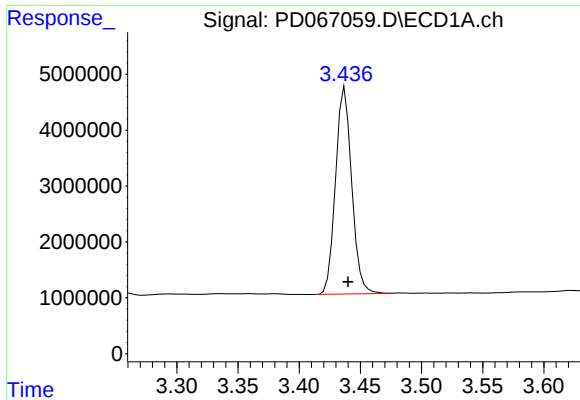

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 34002500
Conc: 18.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
CC-1

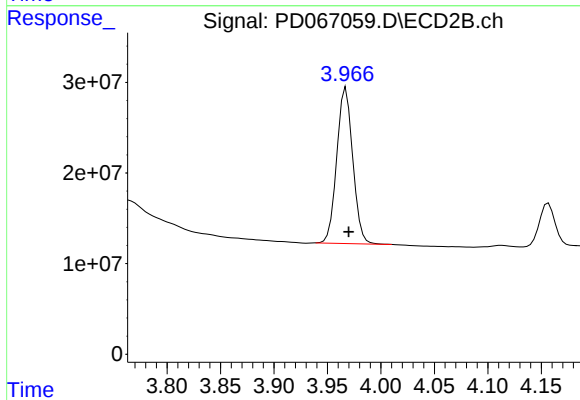


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.002 min
Response: 178808360
Conc: 22.10 ng/ml

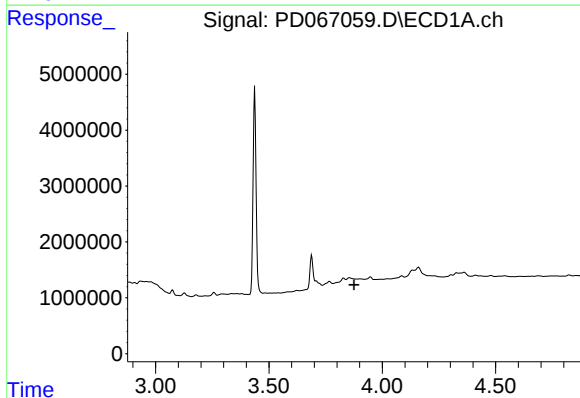


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.876 min
Response: 0
Conc: N.D.

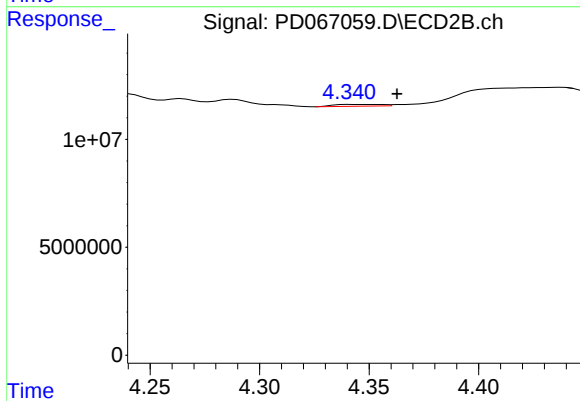

#2 alpha-BHC


R.T.: 4.341 min
Delta R.T.: -0.021 min
Response: 1298252
Conc: 0.12 ng/ml

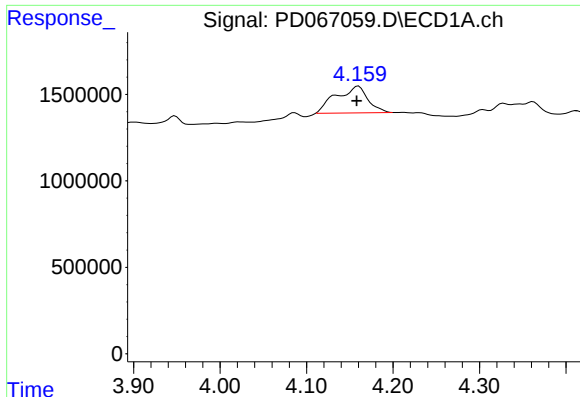

#3 gamma-BHC (Lindane)


R.T.: 4.160 min
Delta R.T.: 0.002 min
Response: 3924632
Conc: 1.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
CC-1

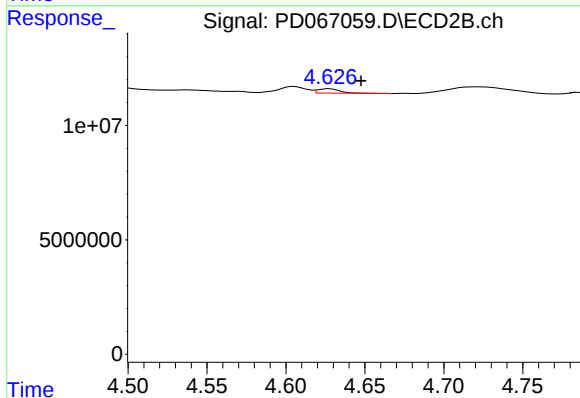


#3 gamma-BHC (Lindane)

R.T.: 4.628 min
Delta R.T.: -0.020 min
Response: 1864876
Conc: 0.19 ng/ml

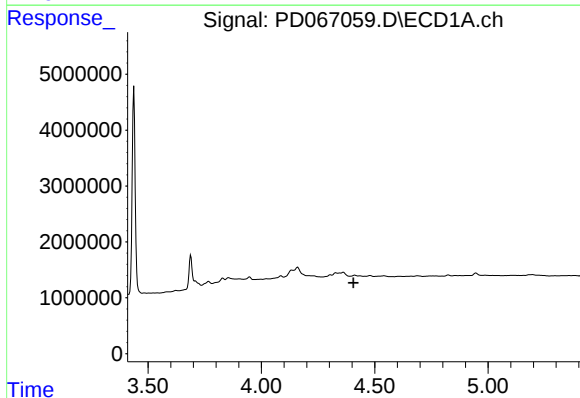


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.406 min
Response: 0
Conc: N.D.

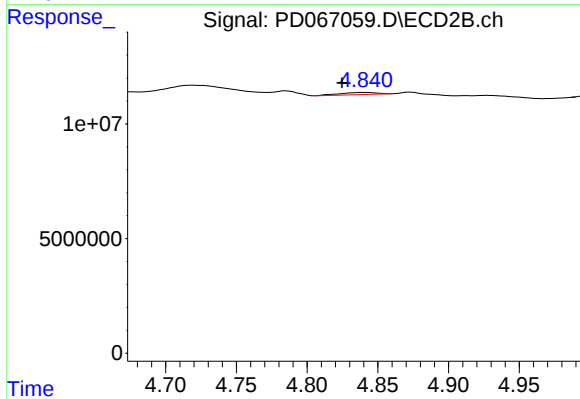

#6 beta-BHC


R.T.: 4.842 min
Delta R.T.: 0.017 min
Response: 1592365
Conc: 0.34 ng/ml

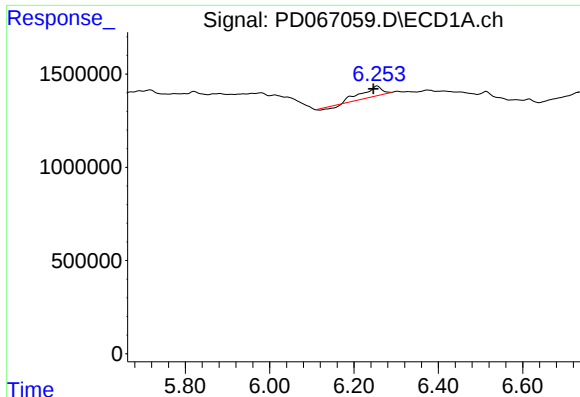

#15 Endosulfan II


R.T.: 6.255 min
Delta R.T.: 0.009 min
Response: 1768314
Conc: 0.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
CC-1

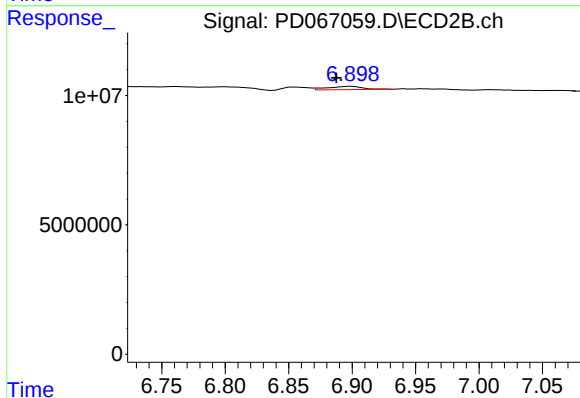


#15 Endosulfan II

R.T.: 6.900 min
Delta R.T.: 0.012 min
Response: 2437969
Conc: 0.35 ng/ml

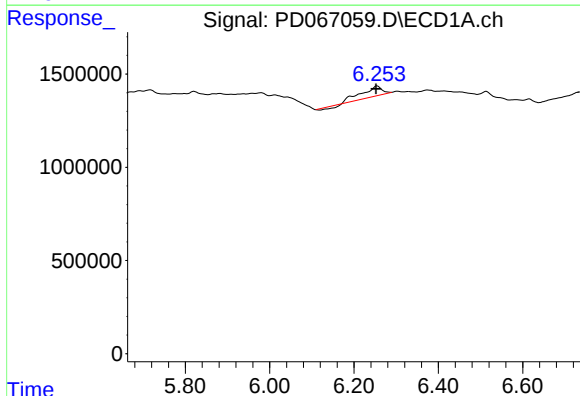


#27 Chlordane-5

R.T.: 6.255 min
Delta R.T.: 0.003 min
Response: 1768314
Conc: 20.91 ng/ml

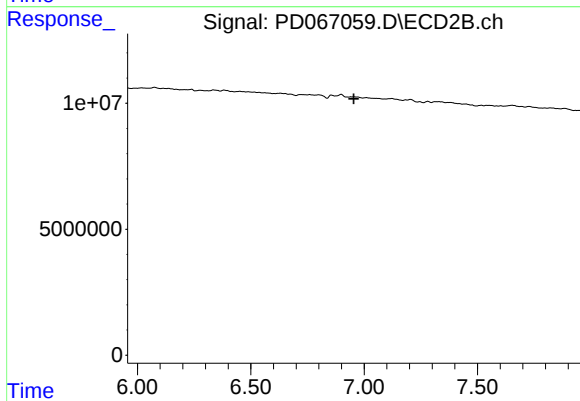

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.955 min
Response: 0
Conc: N.D.

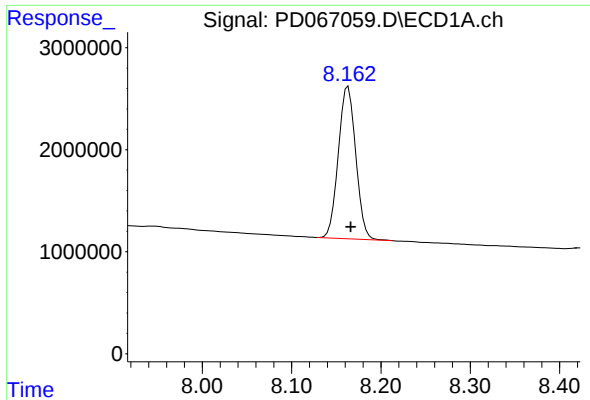

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: -0.003 min
Response: 20209593
Conc: 17.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
CC-1

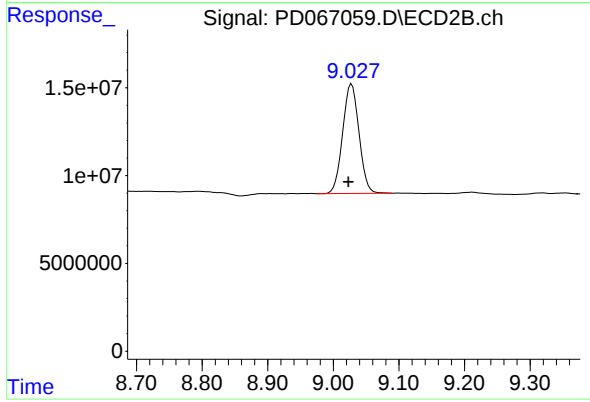

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: 0.005 min
Response: 107847622
Conc: 20.02 ng/ml