

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
 Data File : PD079848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 10:28
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 19:57:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.767f	0	73328	N.D.	<MDL
Target Compounds						
2) A alpha-BHC	0.000	3.324	0	114251	N.D.	<MDL
3) MA gamma-BHC...	0.000	3.655	0	65052	N.D.	<MDL
4) MA Heptachlor	0.000	4.001	0	73496	N.D.	<MDL
5) MB Aldrin	0.000	4.234f	0	237623	N.D.	<MDL
6) B beta-BHC	0.000	3.890f	0	213405	N.D.	0.130
13) MA Dieldrin	0.000	5.364	0	339795	N.D.	0.107
14) MA Endrin	0.000	5.685	0	544837	N.D.	0.199
17) MA 4,4'-DDT	0.000	6.066	0	117402	N.D.	<MDL
19) B Endosulfa...	0.000	6.386	0	168086	N.D.	<MDL
20) A Methoxychlor	0.000	6.647	0	136196	N.D.	0.106
23) Toxaphene-2	0.000	5.364	0	339795	N.D.	20.220
24) Toxaphene-3	0.000	6.647	0	136196	N.D.	2.365
26) Toxaphene-5	0.000	7.090	0	274989	N.D.	8.236

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
Data File : PD079848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2023 10:28
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 19:57:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

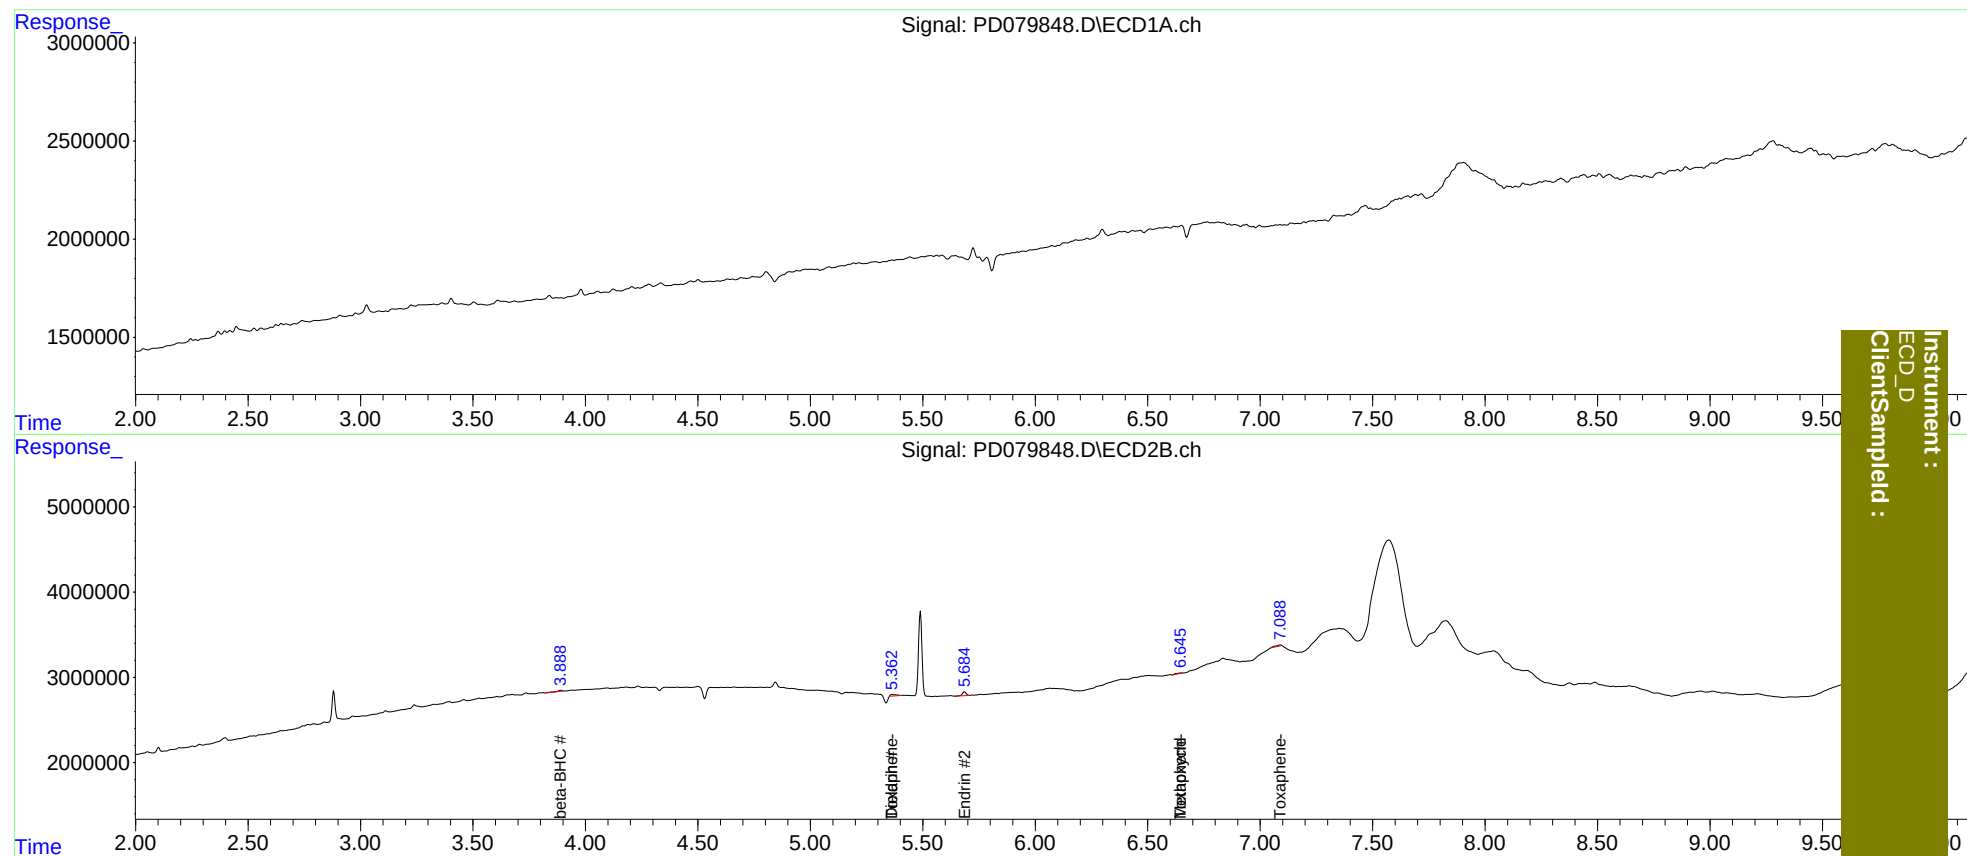


Instrument :
ECD_D
ClientSampled :
0

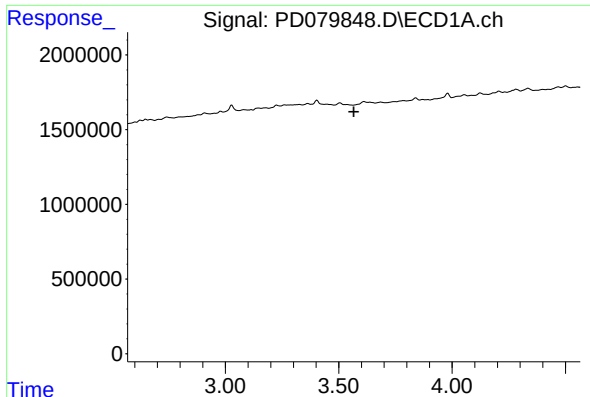

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.567 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

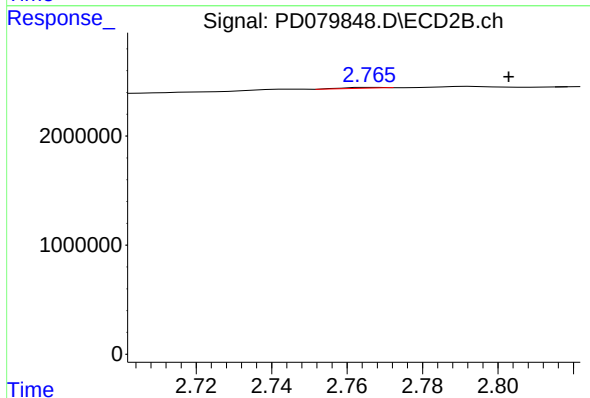


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: -0.036 min
Response: 73328
Conc: N.D.

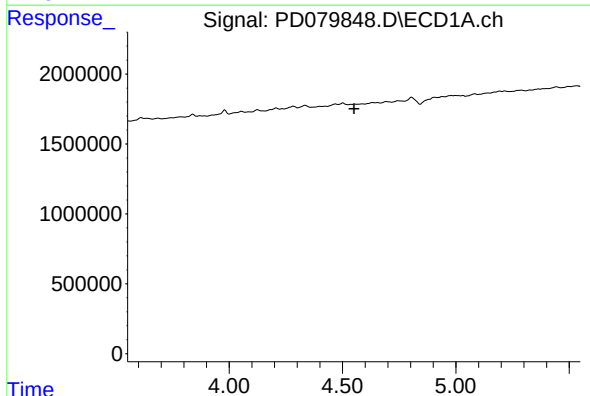


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.551 min
Response: 0
Conc: N.D.

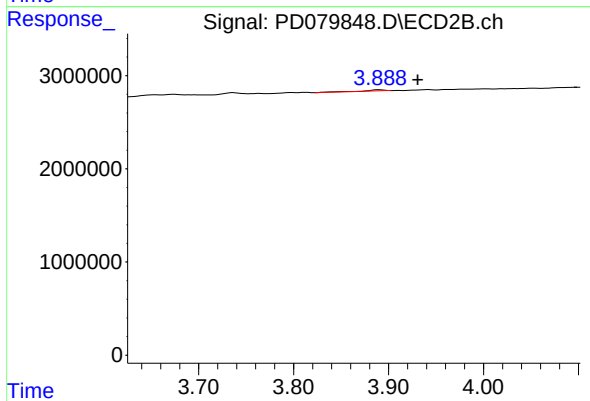

#6 beta-BHC


R.T.: 3.890 min
Delta R.T.: -0.040 min
Response: 213405
Conc: 0.13 ng/ml

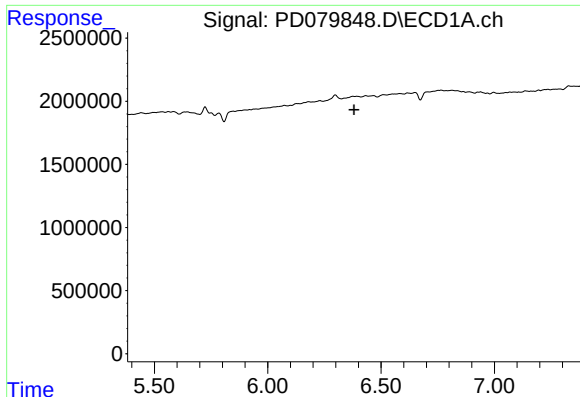

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

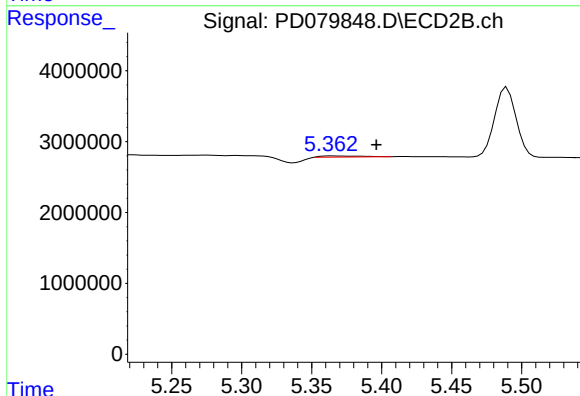


#13 Dieldrin

R.T.: 5.364 min
Delta R.T.: -0.032 min
Response: 339795
Conc: 0.11 ng/ml

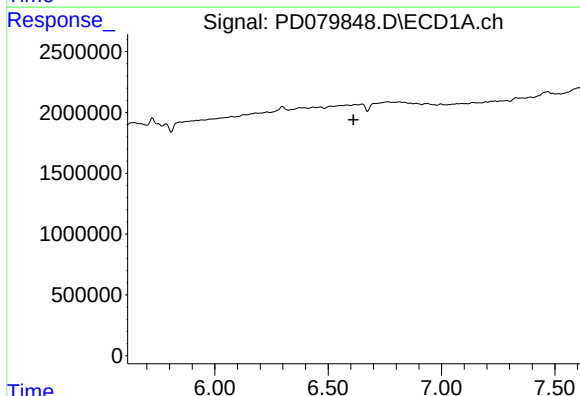


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

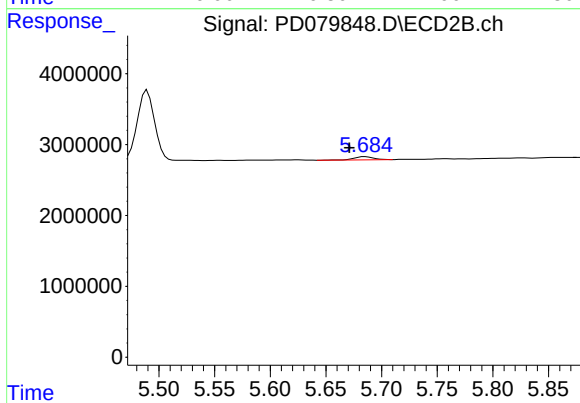

#14 Endrin


R.T.: 5.685 min
Delta R.T.: 0.014 min
Response: 544837
Conc: 0.20 ng/ml

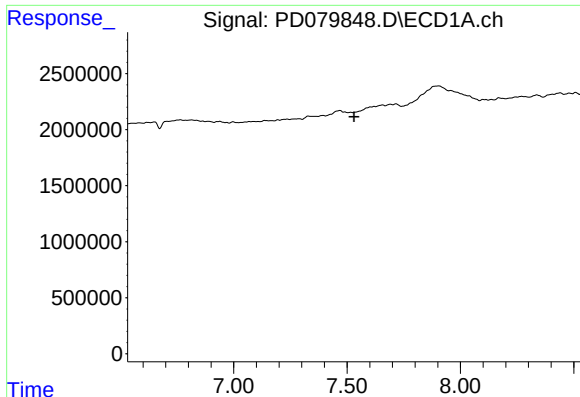

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

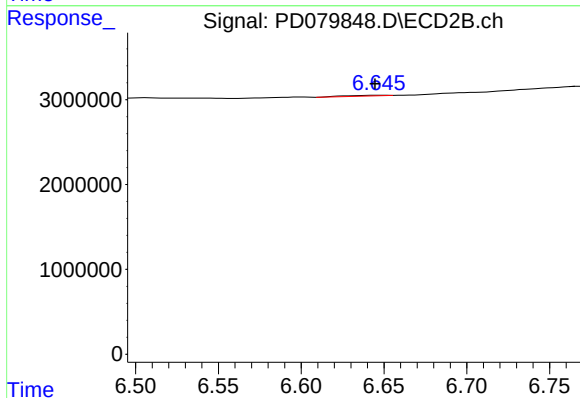


#20 Methoxychlor

R.T.: 6.647 min
Delta R.T.: 0.002 min
Response: 136196
Conc: 0.11 ng/ml

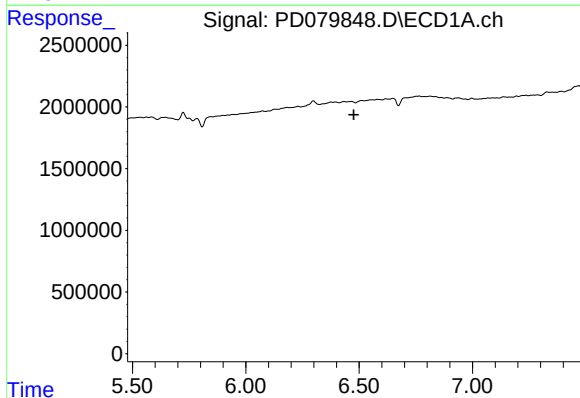


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.477 min
Response: 0
Conc: N.D.

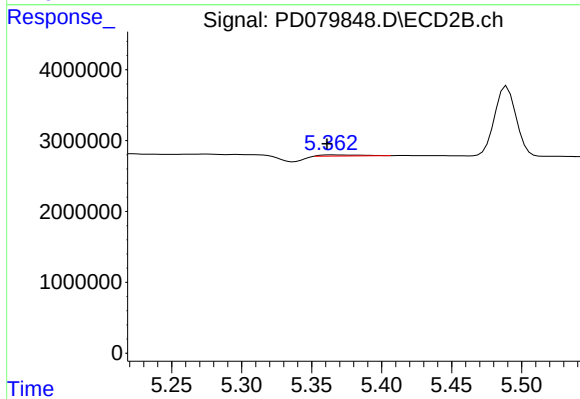

#23 Toxaphene-2


R.T.: 5.364 min
Delta R.T.: 0.003 min
Response: 339795
Conc: 20.22 ng/ml

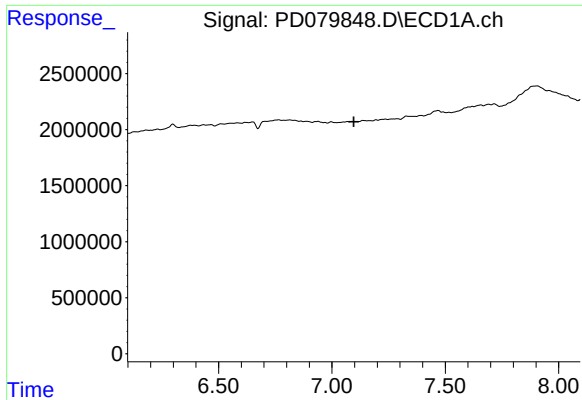

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 7.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

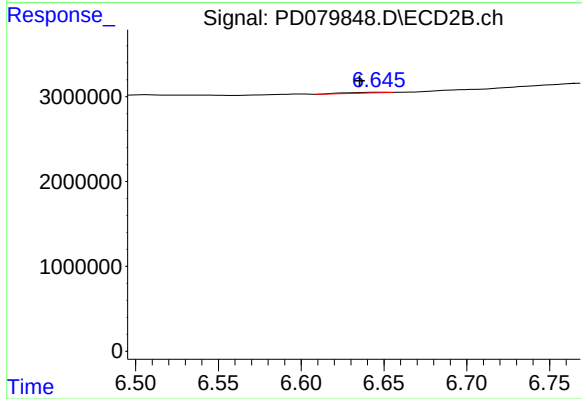


#24 Toxaphene-3

R.T.: 6.647 min
Delta R.T.: 0.012 min
Response: 136196
Conc: 2.37 ng/ml

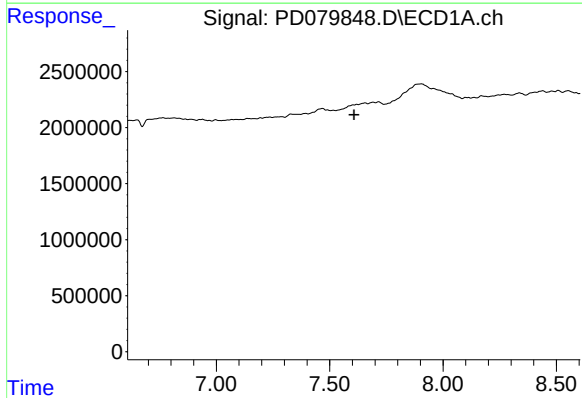


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.608 min
Response: 0
Conc: N.D.

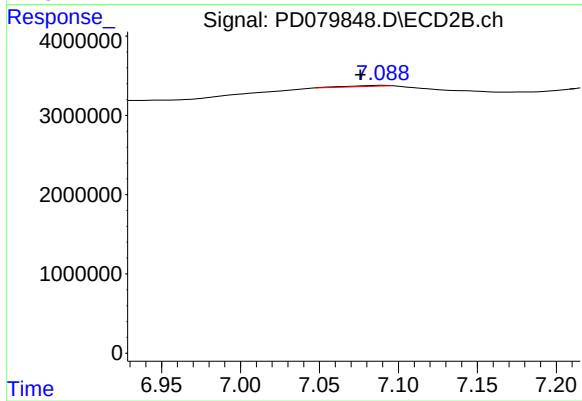

#26 Toxaphene-5


R.T.: 7.090 min
Delta R.T.: 0.014 min
Response: 274989
Conc: 8.24 ng/ml

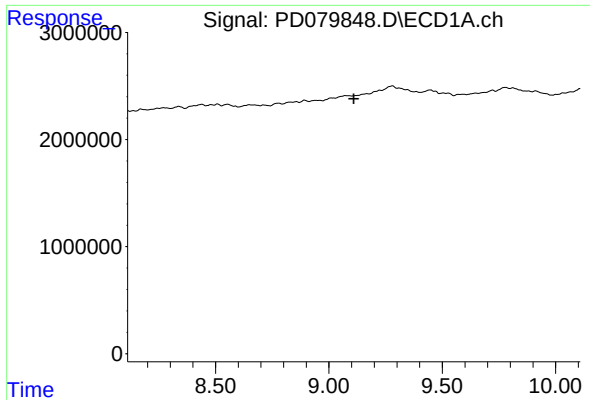

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.110 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

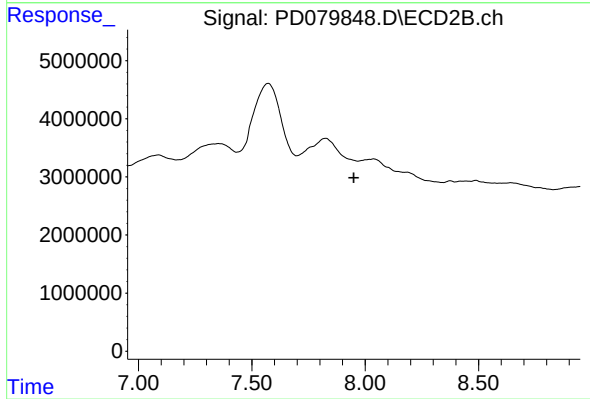

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.949 min
Response: 0
Conc: N.D.