

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
 Data File : PD079855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 15:15
 Operator : AR\AJ
 Sample : PB157407BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 19:59:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.801	29967063	49457947	20.520	21.623
2)	SA Decachlor...	9.116	7.946	35255446	57221130	19.867	23.967
Target Compounds							
3)	MA gamma-BHC...	0.000	3.652	0	206724	N.D.	<MDL
5)	MB Aldrin	0.000	4.238	0	68260	N.D.	<MDL
6)	B beta-BHC	0.000	3.893f	0	125197	N.D.	<MDL
7)	B delta-BHC	0.000	4.184	0	739859	N.D.	0.207
9)	A Endosulfan I	0.000	5.129	0	76762	N.D.	<MDL
11)	B cis-Chlor...	0.000	5.129f	0	76762	N.D.	<MDL
13)	MA Dieldrin	0.000	5.460f	0	1144495	N.D.	0.359
14)	MA Endrin	0.000	5.684	0	480250	N.D.	0.175
15)	B Endosulfa...	0.000	5.925f	0	125046	N.D.	<MDL
17)	MA 4,4'-DDT	0.000	6.018f	0	155115	N.D.	<MDL
18)	B Endrin al...	0.000	6.152	0	106720	N.D.	<MDL
21)	B Endrin ke...	0.000	6.902	0	148276	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
Data File : PD079855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2023 15:15
Operator : AR\AJ
Sample : PB157407BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 19:59:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

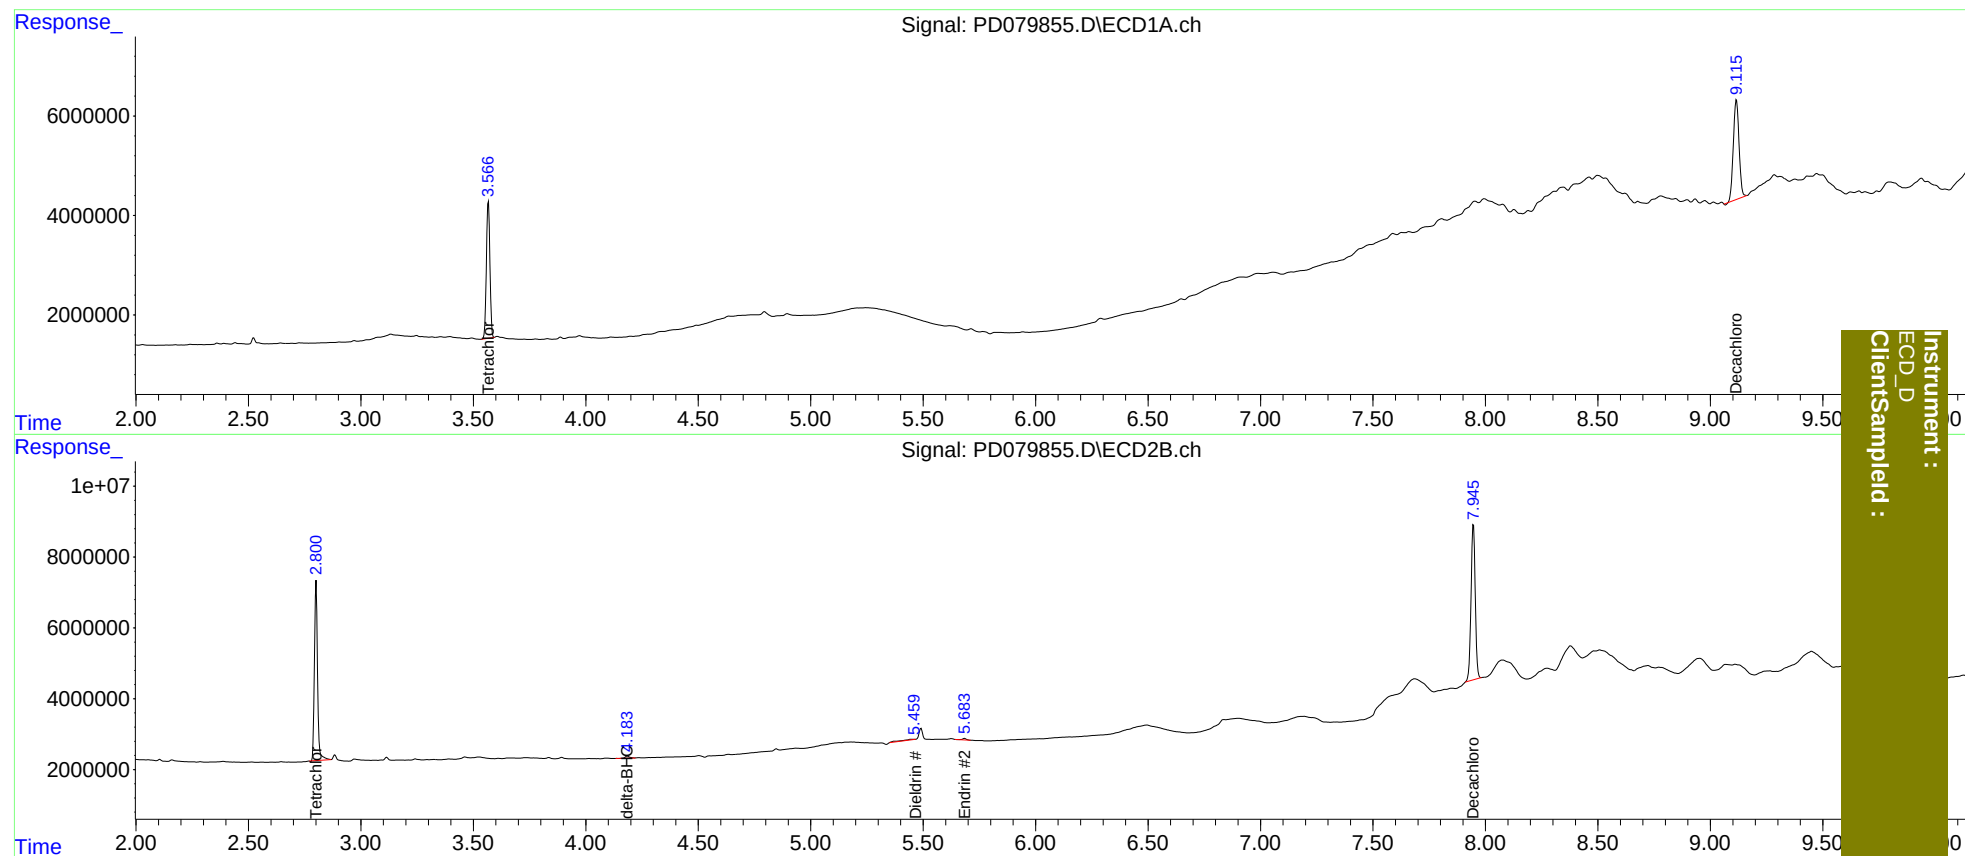


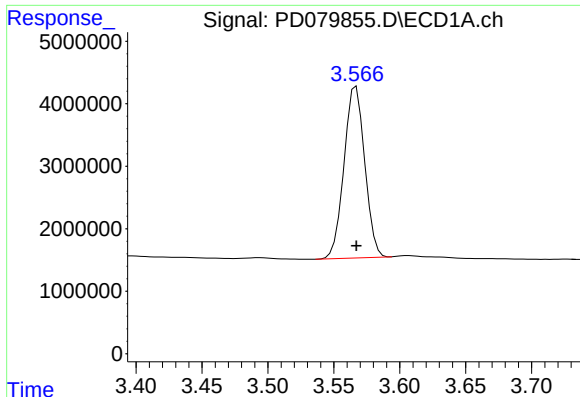

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 29967063
Conc: 20.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

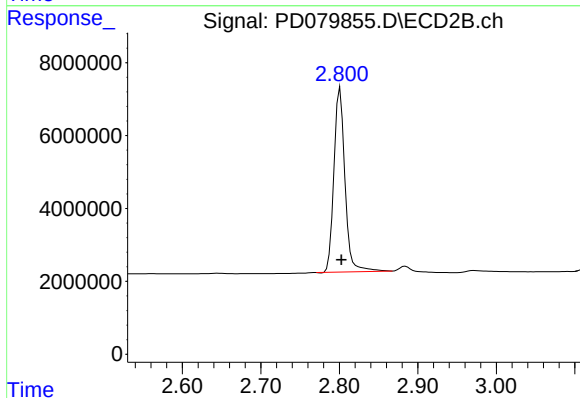


#1 Tetrachloro-m-xylene

R.T.: 2.801 min
Delta R.T.: -0.002 min
Response: 49457947
Conc: 21.62 ng/ml

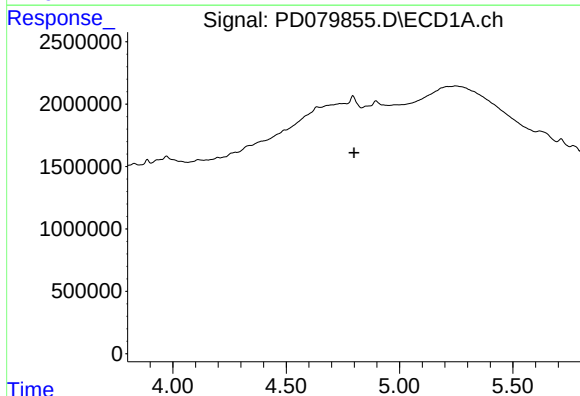


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

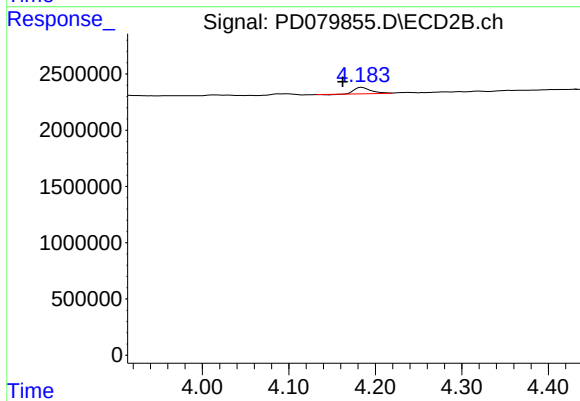

#7 delta-BHC


R.T.: 4.184 min
Delta R.T.: 0.022 min
Response: 739859
Conc: 0.21 ng/ml

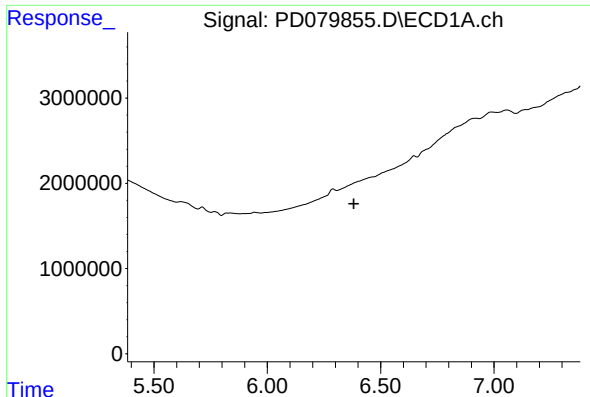

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

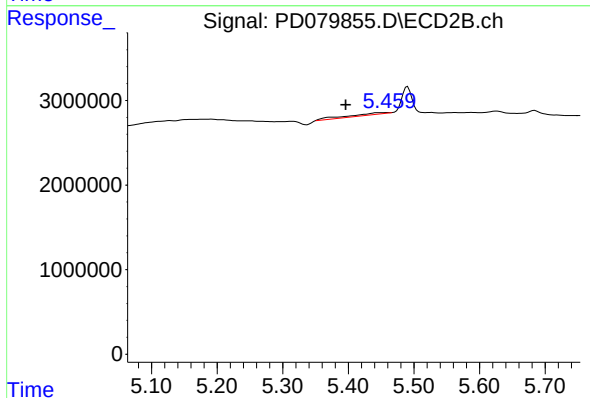


#13 Dieldrin

R.T.: 5.460 min
Delta R.T.: 0.064 min
Response: 1144495
Conc: 0.36 ng/ml

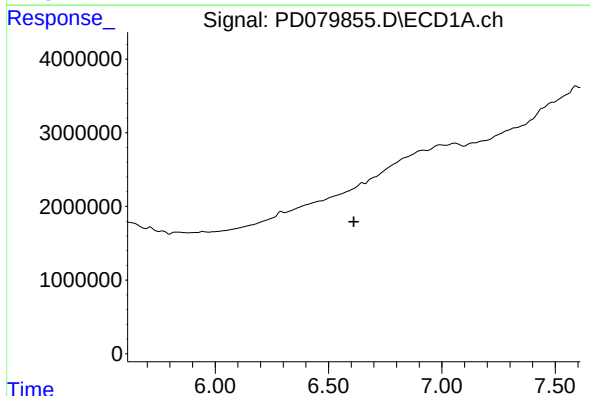


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

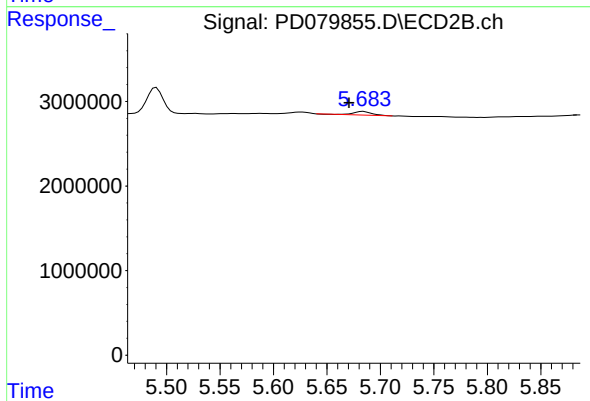

#14 Endrin


R.T.: 5.684 min
Delta R.T.: 0.013 min
Response: 480250
Conc: 0.18 ng/ml

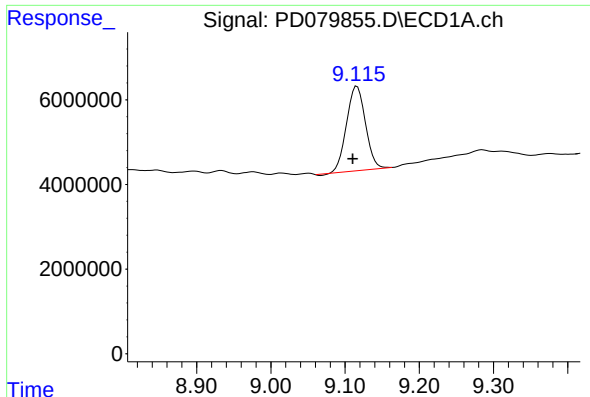

#27 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.006 min
Response: 35255446
Conc: 19.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

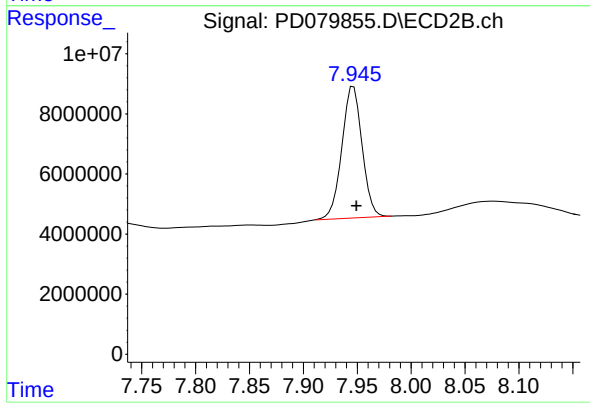

#27 Decachlorobiphenyl

R.T.: 7.946 min
Delta R.T.: -0.003 min
Response: 57221130
Conc: 23.97 ng/ml