

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
 Data File : PD079865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 18:21
 Operator : AR\AJ
 Sample : PB157419BS
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS419

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :Ankita Jodhani 11/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 20:04:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.801	36122879	59939181	24.735	26.205
27)	SA Decachlor...	9.116	7.946	55462887	86930663	31.255	36.411
Target Compounds							
2)	A alpha-BHC	4.024	3.304	8974325	13700812	3.622	3.779
3)	MA gamma-BHC...	4.358	3.634	9351741	13891864	3.958	4.044
4)	MA Heptachlor	4.951	3.975	9878949	13495116	3.944	4.045
5)	MB Aldrin	5.294	4.256	10956149	17611136	4.672	5.412
6)	B beta-BHC	4.551	3.929	5277225	7133179	4.860	4.356
7)	B delta-BHC	4.800	4.159	13011662	17035678	5.222	4.768
8)	B Heptachlo...	5.720	4.758	11687831	16081387	5.272	5.199
9)	A Endosulfan I	6.108	5.128	8215919	11285527	3.974	4.071
10)	B trans-Chl...	5.977	5.008	11001325	15850462	5.170	5.339
11)	B cis-Chlor...	6.057	5.073	10635008	15573417	4.883	5.130
12)	B 4,4'-DDE	6.227	5.261	18778275	29021601	9.512	10.364
13)	MA Dieldrin	6.383	5.393	16591888	26330320	7.542	8.269
14)	MA Endrin	6.613	5.668	13626676	23155789	7.468	8.455
15)	B Endosulfa...	6.831	5.961	18116550	26728144	9.523	10.291
16)	A 4,4'-DDD	6.744	5.815	12258177	20266854	7.567	8.609
17)	MA 4,4'-DDT	7.061	6.067	11501725	17929378	6.751	7.464
18)	B Endrin al...	6.962	6.140	14011424	22228649	9.400	10.985
19)	B Endosulfa...	7.195	6.363	17328552	26085305	9.306	10.498
20)	A Methoxychlor	7.534	6.642	34875828	55603522	37.832	43.259
21)	B Endrin ke...	7.683	6.867	18691948	29262311	9.567	10.293m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
Data File : PD079865.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2023 18:21
Operator : AR\AJ
Sample : PB157419BS
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 20:04:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

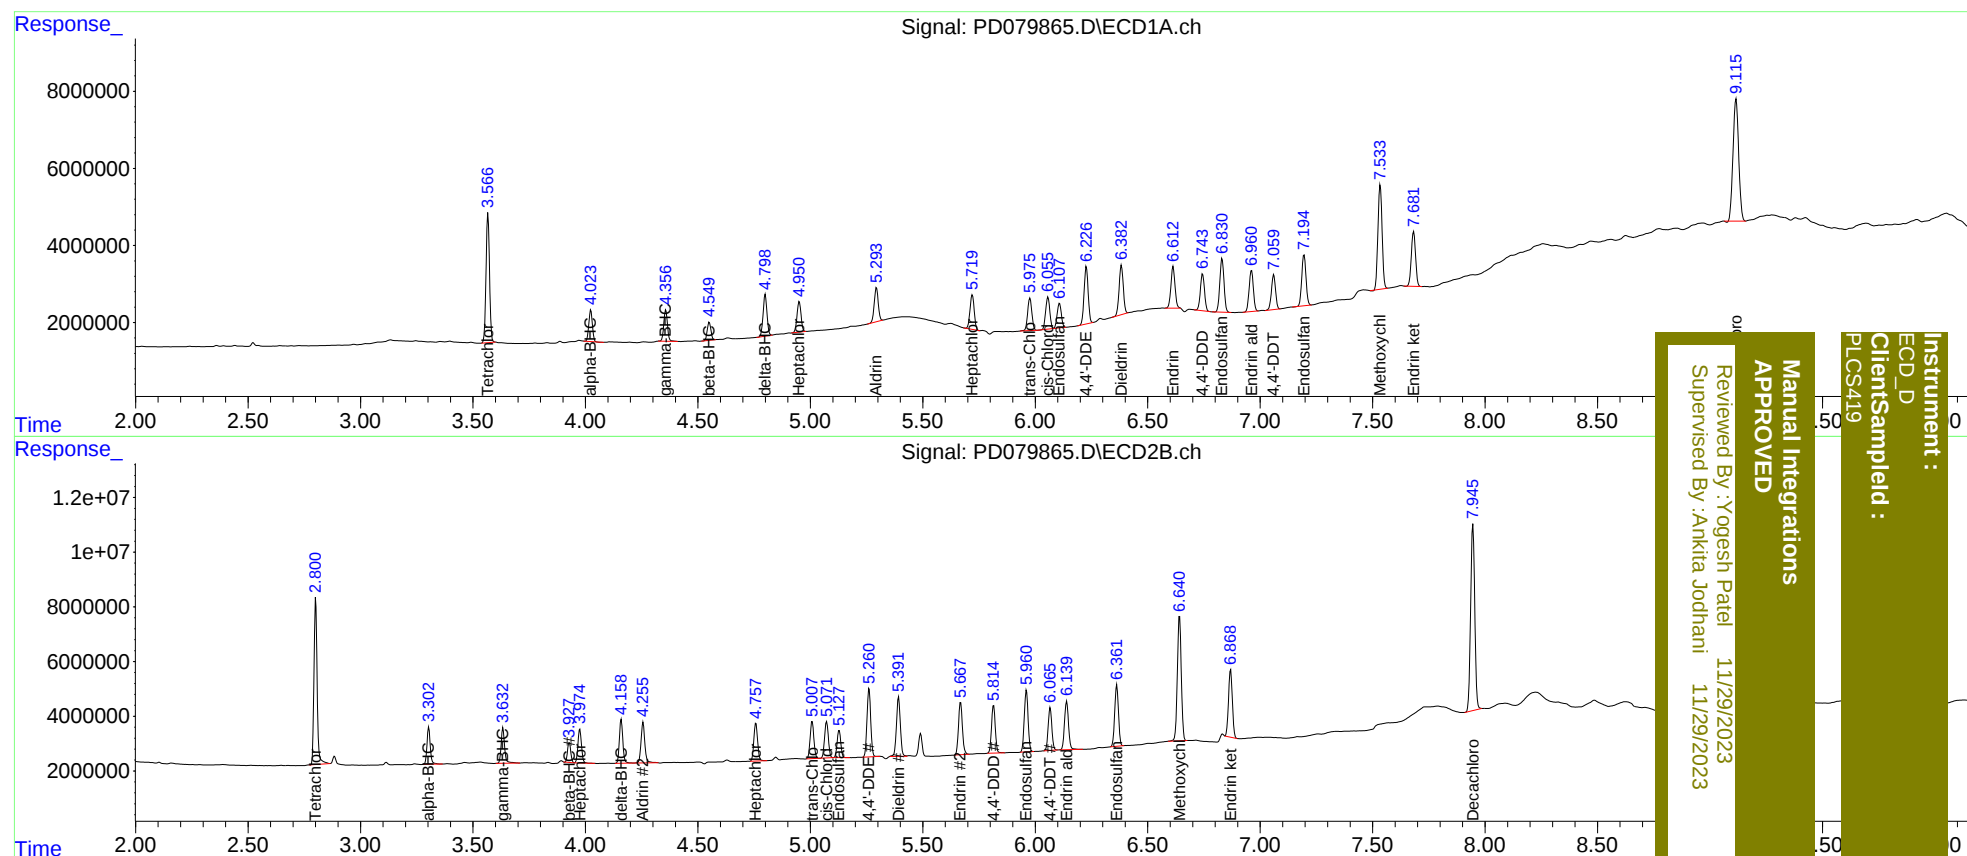

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/29/2023
Supervised By : Ankita Jodhani 11/29/2023

Instrument :
ECD_D
Client Sampled :
PLCS419