

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
 Data File : PD079858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 16:21
 Operator : AR\AJ
 Sample : 05456-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E05M5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :Ankita Jodhani 11/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 10:51:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.802	23199825	27725164	15.886	12.121
27)	SA Decachlor...	9.103	7.945	37499011	55310450	21.132	23.167
Target Compounds							
9)	A Endosulfan I	6.137	5.153	26482292	66129194	12.811m	23.854m#
10)	B trans-Chl...	5.976	5.011	37487172	64428214	17.618m	21.702
11)	B cis-Chlor...	6.059	5.073	44852873	48752349	20.594	16.061
16)	A 4,4'-DDD	6.735	5.813	22456916	28676930	13.863	12.182m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
Data File : PD079858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2023 16:21
Operator : AR\AJ
Sample : 05456-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 10:51:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

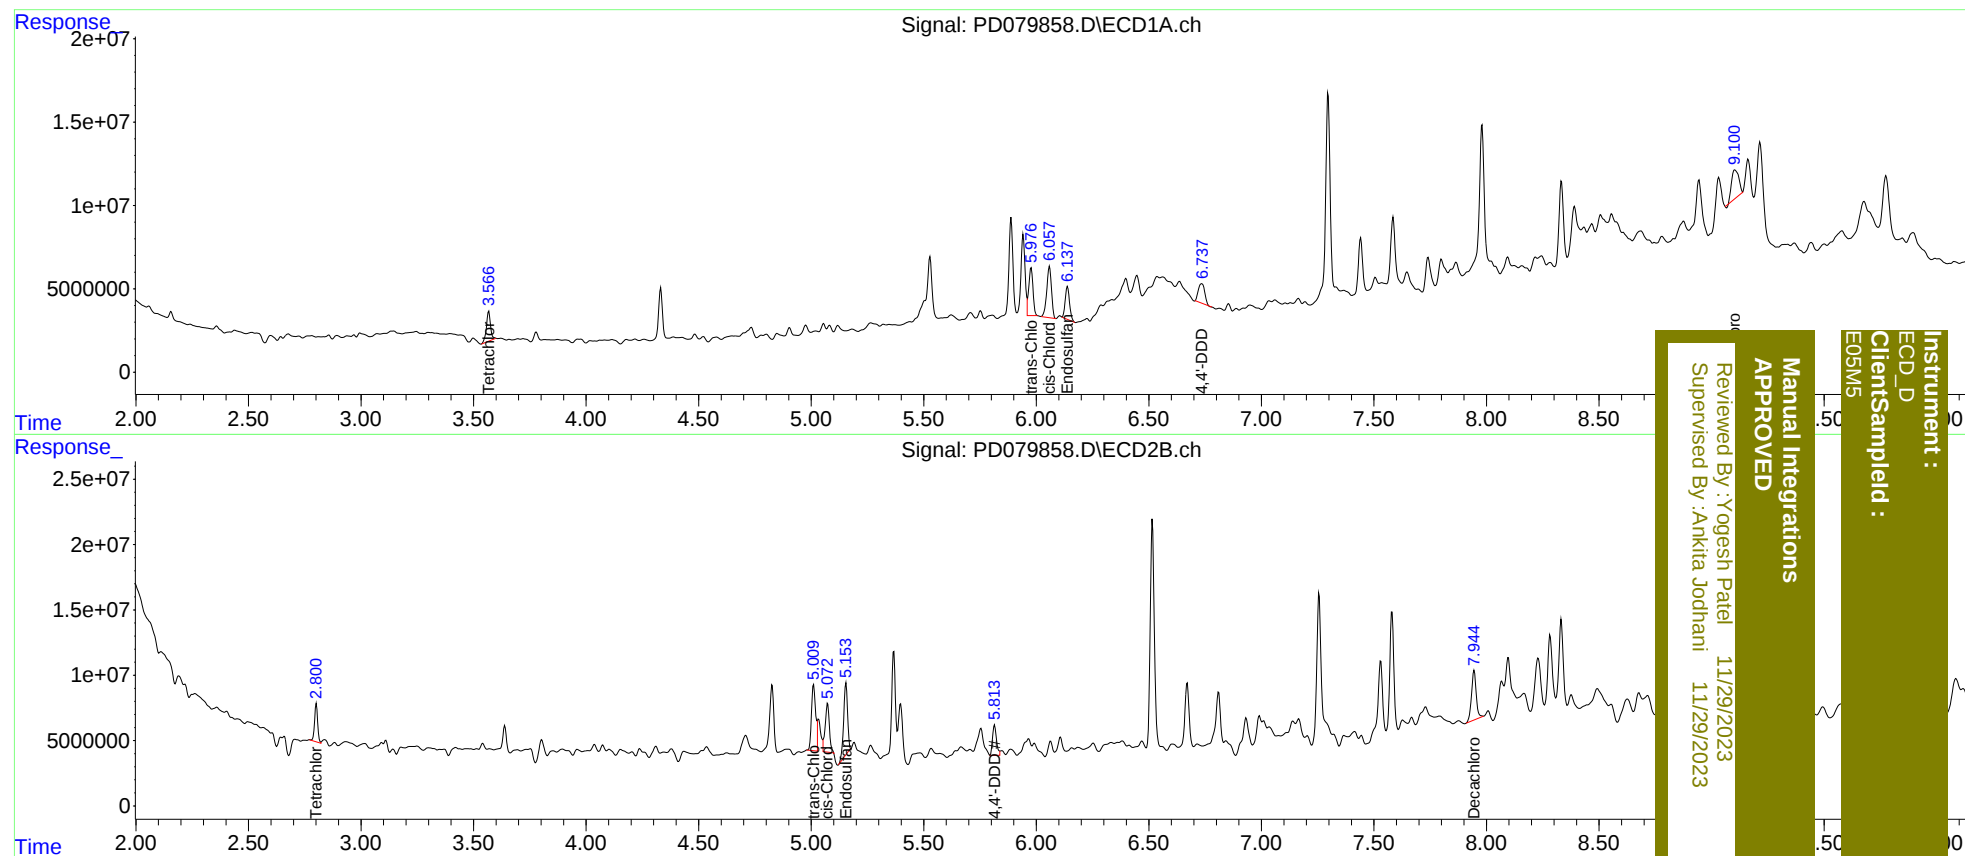

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/29/2023
Supervised By : Ankita Jodhani 11/29/2023

Instrument :
ECD_D
ClientSampled :
E05M5