

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
 Data File : PD079870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 19:27
 Operator : AR\AJ
 Sample : 05497-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
ClientSampleId :
 C0AC2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :Ankita Jodhani 11/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 20:06:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.568	2.802	22095532	36889455	15.130	16.128
27) SA Decachlor...	9.115	7.946	29781173	40963364	16.782m	17.158
Target Compounds						
5) MB Aldrin	5.279	4.276	2489437	3970631	1.062m	1.220
6) B beta-BHC	4.566	3.954	2742293	6219566	2.526m	3.798m#
7) B delta-BHC	4.798	4.153	3342375	3845208	1.341m	1.076
16) A 4,4'-DDD	6.727	5.811	10825986	16992930	6.683m	7.218

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
 Data File : PD079870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 19:27
 Operator : AR\AJ
 Sample : 05497-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 20:06:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

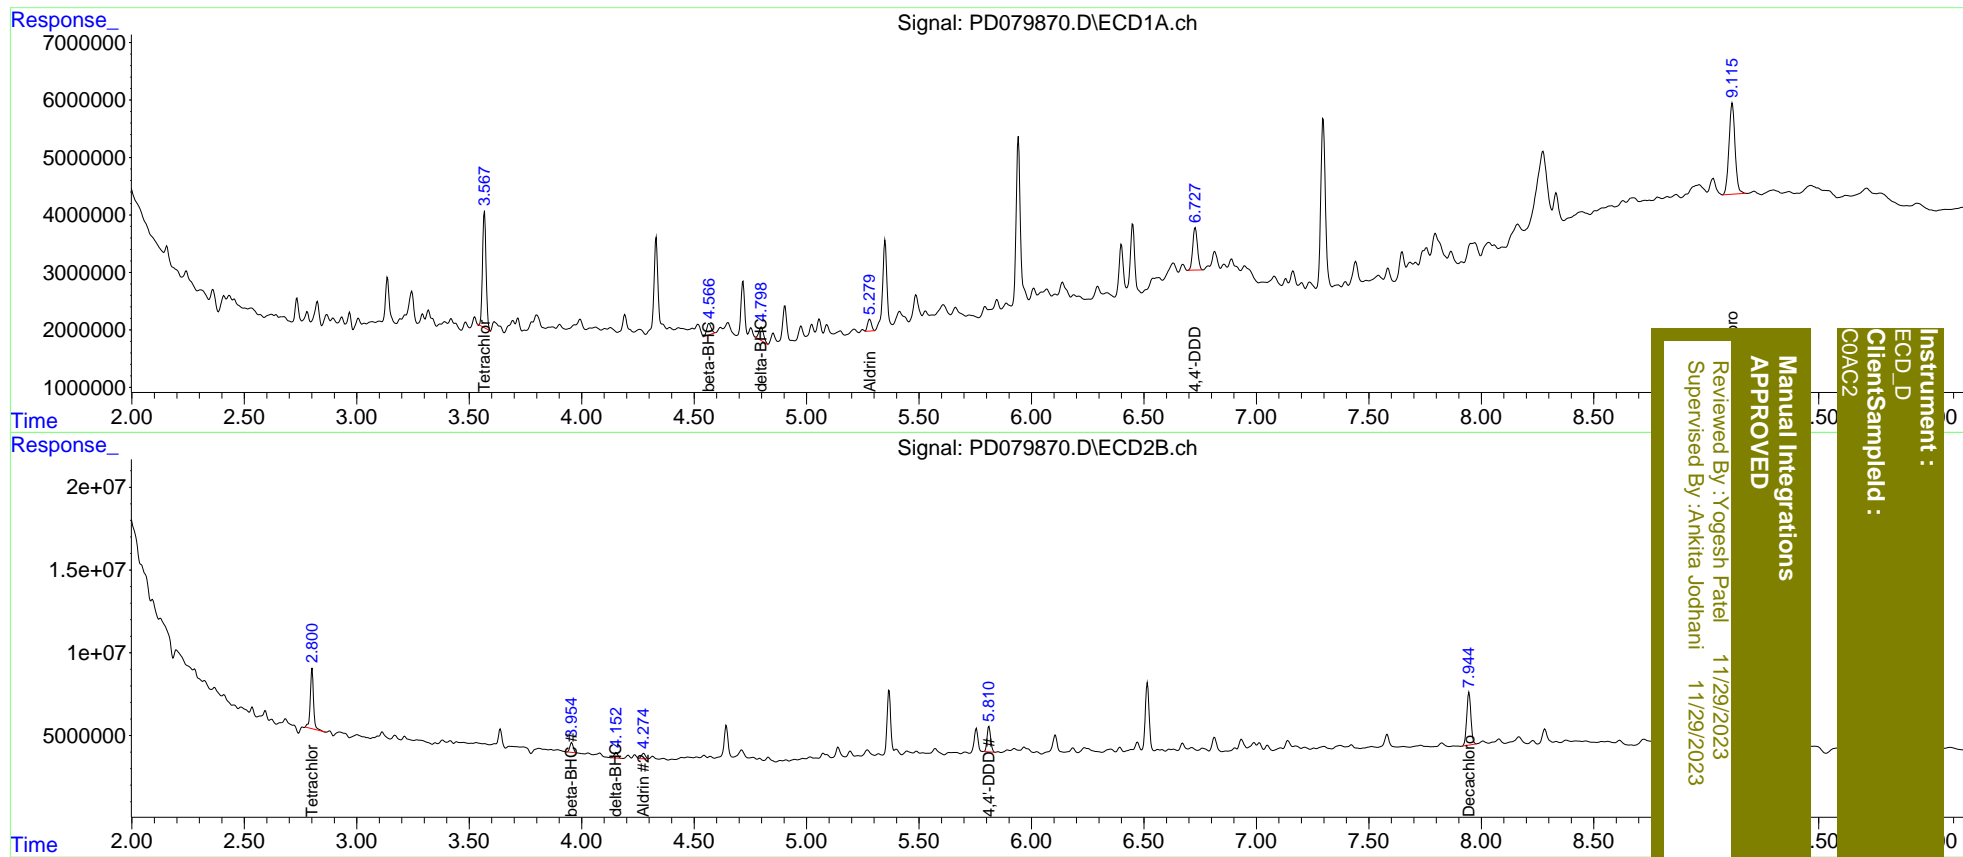

Instrument : ECD_D
 ClientSampled : COAC2
 Manual Integrations APPROVED
 Reviewed By : Yogesh Patel 11/29/2023
 Supervised By : Ankita Jodhani 11/29/2023