

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
 Data File : PD079871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2023 19:41
 Operator : AR\AJ
 Sample : 05497-12MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AC2MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/29/2023
 Supervised By :Ankita Jodhani 11/29/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 02:59:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.802	21205690	35502242	14.521	15.521
27)	SA Decachlor...	9.115	7.946	29787676	39473843	16.786	16.534
Target Compounds							
2)	A alpha-BHC	4.024	3.304	116.6E6	183.8E6	47.061	50.693
3)	MA gamma-BHC...	4.356	3.634	109.0E6	173.5E6	46.136m	50.516
4)	MA Heptachlor	4.951	3.975	97743092	152.1E6	39.025	45.599
5)	MB Aldrin	5.294	4.256	95257531	139.8E6	40.622	42.951
6)	B beta-BHC	4.552	3.929	40627440	62082560	37.417	37.909
7)	B delta-BHC	4.800	4.159	99402179	149.0E6	39.890	41.714
8)	B Heptachlo...	5.721	4.758	86667764	134.2E6	39.094	43.391
9)	A Endosulfan I	6.107	5.129	90834726	129.7E6	43.941	46.778
10)	B trans-Chl...	5.975	5.008	87700612	129.5E6	41.218m	43.634
11)	B cis-Chlor...	6.057	5.073	95202981	133.0E6	43.712	43.815
12)	B 4,4'-DDE	6.227	5.262	185.9E6	287.7E6	94.167	102.756
13)	MA Dieldrin	6.382	5.393	212.8E6	316.7E6	96.751	99.457
14)	MA Endrin	6.613	5.668	182.3E6	290.6E6	99.933	106.107
15)	B Endosulfa...	6.830	5.960	179.9E6	276.1E6	94.542	106.326
16)	A 4,4'-DDD	6.744	5.814	164.6E6	261.2E6	101.634	110.948
17)	MA 4,4'-DDT	7.059	6.067	174.0E6	248.7E6	102.123	103.534
18)	B Endrin al...	6.960	6.139	133.1E6	188.0E6	89.314	92.897m
19)	B Endosulfa...	7.196	6.362	173.1E6	257.4E6	92.941	103.582
20)	A Methoxychlor	7.533	6.642	436.9E6	634.1E6	473.971	493.297
21)	B Endrin ke...	7.682	6.869	185.5E6	289.9E6	94.956	101.971

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112823\
Data File : PD079871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2023 19:41
Operator : AR\AJ
Sample : 05497-12MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 02:59:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

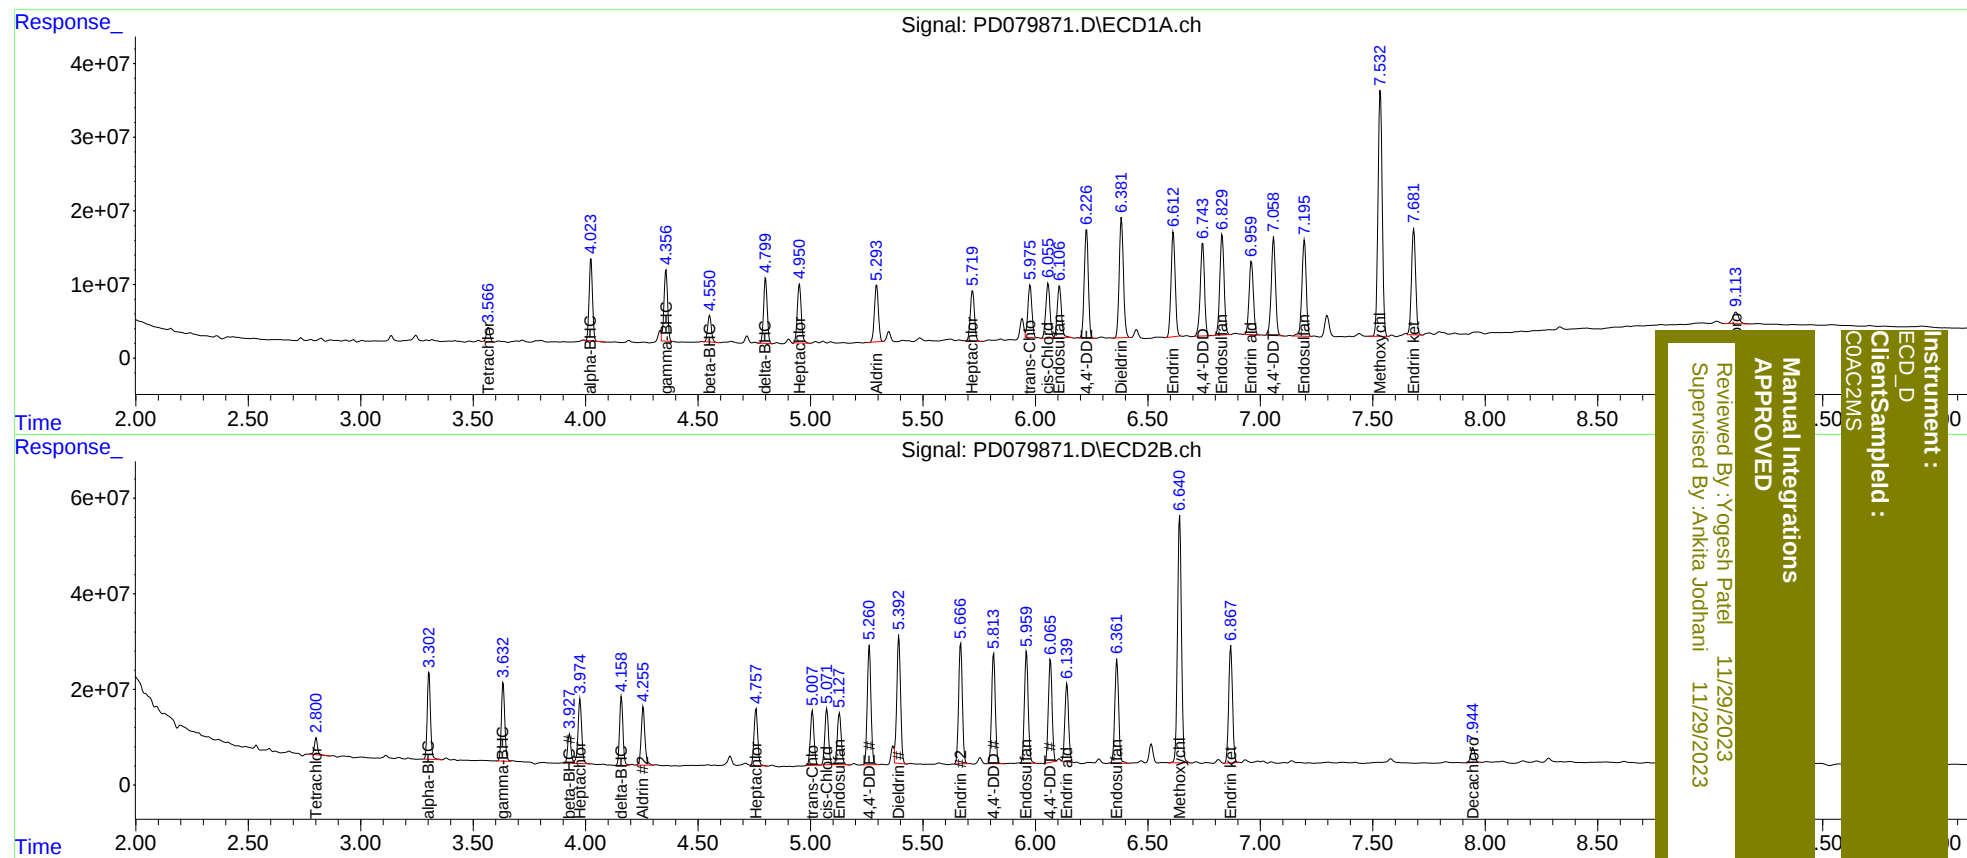

Instrument :
ECD_D
ClientSampled :
COAC2MS

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/29/2023
Supervised By : Ankita Jodhani 11/29/2023