

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121921\
 Data File : PD067449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Dec 2021 17:42
 Operator : AR\AJ
 Sample : M5090-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 20 00:53:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121821CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 18 01:09:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.965	43070223	171.2E6	20.580	16.259
27)	SA Decachlor...	8.158	9.020	38706161	199.4E6	39.290	34.509
Target Compounds							
2)	A alpha-BHC	3.871	4.359	173.9E6	540.9E6	55.325	39.838 #
3)	MA gamma-BHC...	4.153	4.644	175.5E6	510.2E6	58.060	42.608 #
4)	MA Heptachlor	4.445	5.143	166.8E6	459.1E6	53.646	44.248
5)	MB Aldrin	4.690	5.447	163.9E6	439.5E6	53.139	46.604
6)	B beta-BHC	4.401	4.822	65223116	221.9E6	47.844	40.572
7)	B delta-BHC	4.603	5.037	136.9E6	428.0E6	47.867	42.848
8)	B Heptachlo...	5.131	5.836	148.9E6	360.5E6	53.888	56.271
9)	A Endosulfan I	5.467	6.193	135.0E6	364.8E6	52.949	47.402
10)	B trans-Chl...	5.355	6.070	150.0E6	387.8E6	52.370	47.267
11)	B cis-Chlor...	5.413	6.141	145.1E6	384.2E6	52.115	47.803
12)	B 4,4'-DDE	5.577	6.302	281.8E6	726.2E6	113.197	101.846
13)	MA Dieldrin	5.709	6.451	305.9E6	779.1E6	110.229	99.691
14)	MA Endrin	5.966	6.669	266.2E6	664.3E6	111.367	99.699
15)	B Endosulfa...	6.239	6.884	222.1E6	643.9E6	100.550	97.028
16)	A 4,4'-DDD	6.091	6.796	216.4E6	604.4E6	109.876	99.779
17)	MA 4,4'-DDT	6.330	7.093	228.9E6	629.6E6	111.427	104.657
18)	B Endrin al...	6.408	7.009	182.5E6	544.9E6	112.642	106.486
19)	B Endosulfa...	6.619	7.232	175.7E6	587.6E6	93.964	96.325
20)	A Methoxychlor	6.877	7.555	497.9E6	1455.0E6	528.742	489.539
21)	B Endrin ke...	7.111	7.704	210.0E6	705.8E6	106.915	99.300
22)	Toxaphene-1	5.709	6.302	305.9E6	726.2E6	18892.378	20236.161
23)	Toxaphene-2	6.091	6.669	216.4E6	664.3E6	13328.996	18190.913 #
24)	Toxaphene-3	6.239	7.093	222.1E6	629.6E6	5949.467	6467.489
25)	Toxaphene-4	6.545	7.232	1647686	587.6E6	43.505	5960.104 #
26)	Toxaphene-5	6.946	7.637	1355729	3752368	36.486	48.342 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121921\
Data File : PD067449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Dec 2021 17:42
Operator : AR\AJ
Sample : M5090-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 20 00:53:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121821CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 18 01:09:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

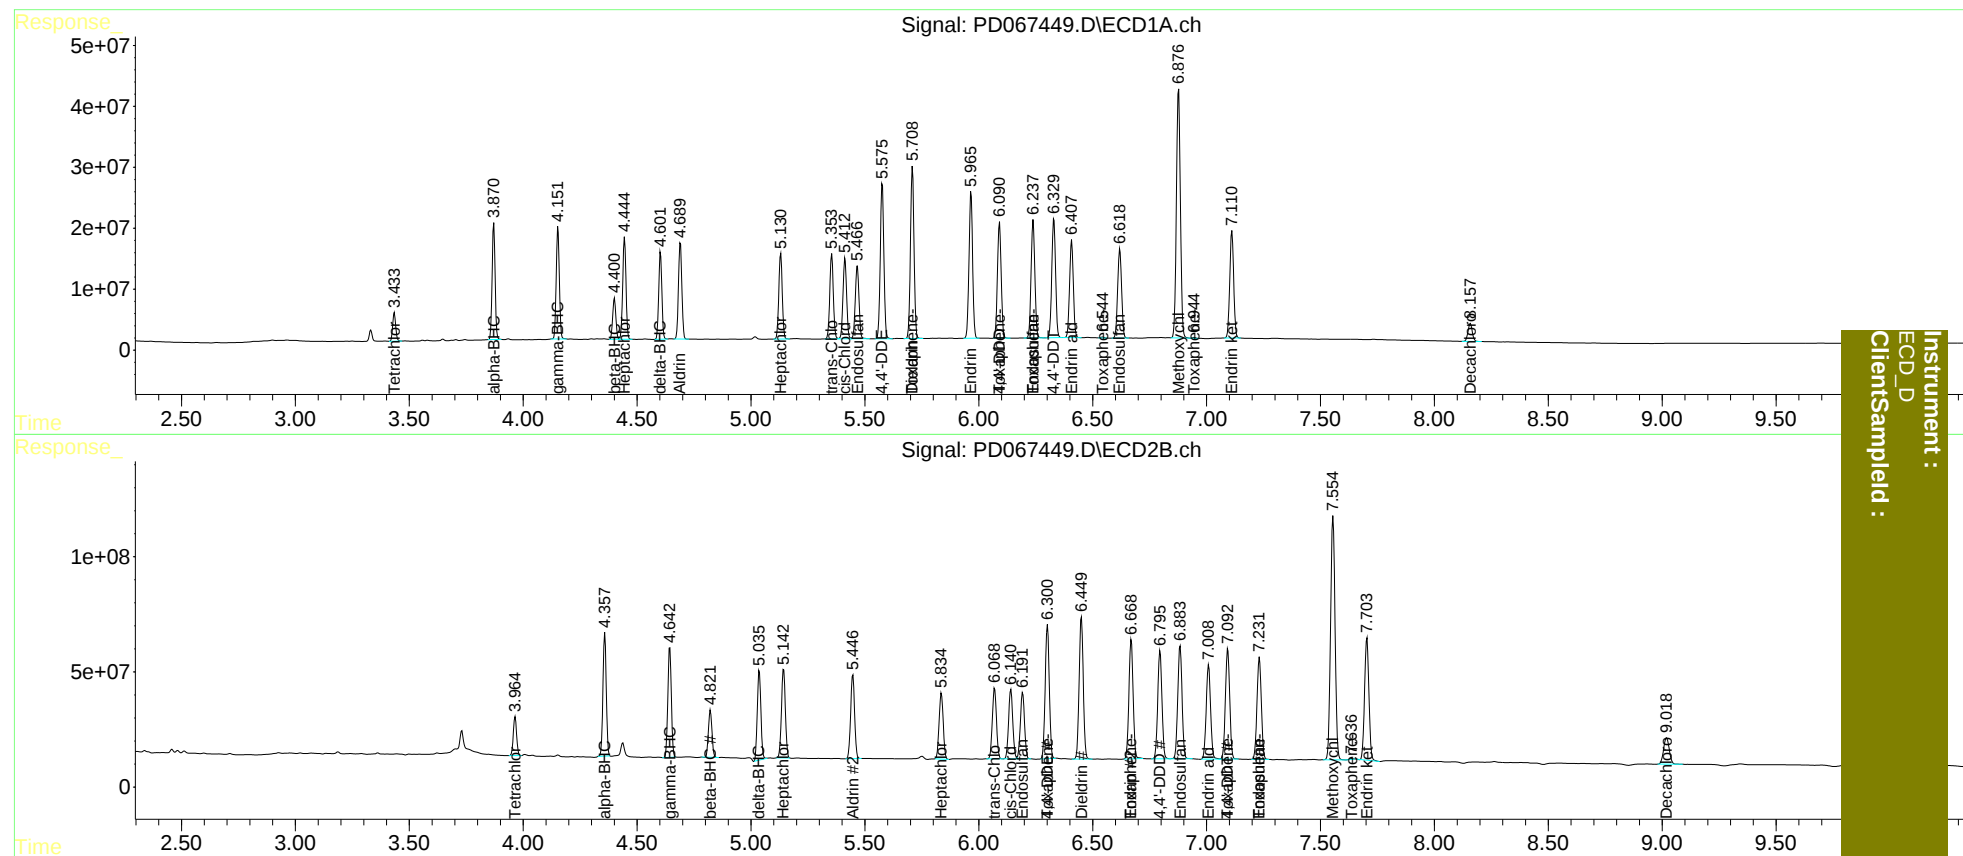

Instrument :
ECD_D
ClientSampled :